
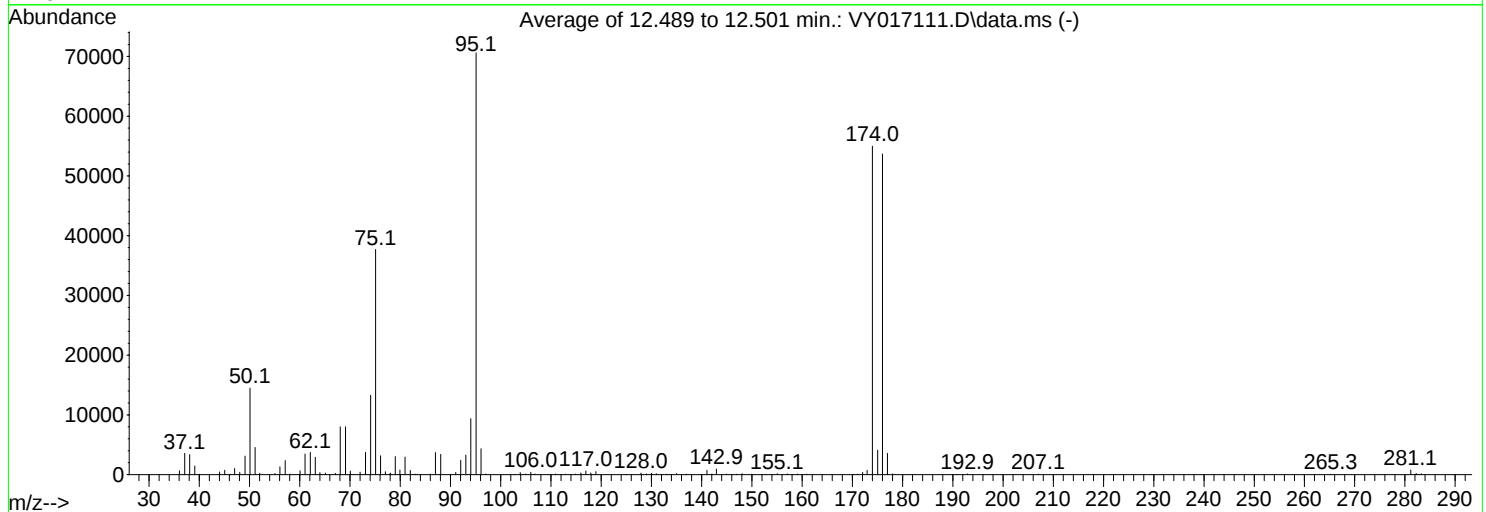


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012624\
Data File : VY017111.D
Acq On : 26 Jan 2024 08:45
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012424S.M
Title : SW846 8260
Last Update : Thu Jan 25 04:44:10 2024

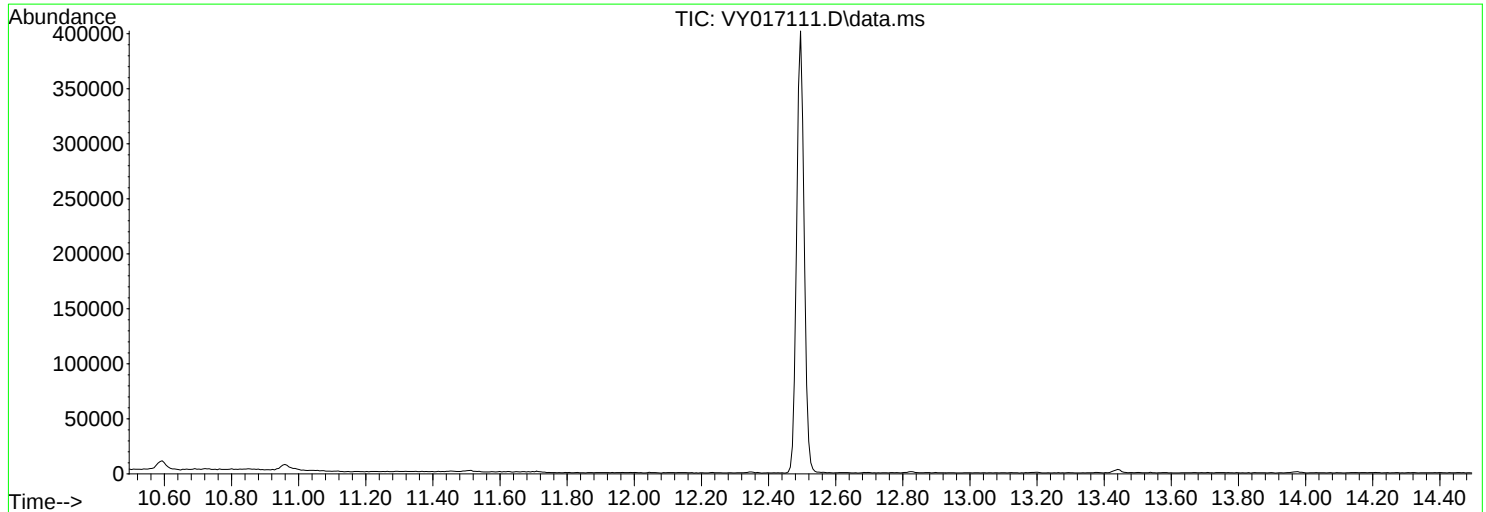

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1741

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	14503	PASS
75	95	30	60	53.4	37680	PASS
95	95	100	100	100.0	70608	PASS
96	95	5	9	6.2	4346	PASS
173	174	0.00	2	1.3	716	PASS
174	95	50	100	77.9	54979	PASS
175	174	5	9	7.5	4110	PASS
176	174	95	101	97.6	53683	PASS
177	176	5	9	6.6	3568	PASS