
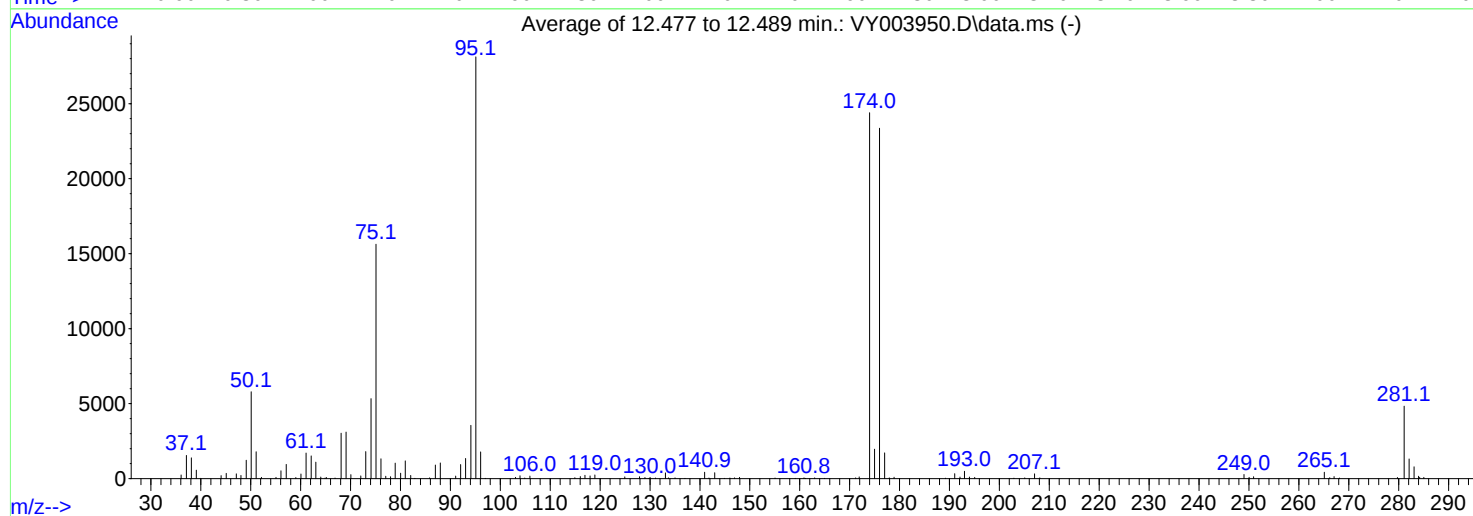


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012821\
 Data File : VY003950.D
 Acq On : 28 Jan 2021 11:03
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012821S.M
 Title : SW846 8260
 Last Update : Mon Feb 01 00:38:02 2021

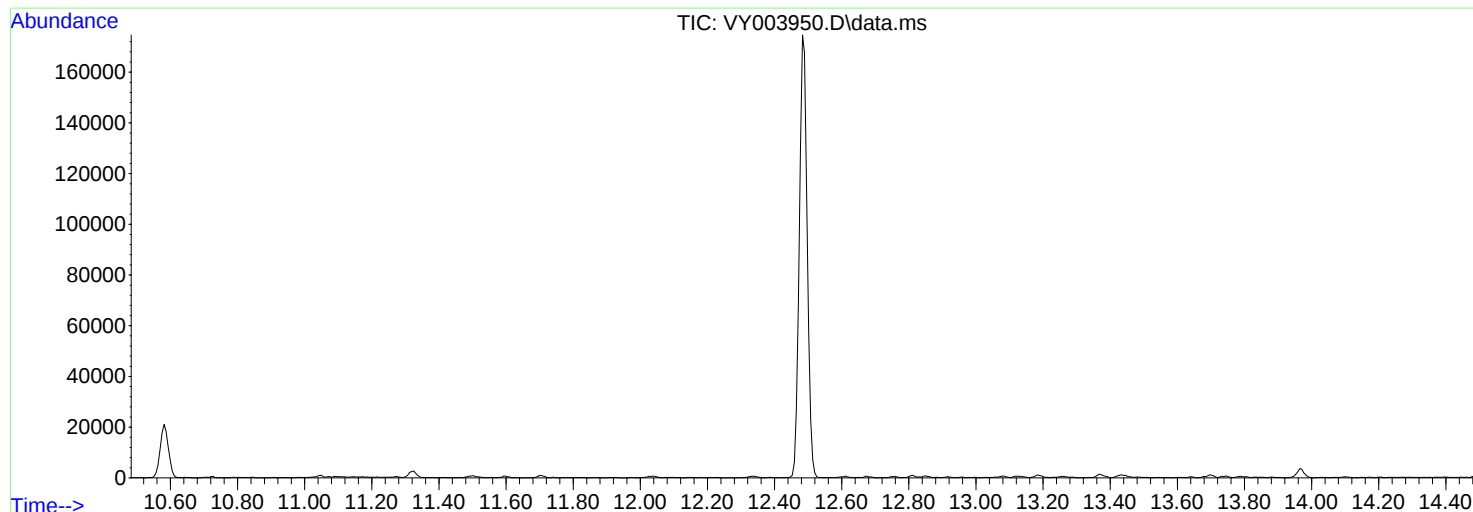

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	5792	PASS
75	95	30	60	55.6	15624	PASS
95	95	100	100	100.0	28123	PASS
96	95	5	9	6.3	1784	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.8	24400	PASS
175	174	5	9	8.0	1962	PASS
176	174	95	101	95.7	23360	PASS
177	176	5	9	7.3	1713	PASS