
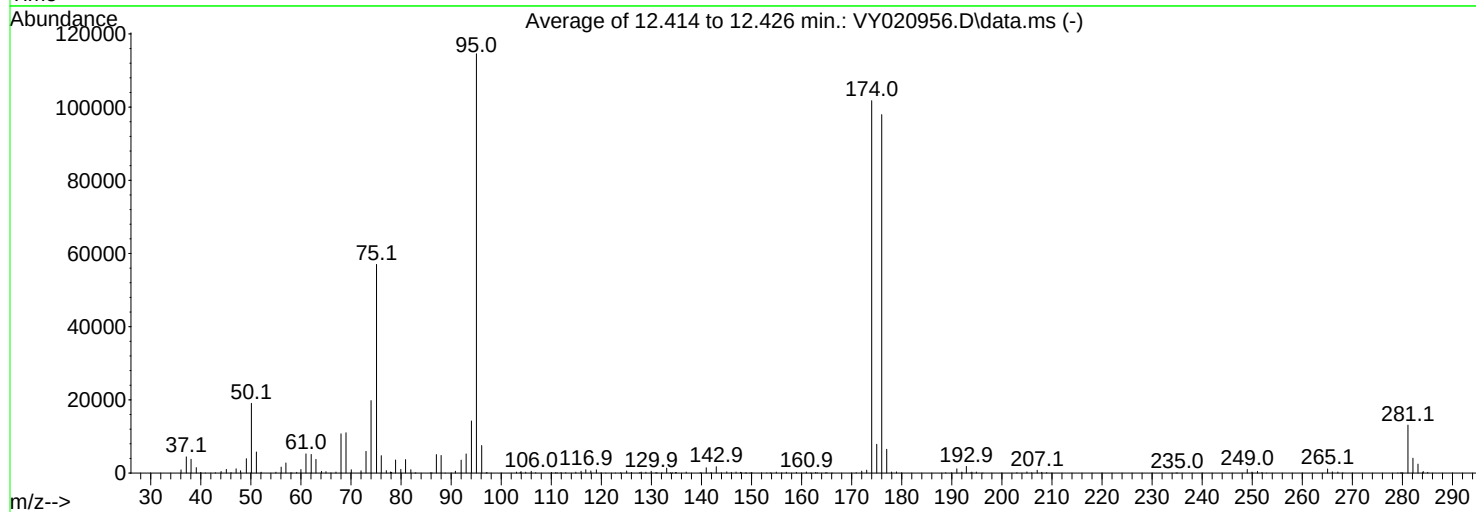


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY012925\  
Data File : VY020956.D  
Acq On : 29 Jan 2025 08:13  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y012425S.M  
Title : SW846 8260  
Last Update : Sat Jan 25 01:12:18 2025

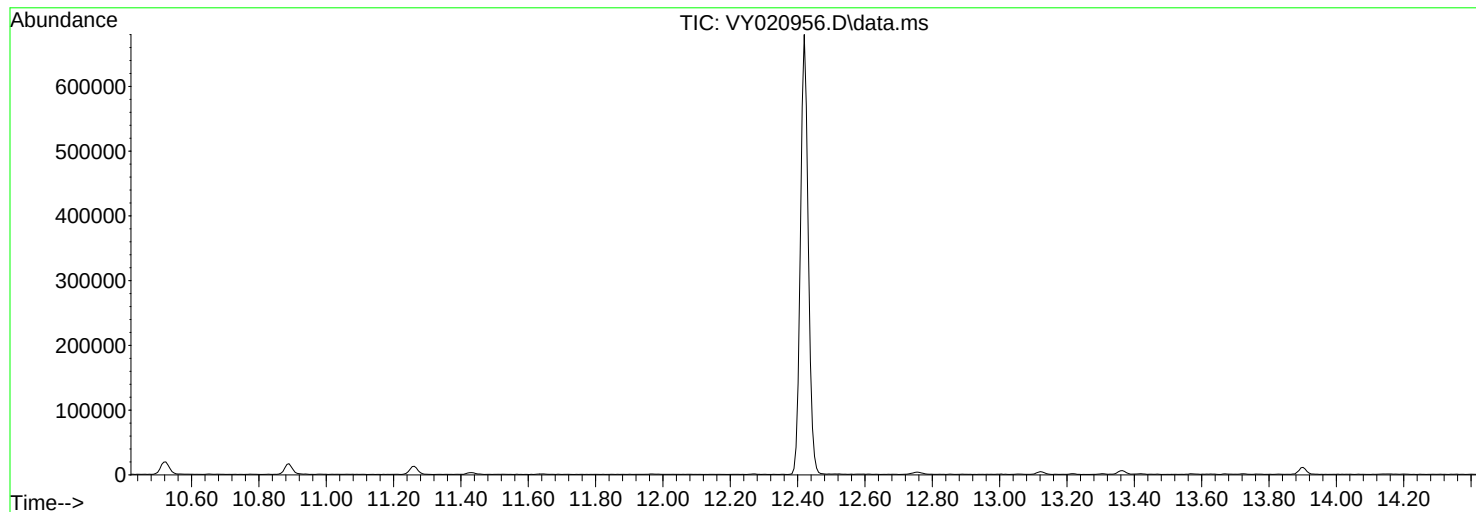

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1746

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 16.6         | 19064      | PASS                |
| 75             | 95              | 30              | 60              | 49.8         | 57021      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 114584     | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 7533       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.8          | 802        | PASS                |
| 174            | 95              | 50              | 100             | 88.8         | 101749     | PASS                |
| 175            | 174             | 5               | 9               | 7.7          | 7864       | PASS                |
| 176            | 174             | 95              | 101             | 96.3         | 97949      | PASS                |
| 177            | 176             | 5               | 9               | 6.7          | 6514       | PASS                |