
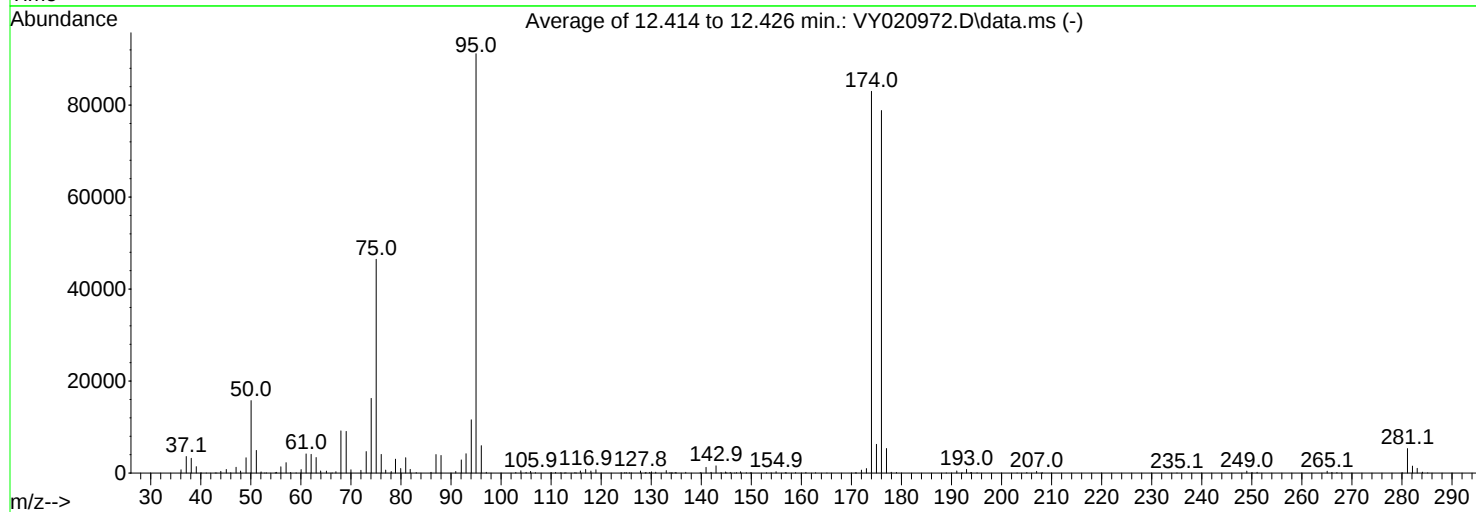


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY013025\
Data File : VY020972.D
Acq On : 30 Jan 2025 07:58
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y013025S.M
Title : SW846 8260
Last Update : Fri Jan 31 10:11:31 2025

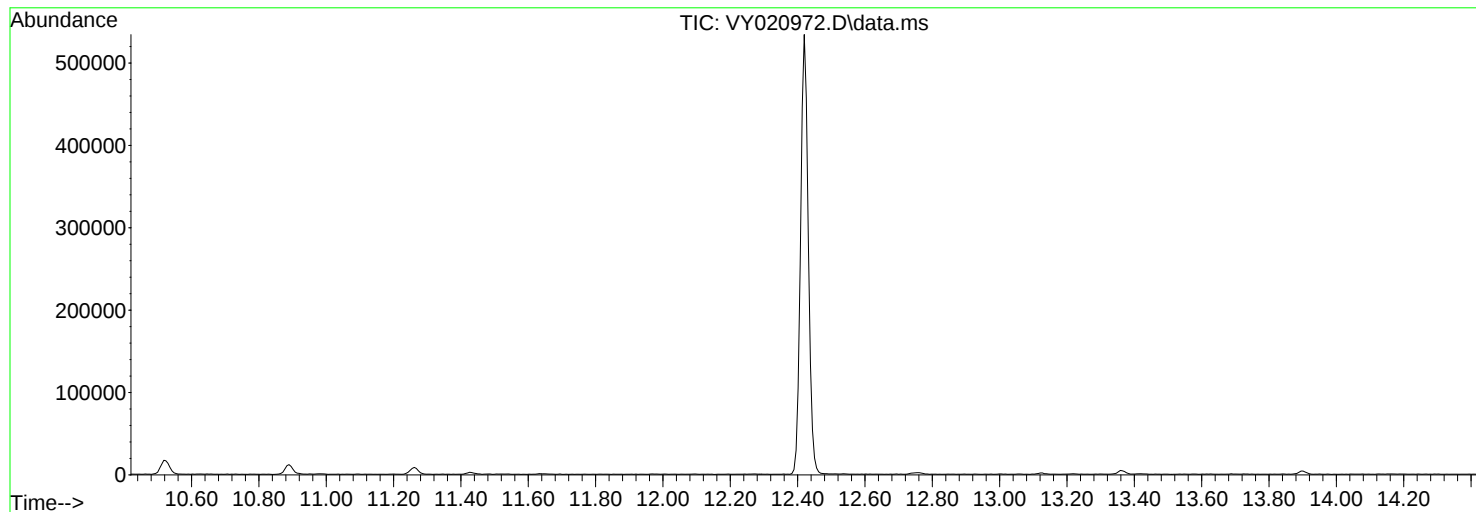

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1746

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	15763	PASS
75	95	30	60	51.0	46483	PASS
95	95	100	100	100.0	91163	PASS
96	95	5	9	6.5	5959	PASS
173	174	0.00	2	1.2	978	PASS
174	95	50	100	91.0	82989	PASS
175	174	5	9	7.5	6257	PASS
176	174	95	101	95.0	78816	PASS
177	176	5	9	6.8	5347	PASS