


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv013120\
Data File : VY001444.D
Acq On : 31 Jan 2020 09:38
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y012120S.M
Title : SW846 8260
Last Update : Thu Jan 23 01:21:47 2020

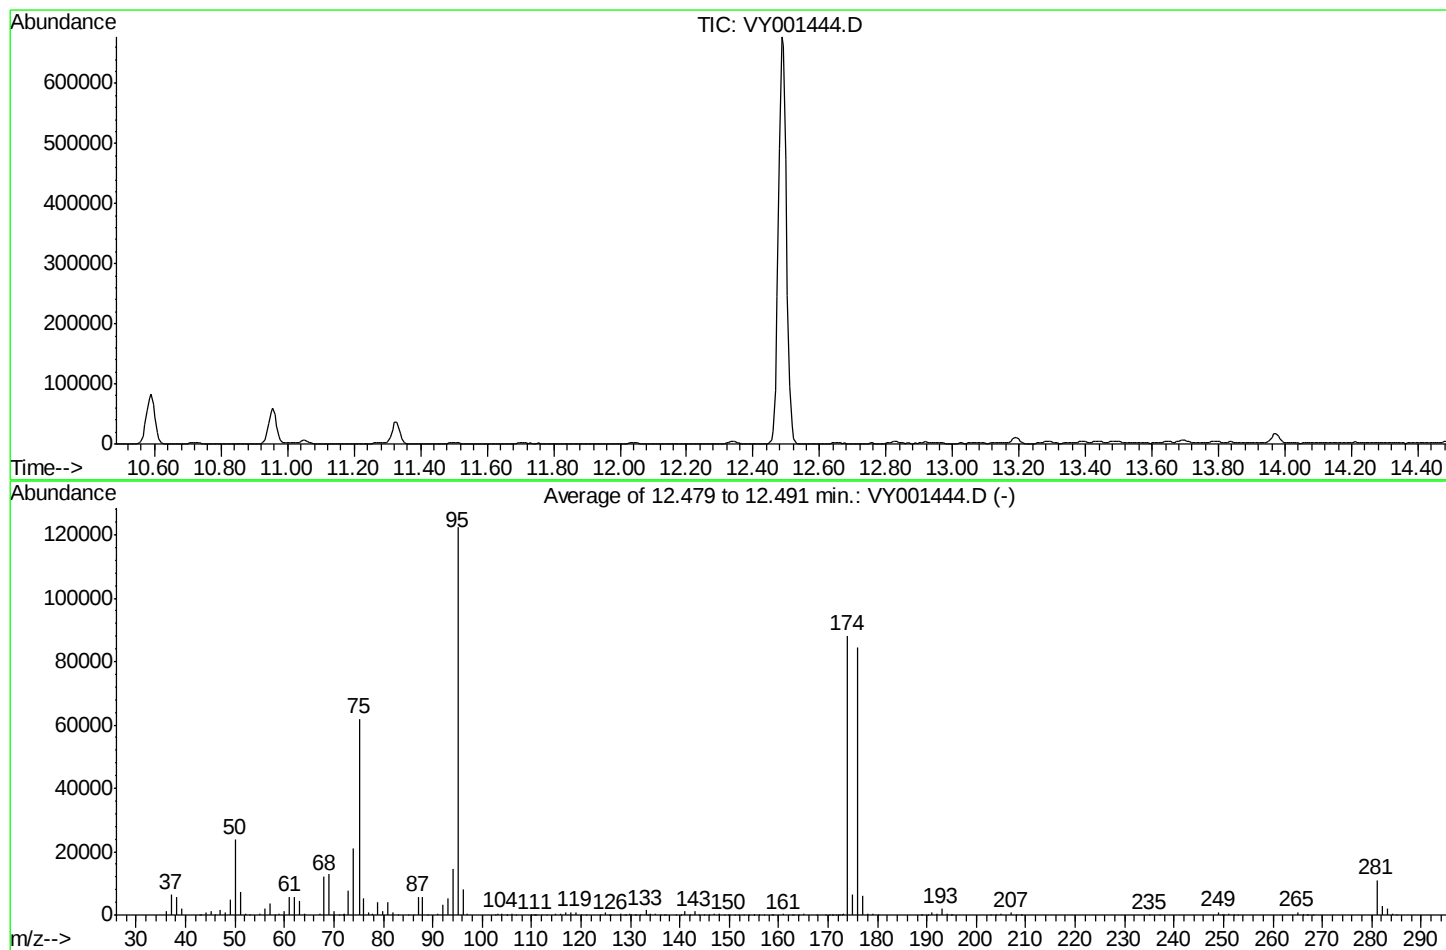

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	23709	PASS
75	95	30	60	50.7	62010	PASS
95	95	100	100	100.0	122384	PASS
96	95	5	9	6.7	8246	PASS
173	174	0.00	2	0.5	474	PASS
174	95	50	100	72.1	88282	PASS
175	174	5	9	7.4	6559	PASS
176	174	95	101	95.6	84418	PASS
177	176	5	9	7.3	6146	PASS