

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020123\
 Data File : VY012442.D
 Acq On : 01 Feb 2023 15:16
 Operator : KP/MD
 Sample : 01386-01
 Misc : 6.12g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 JPP-9-013123

Quant Time: Feb 01 23:05:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 04:31:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	185868	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	315811	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	301158	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	132467	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	110859	73.831	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	147.660%
35) Dibromofluoromethane	7.722	113	93821	56.106	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	112.220%
50) Toluene-d8	10.179	98	376314	66.368	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	132.740%
62) 4-Bromofluorobenzene	12.483	95	121517	51.549	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	103.100%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020123\
Data File : VY012442.D
Acq On : 01 Feb 2023 15:16
Operator : KP/MD
Sample : 01386-01
Misc : 6.12g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
JPP-9-013123

Quant Time: Feb 01 23:05:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 04:31:47 2023
Response via : Initial Calibration




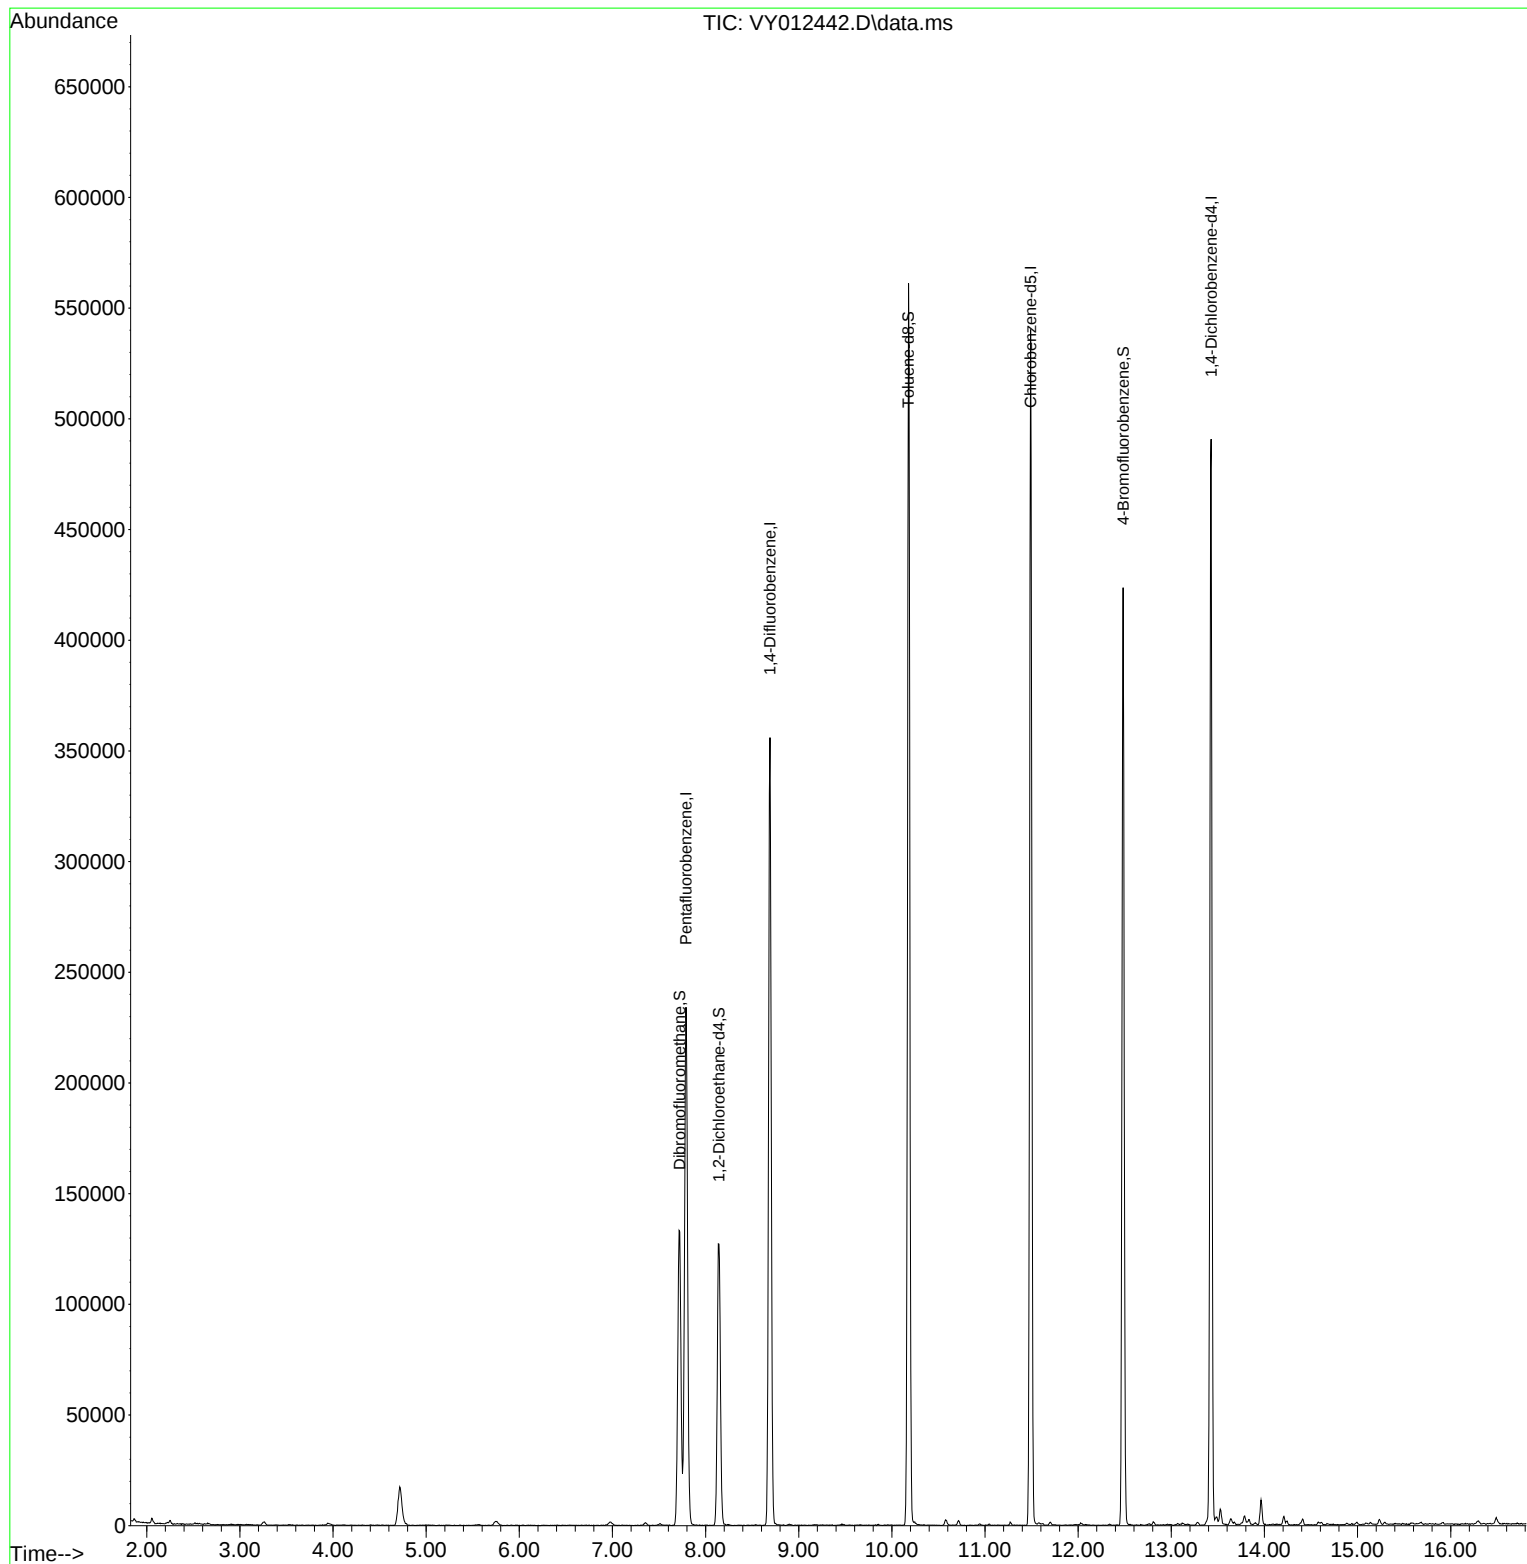




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012442.D
Acq: 01 Feb 2023 15:16




Instrument :
MSVOA_Y
ClientSampleId :
JPP-9-013123


Tgt Ion:168 Resp: 185868
Ion Ratio Lower Upper
168 100
99 53.7 44.0 66.0

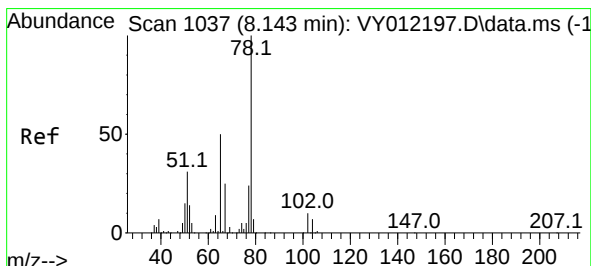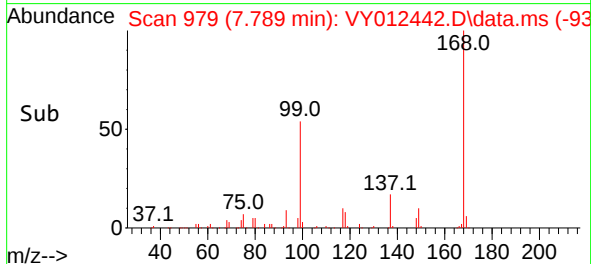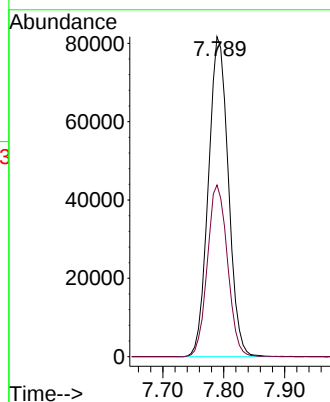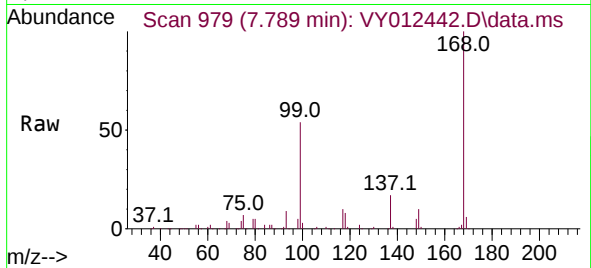

#33
1,2-Dichloroethane-d4
Concen: 73.831 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY012442.D
Acq: 01 Feb 2023 15:16

Tgt Ion: 65 Resp: 110859
Ion Ratio Lower Upper
65 100
67 49.7 0.0 103.2

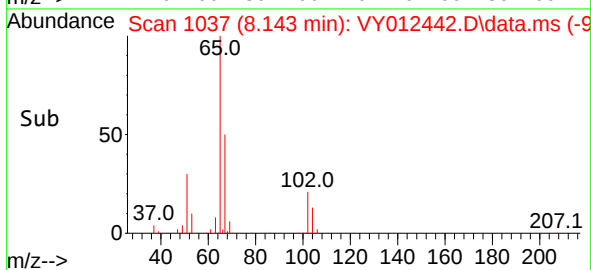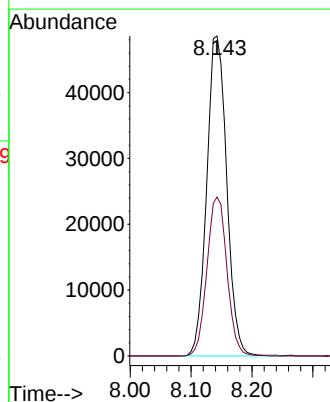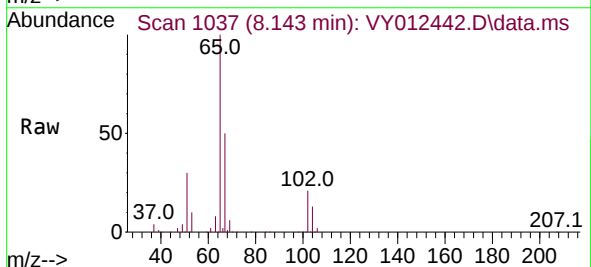

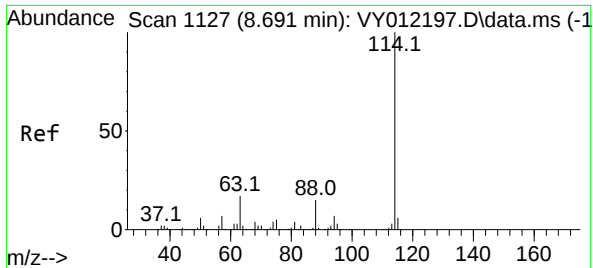

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012442.D

Acq: 01 Feb 2023 15:16

Instrument :

MSVOA_Y

ClientSampleId :

JPP-9-013123





Tgt Ion:114 Resp: 315811

Ion Ratio Lower Upper

114 100

63 18.0 0.0 39.6

88 14.6 0.0 32.2

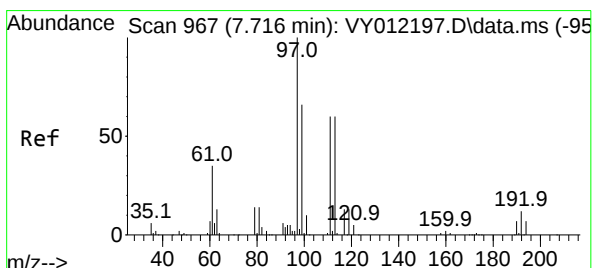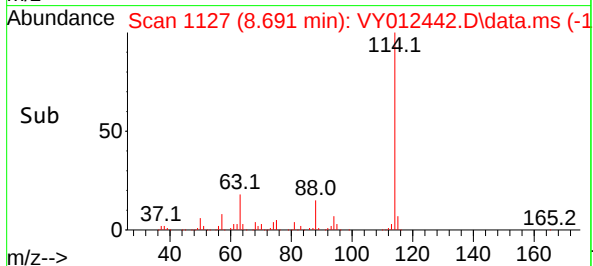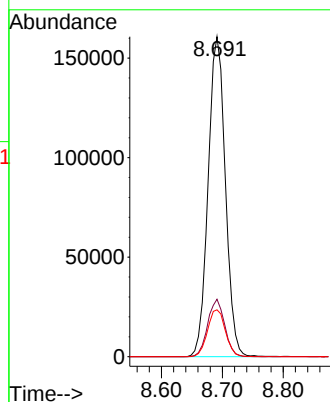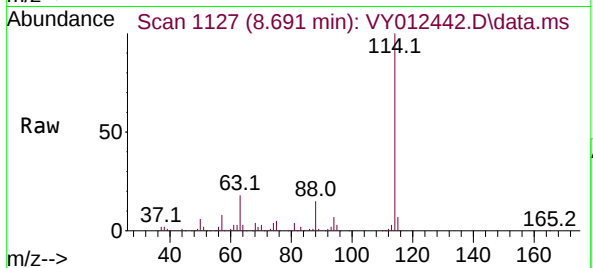

#35

Dibromofluoromethane

Concen: 56.106 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY012442.D

Acq: 01 Feb 2023 15:16




Tgt Ion:113 Resp: 93821


Ion Ratio Lower Upper

113 100

111 103.0 83.0 124.4

192 21.7 16.0 24.0

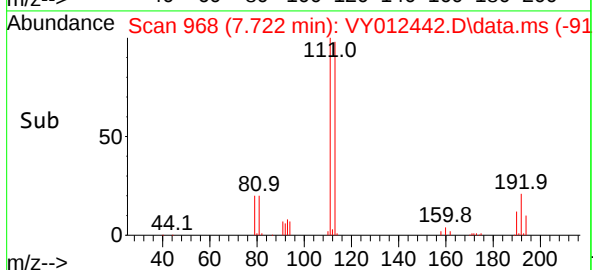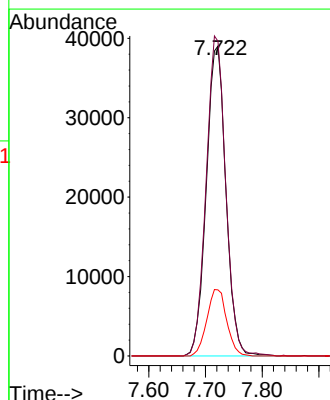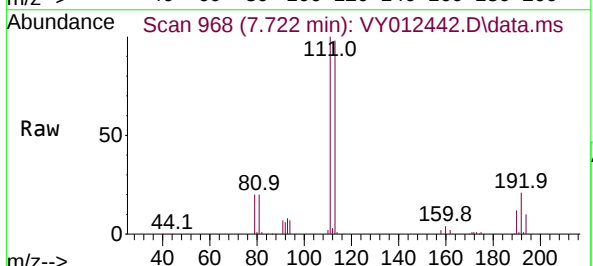

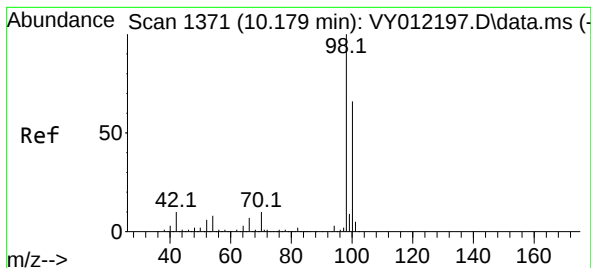

#50

Toluene-d8

Concen: 66.368 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.000 min

Lab File: VY012442.D

Acq: 01 Feb 2023 15:16

Instrument :

MSVOA_Y

ClientSampleId :





JPP-9-013123

Tgt Ion: 98 Resp: 376314

Ion Ratio Lower Upper

98 100

100 64.5 51.9 77.9

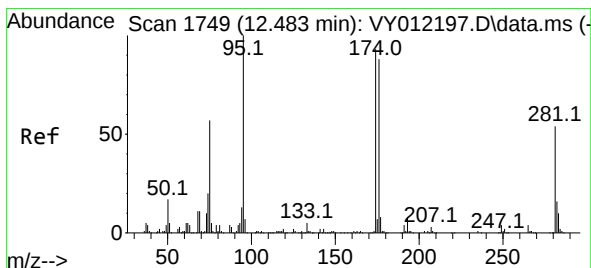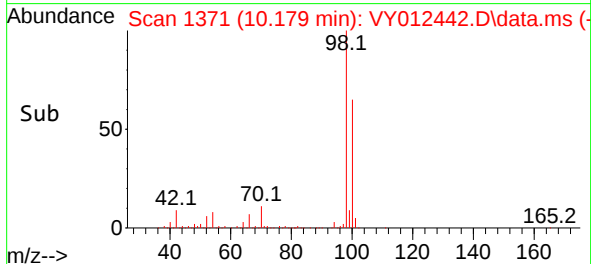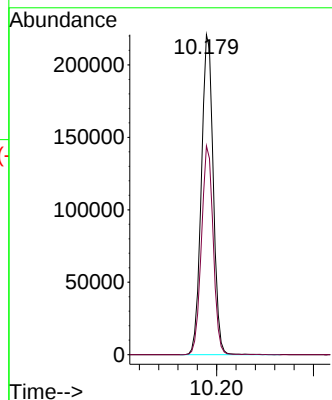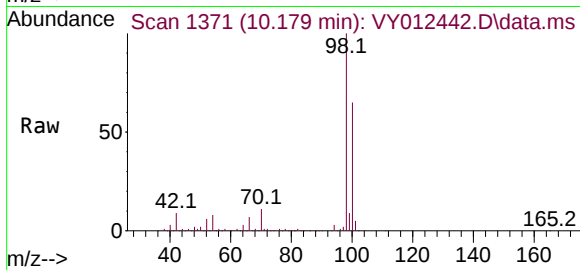

#62

4-Bromofluorobenzene

Concen: 51.549 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VY012442.D

Acq: 01 Feb 2023 15:16




Tgt Ion: 95 Resp: 121517


Ion Ratio Lower Upper

95 100

174 93.2 0.0 172.0

176 89.1 0.0 167.6

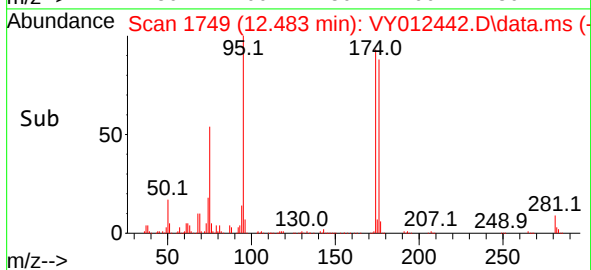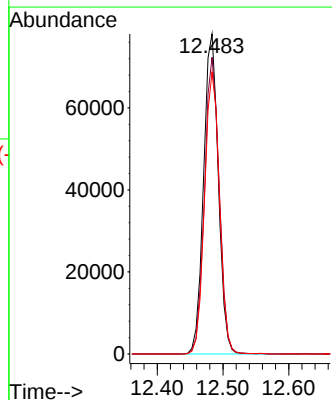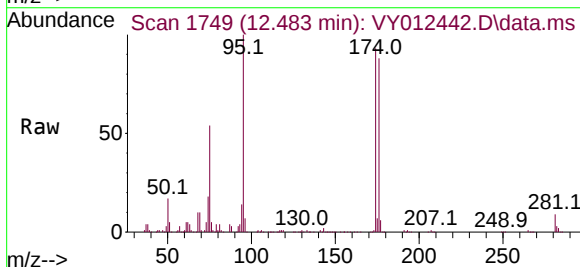

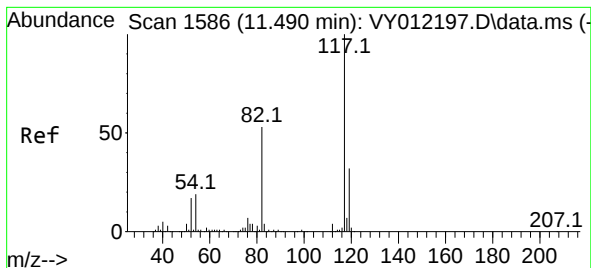

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY012442.D

Acq: 01 Feb 2023 15:16

Instrument :

MSVOA_Y

ClientSampleId :

JPP-9-013123





Tgt Ion:117 Resp: 301158

Ion Ratio Lower Upper

117 100

82 52.7 44.8 67.2

119 31.7 25.4 38.2

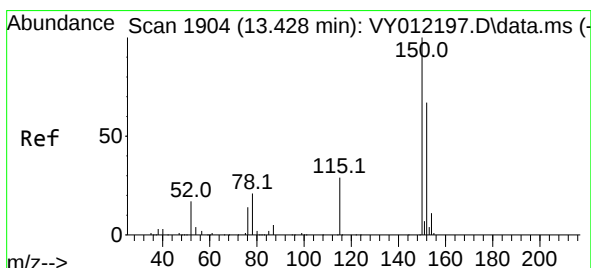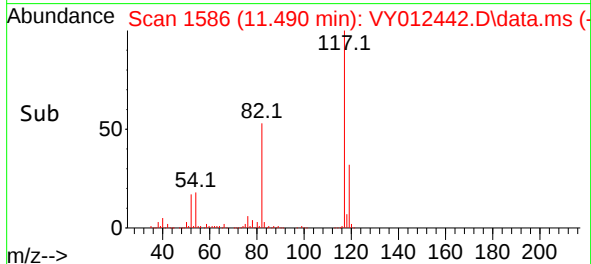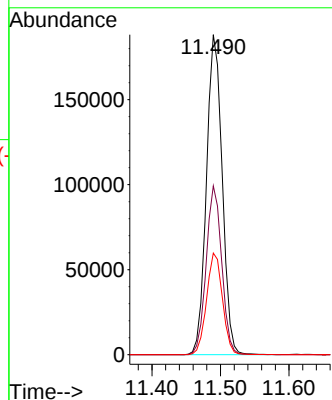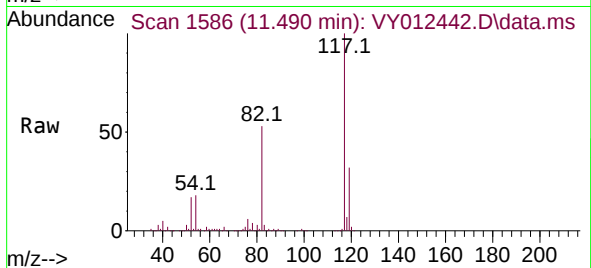

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY012442.D

Acq: 01 Feb 2023 15:16

Tgt Ion:152 Resp: 132467

Ion Ratio Lower Upper

152 100

115 57.3 29.1 87.3

150 156.5 0.0 342.6

