

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020222\
 Data File : VY007360.D
 Acq On : 02 Feb 2022 17:32
 Operator : SY/MD
 Sample : N1303-05
 Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CC-7

Quant Time: Feb 02 17:51:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y02022221S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 02 16:01:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	7.789	168	92047	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	165814	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	148499	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	61501	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	50080	47.30	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	94.60%
35) Dibromofluoromethane	7.722	113	33120	31.11	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	62.22%
50) Toluene-d8	10.179	98	200451	50.96	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	101.92%
62) 4-Bromofluorobenzene	12.477	95	78649	58.82	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	117.64%
Target Compounds						
					Qvalue	
3) Chloromethane	2.113	50	856	Below Cal	#	83
11) Tert butyl alcohol	4.954	59	48	Below Cal	#	77
16) Acetone	3.942	43	8089	23.52	ug/l	# 77
20) Methylene Chloride	4.723	84	1283	Below Cal	#	79
25) 2-Butanone	6.984	43	1342	3.23	ug/l	# 69
29) Tetrahydrofuran	7.356	42	321	1.34	ug/l	# 49
31) Cyclohexane	7.795	56	2116	1.02	ug/l	# 10
36) 1,1-Dichloropropene	7.789	75	7904	4.25	ug/l	# 51
37) Ethyl Acetate	6.984	43	1342	1.45	ug/l	# 72
38) Carbon Tetrachloride	7.789	117	9910	5.07	ug/l	# 17
51) 4-Methyl-2-Pentanone	10.063	43	1125	1.28	ug/l	89
52) Toluene	10.246	92	3712	1.19	ug/l	93
55) 1,1,2-Trichloroethane	10.618	97	1430	1.50	ug/l	# 15
59) 2-Hexanone	10.801	43	8892	13.90	ug/l	# 34
67) Ethyl Benzene	11.593	91	820590	130.90	ug/l	99
68) m/p-Xylenes	11.697	106	1688595	727.29	ug/l	99
69) o-Xylene	12.026	106	646390	294.46	ug/l	99
70) Styrene	12.026	104	37710	10.42	ug/l	# 1
73) Isopropylbenzene	12.325	105	261545	46.53	ug/l	98
74) N-amyl acetate	12.124	43	152989	109.96	ug/l	# 66
75) 1,1,2,2-Tetrachloroethane	12.556	83	15539	15.14	ug/l	# 68
76) 1,2,3-Trichloropropane	12.672	75	5862	7.91	ug/l	# 100
78) n-propylbenzene	12.666	91	924516	135.80	ug/l	100
79) 2-Chlorotoluene	12.733	91	402221	106.71	ug/l	# 41
80) 1,3,5-Trimethylbenzene	12.813	105	1873771	408.65	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.325	75	3279	8.98	ug/l	# 45
82) 4-Chlorotoluene	12.813	91	219815	56.78	ug/l	# 44
83) tert-Butylbenzene	13.117	119	704246	176.43	ug/l	# 62
84) 1,2,4-Trimethylbenzene	13.117	105	5831172	1291.61	ug/l	99
85) sec-Butylbenzene	13.117	105	5831172	973.93	ug/l	# 56
86) p-Isopropyltoluene	13.367	119	252253	51.72	ug/l	98
89) n-Butylbenzene	13.697	91	159292	33.93	ug/l	# 70
90) Hexachloroethane	13.971	117	66622	72.28	ug/l	# 6
92) 1,2-Dibromo-3-Chloropr...	14.331	75	2809	16.84	ug/l	# 6
95) Naphthalene	15.233	128	870933	350.24	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020222\
Data File : VY007360.D
Acq On : 02 Feb 2022 17:32
Operator : SY/MD
Sample : N1303-05
Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CC-7

Quant Time: Feb 02 17:51:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y0202221S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 02 16:01:48 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020222\
Data File : VY007360.D
Acq On : 02 Feb 2022 17:32
Operator : SY/MD
Sample : N1303-05
Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CC-7

Quant Time: Feb 02 17:51:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y0202221S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 02 16:01:48 2022
Response via : Initial Calibration




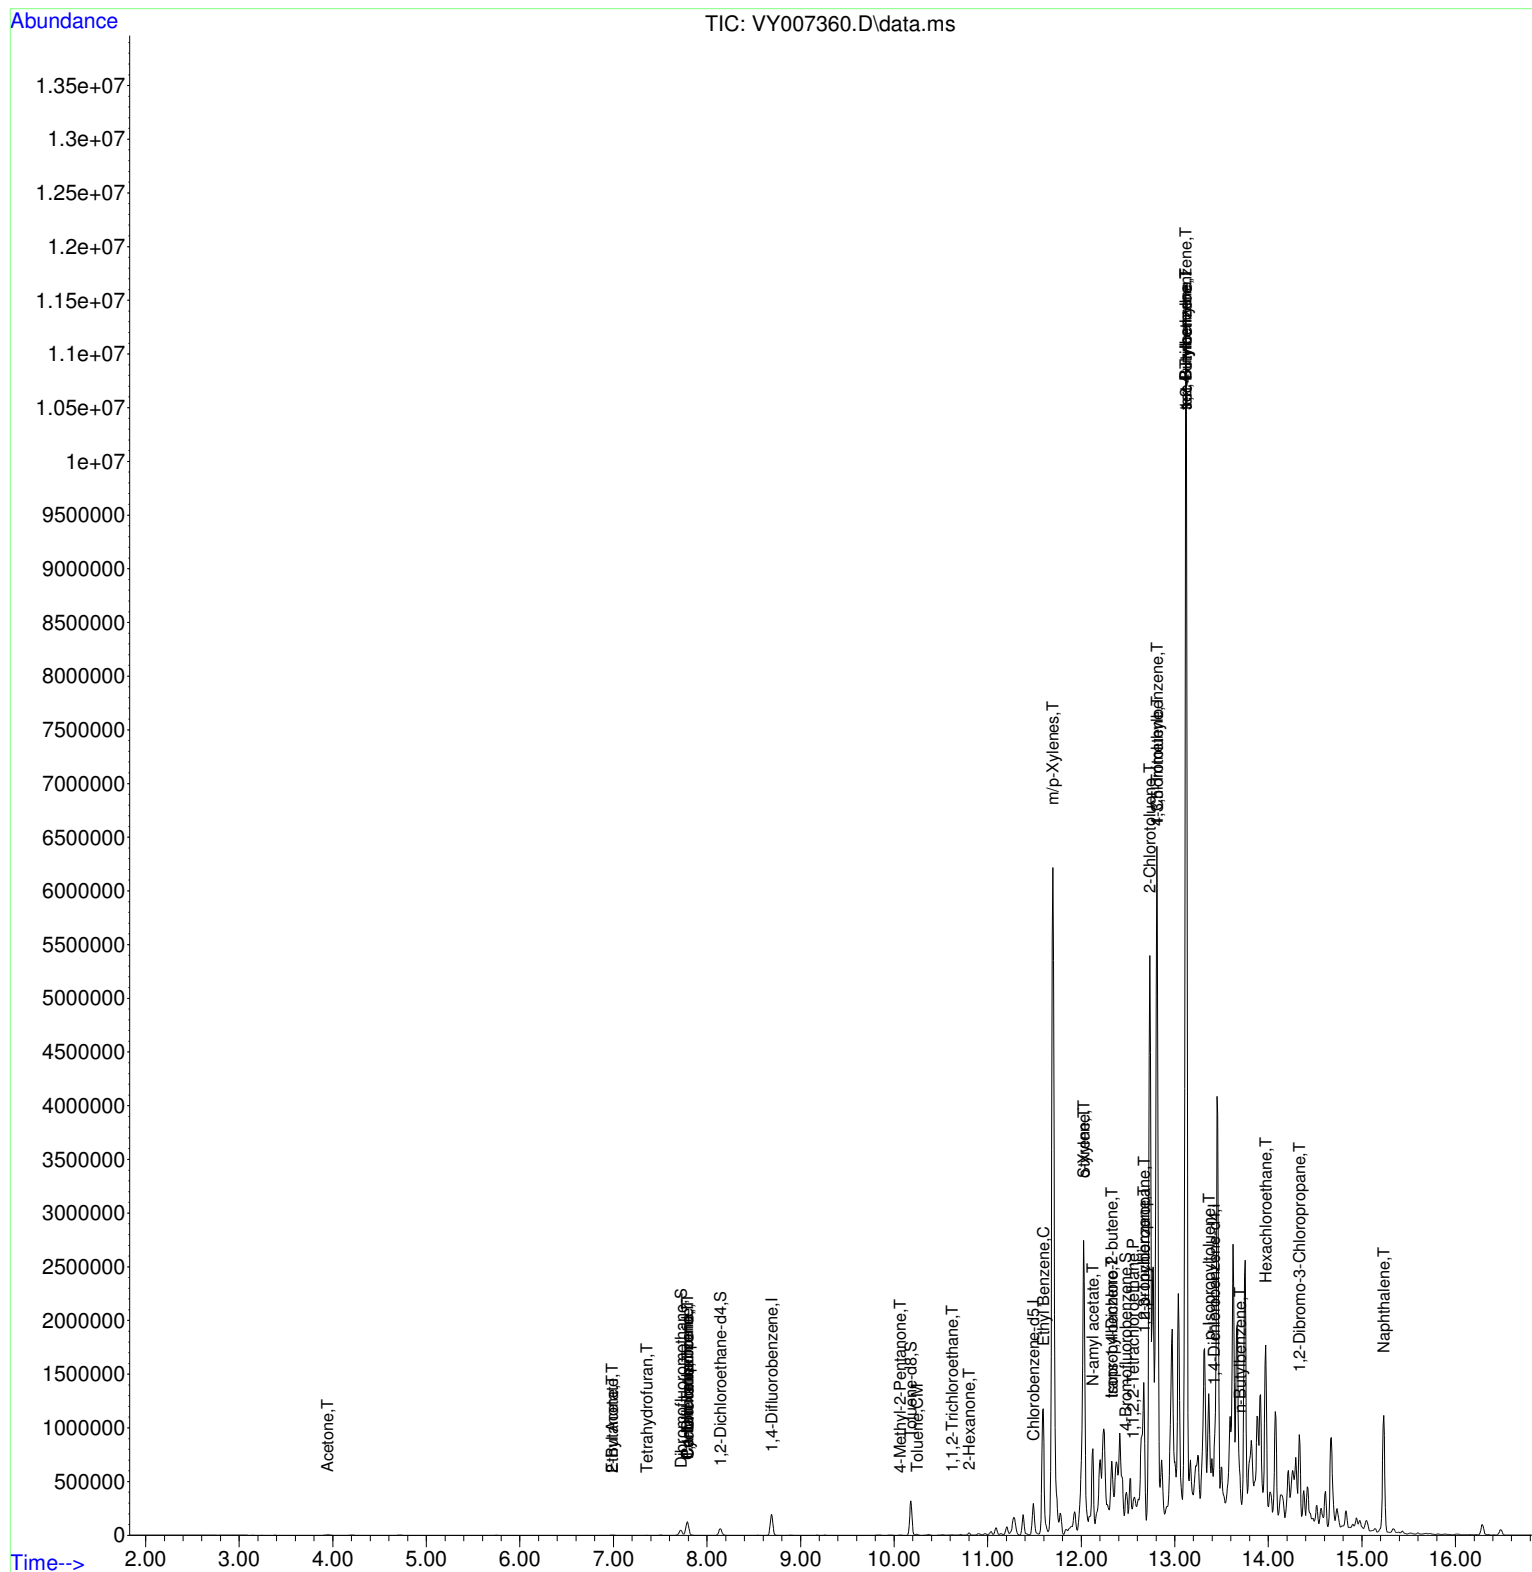




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.789 min Scan# 9
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion:168 Resp: 92047
Ion Ratio Lower Upper
168 100
99 62.0 46.9 70.3

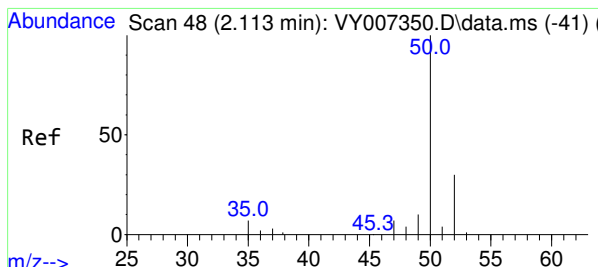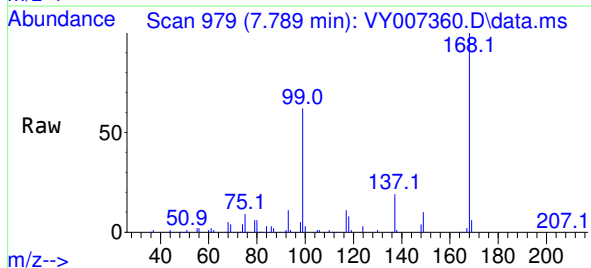

#3
Chloromethane
Concen: Below Cal
RT: 2.113 min Scan# 48
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 50 Resp: 856
Ion Ratio Lower Upper
50 100
52 40.0 24.6 37.0#


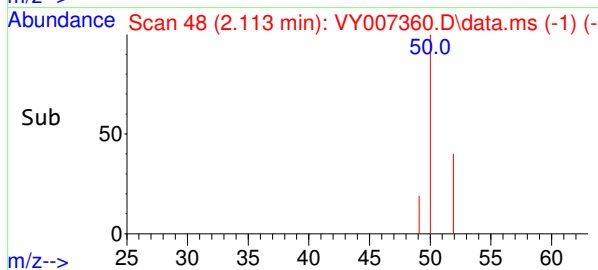

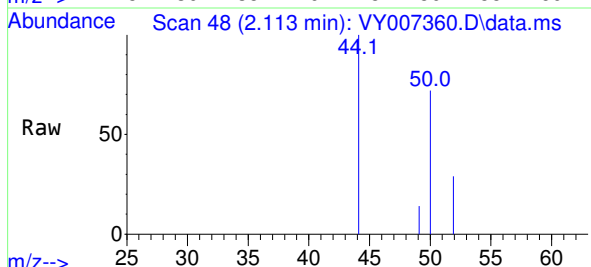




#11
Tert butyl alcohol
Concen: Below Cal
RT: 4.954 min Scan# 513
Delta R.T. 0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 59 Resp: 48
Ion Ratio Lower Upper
59 100
57 0.0 6.4 9.6#

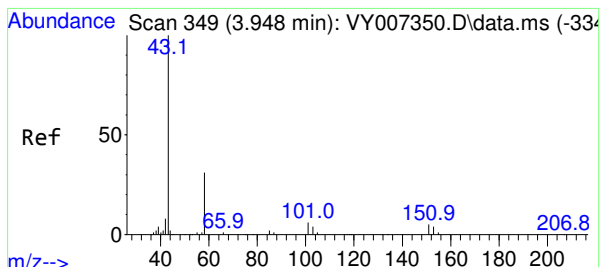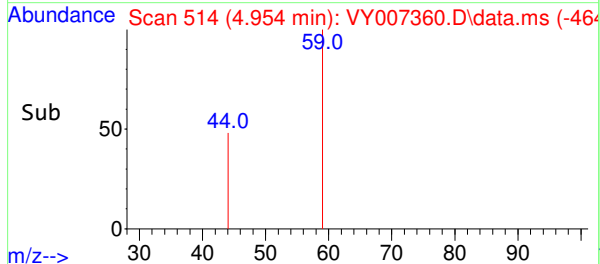

#16
Acetone
Concen: 23.52 ug/l
RT: 3.942 min Scan# 348
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 43 Resp: 8089
Ion Ratio Lower Upper
43 100
58 39.5 22.0 33.0#

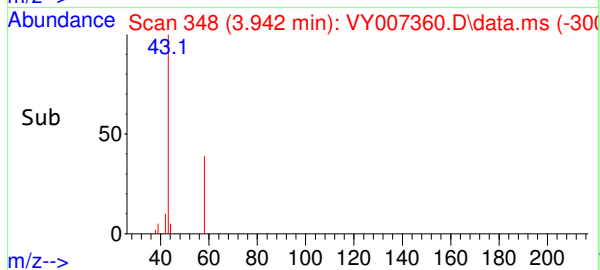




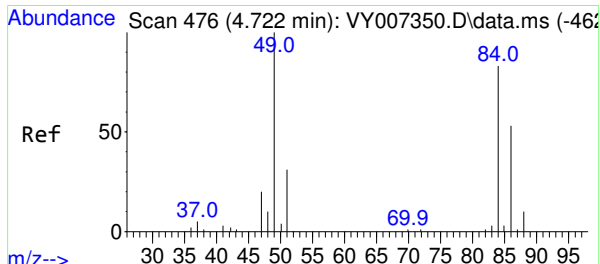


#20
Methylene Chloride
Concen: Below Cal
RT: 4.723 min Scan# 41
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Instrument :
MSVOA_Y
ClientSampleId :
CC-7

Tgt Ion: 84 Resp: 1283




Ion	Ratio	Lower	Upper
84	100		
49	109.2	114.4	171.6#
51	26.2	35.3	52.9#
86	69.7	53.7	80.5

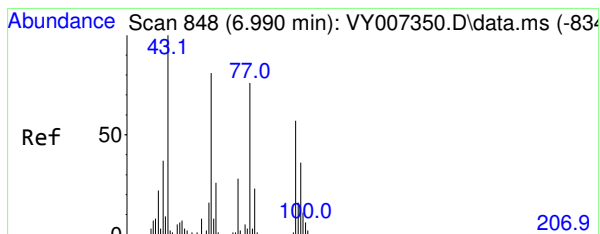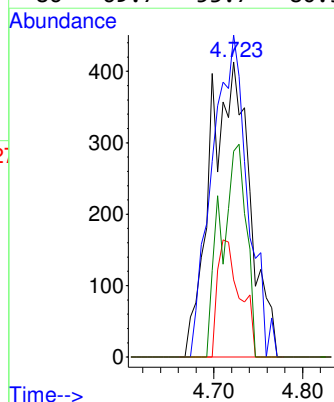


#25
2-Butanone
Concen: 3.23 ug/l
RT: 6.984 min Scan# 847
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 43 Resp: 1342

Ion	Ratio	Lower	Upper
43	100		
72	36.9	17.7	26.5#


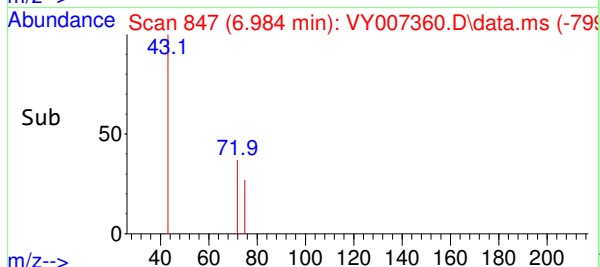
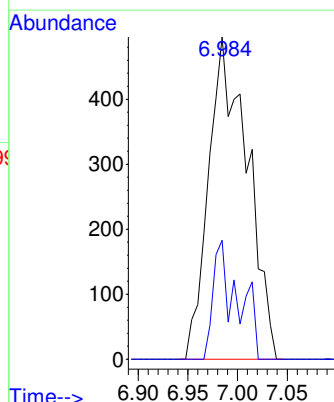
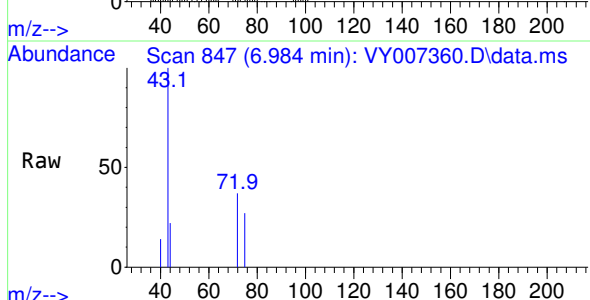




#29
Tetrahydrofuran
Concen: 1.34 ug/l
RT: 7.356 min Scan# 907
Delta R.T. 0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 42 Resp: 321
Ion Ratio Lower Upper
42 100
72 13.7 30.3 45.5#
71 0.0 29.0 43.4#

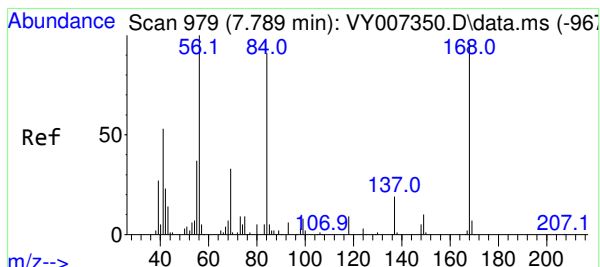

#31
Cyclohexane
Concen: 1.02 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 56 Resp: 2116
Ion Ratio Lower Upper
56 100
69 153.4 26.7 40.1#
84 121.9 67.2 100.8#


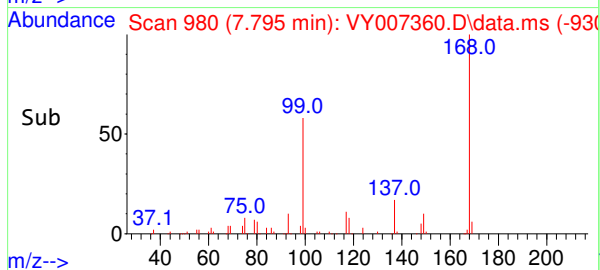






#33
1,2-Dichloroethane-d4
Concen: 47.30 ug/l
RT: 8.143 min Scan# 1
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 65 Resp: 50080
Ion Ratio Lower Upper
65 100
67 52.7 0.0 99.4

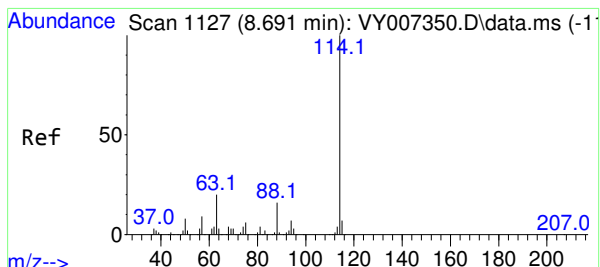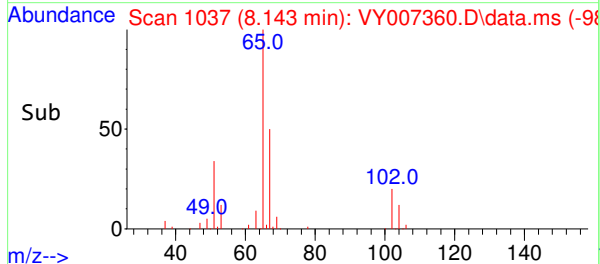

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 114 Resp: 165814
Ion Ratio Lower Upper
114 100
63 19.7 0.0 43.2
88 16.1 0.0 31.8


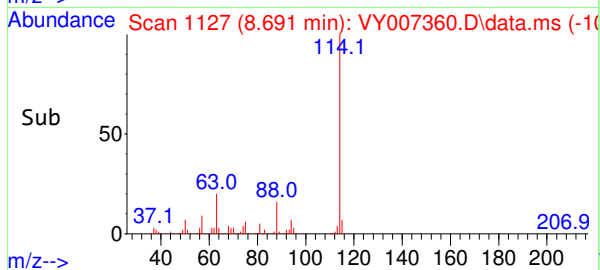




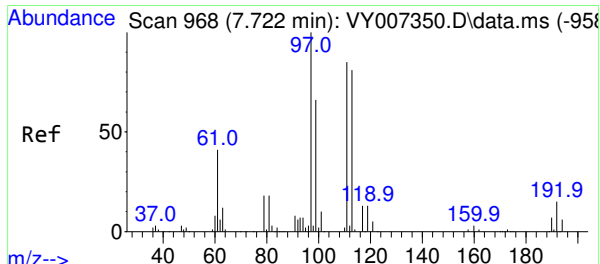

#35
Dibromofluoromethane
Concen: 31.11 ug/l
RT: 7.722 min Scan# 968
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 113 Resp: 33120
Ion Ratio Lower Upper
113 100
111 104.6 82.6 124.0
192 17.6 17.6 26.4#

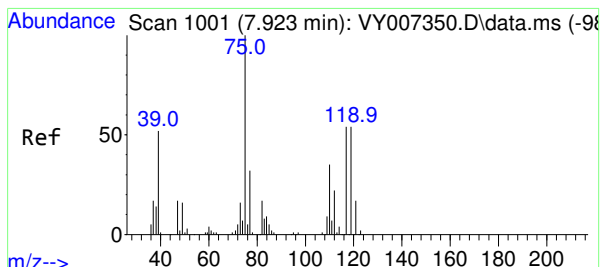

#36
1,1-Dichloropropene
Concen: 4.25 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.134 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 75 Resp: 7904
Ion Ratio Lower Upper
75 100
110 9.1 17.1 51.2#
77 0.0 24.4 36.6#


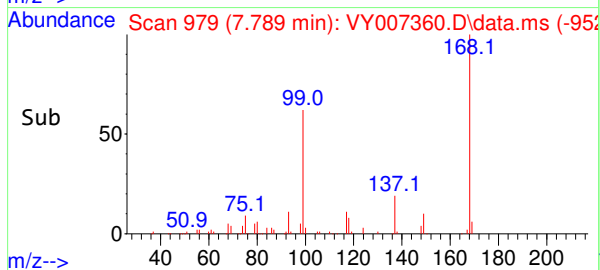




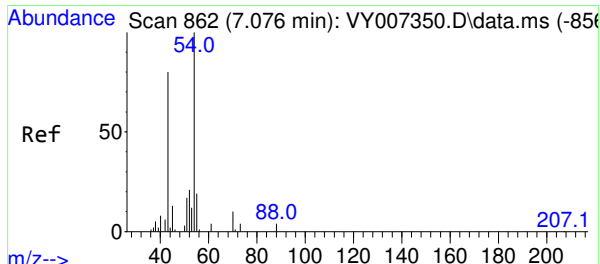

#37
Ethyl Acetate
Concen: 1.45 ug/l
RT: 6.984 min Scan# 862
Delta R.T. -0.091 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 43 Resp: 1342
Ion Ratio Lower Upper
43 100
61 0.0 9.7 14.5#
70 0.0 7.1 10.7#

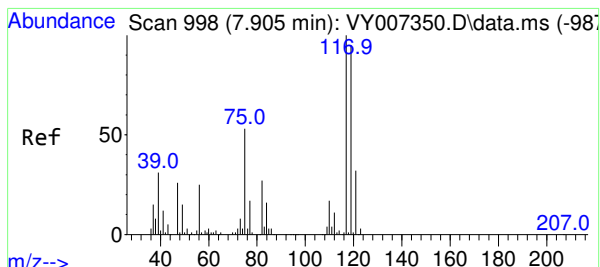

#38
Carbon Tetrachloride
Concen: 5.07 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.116 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 117 Resp: 9910
Ion Ratio Lower Upper
117 100
119 6.7 77.9 116.9#
121 0.0 24.8 37.2#


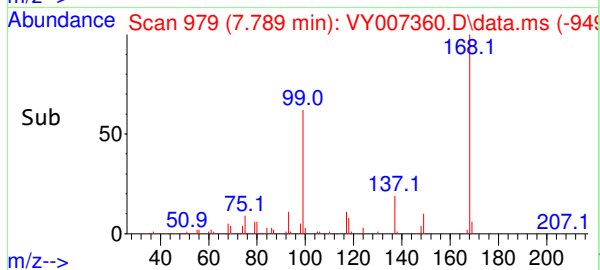




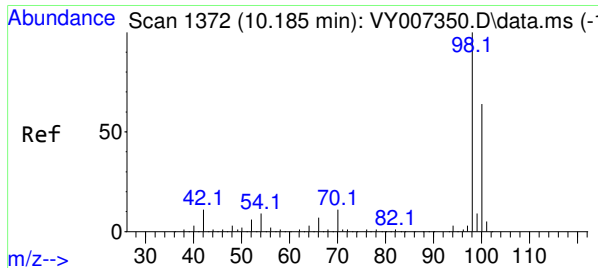

#50
Toluene-d8
Concen: 50.96 ug/l
RT: 10.179 min Scan# 1
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 98 Resp: 200451
Ion Ratio Lower Upper
98 100
100 64.5 50.2 75.2

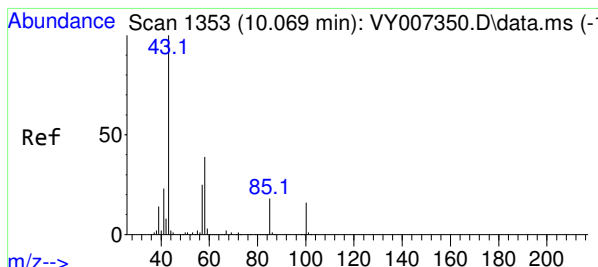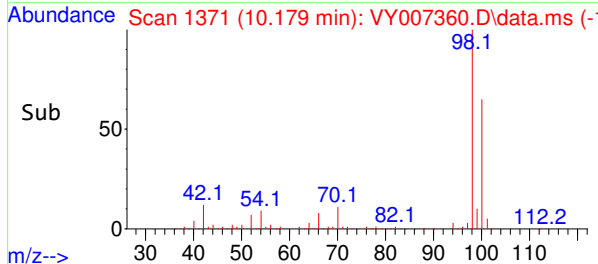

#51
4-Methyl-2-Pentanone
Concen: 1.28 ug/l
RT: 10.063 min Scan# 1352
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 43 Resp: 1125
Ion Ratio Lower Upper
43 100
58 41.8 28.1 42.1


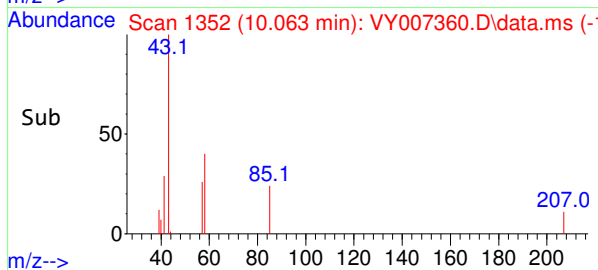




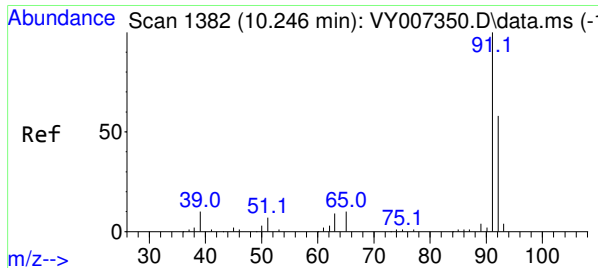

#52
Toluene
Concen: 1.19 ug/l
RT: 10.246 min Scan# 1
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 92 Resp: 3712
Ion Ratio Lower Upper
92 100
91 168.6 142.6 213.8

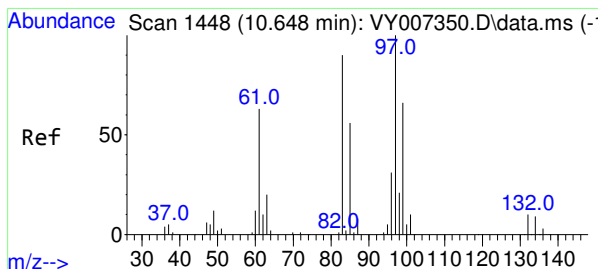

#55
1,1,2-Trichloroethane
Concen: 1.50 ug/l
RT: 10.618 min Scan# 1443
Delta R.T. -0.030 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 97 Resp: 1430
Ion Ratio Lower Upper
97 100
83 0.0 69.8 104.8#
85 0.0 44.3 66.5#
99 0.0 49.8 74.6#


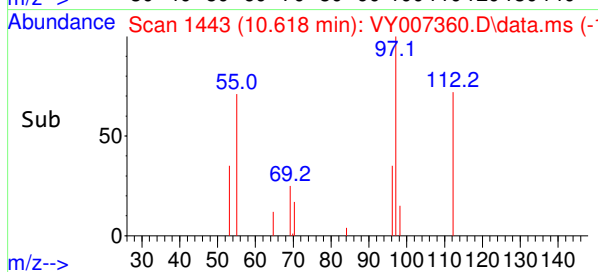






#59
2-Hexanone
Concen: 13.90 ug/l
RT: 10.801 min Scan# 1
Delta R.T. -0.030 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 43 Resp: 8892
Ion Ratio Lower Upper
43 100
58 4.2 24.4 73.4#

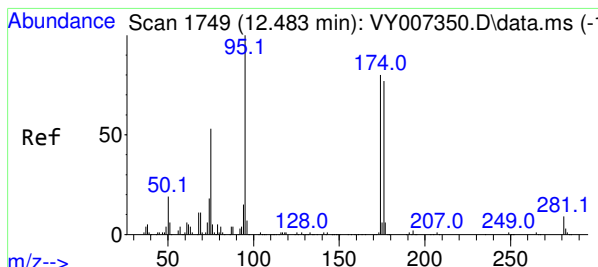

#62
4-Bromofluorobenzene
Concen: 58.82 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 95 Resp: 78649
Ion Ratio Lower Upper
95 100
174 60.9 0.0 177.0
176 58.1 0.0 175.8


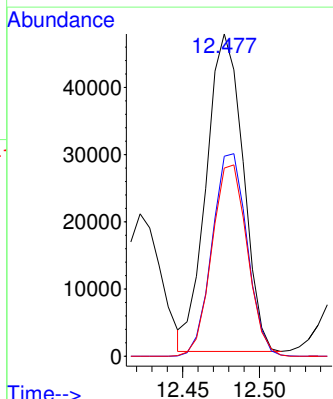
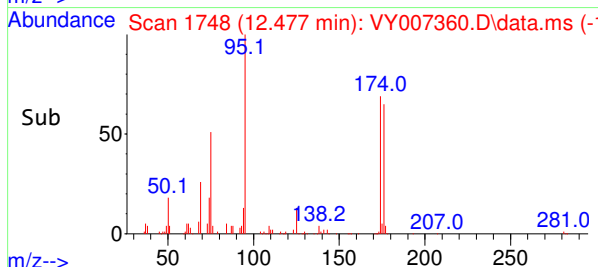





#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.490 min Scan# 1
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 117 Resp: 148499
Ion Ratio Lower Upper
117 100
82 55.9 43.0 64.4
119 32.2 25.4 38.0

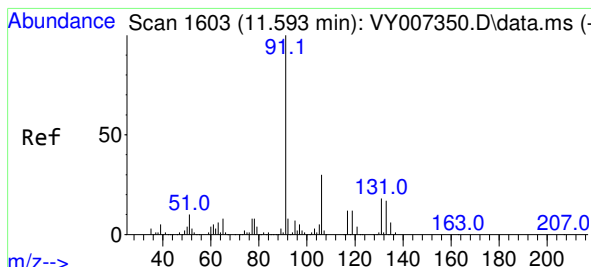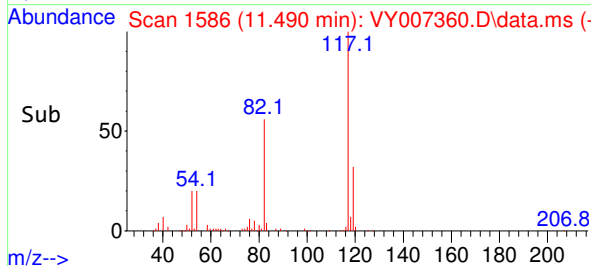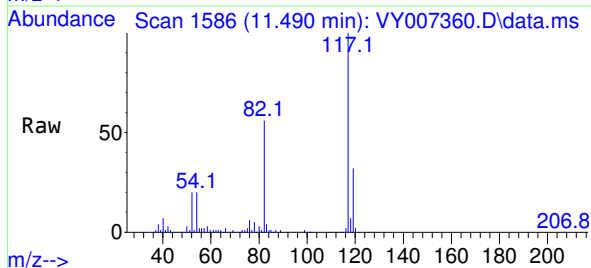

#67
Ethyl Benzene
Concen: 130.90 ug/l
RT: 11.593 min Scan# 1603
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 91 Resp: 820590
Ion Ratio Lower Upper
91 100
106 30.3 24.5 36.7


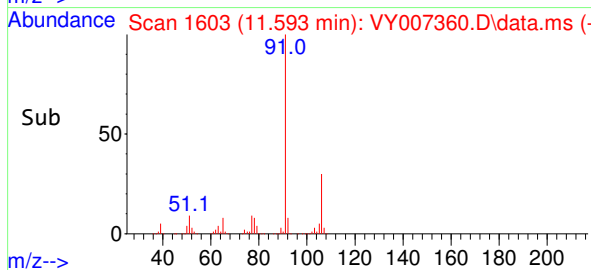

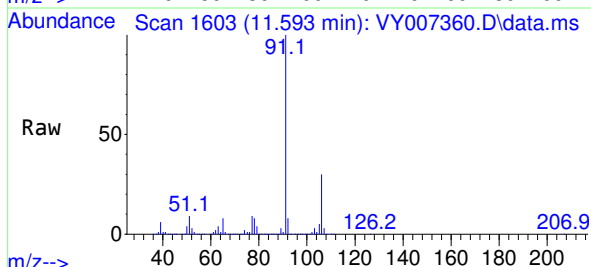




#68
m/p-Xylenes
Concen: 727.29 ug/l
RT: 11.697 min Scan# 1
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion:106 Resp: 1688595
Ion Ratio Lower Upper
106 100
91 207.1 166.6 249.8

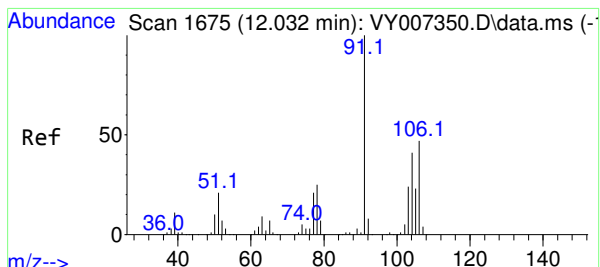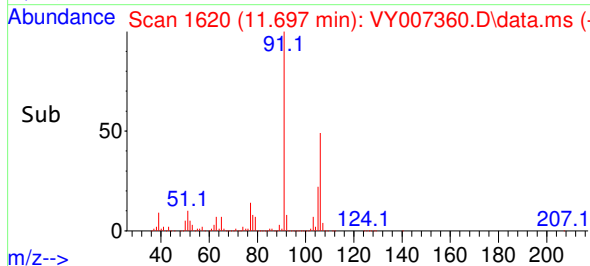

#69
o-Xylene
Concen: 294.46 ug/l
RT: 12.026 min Scan# 1674
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion:106 Resp: 646390
Ion Ratio Lower Upper
106 100
91 219.6 110.3 331.0









#70
Styrene
Concen: 10.42 ug/l
RT: 12.026 min Scan# 1
Delta R.T. -0.018 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion:104 Resp: 37710
Ion Ratio Lower Upper
104 100
78 277.9 42.4 63.6#
103 245.4 44.4 66.6#

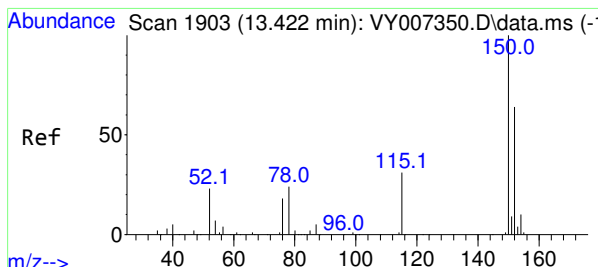

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion:152 Resp: 61501
Ion Ratio Lower Upper
152 100
115 51.9 28.2 84.7
150 143.3 0.0 347.6


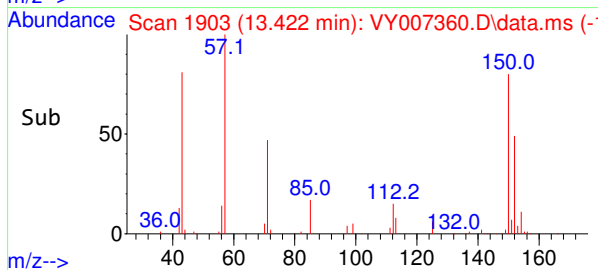






#73
Isopropylbenzene
Concen: 46.53 ug/l
RT: 12.325 min Scan# 1
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 105 Resp: 261545
Ion Ratio Lower Upper
105 100
120 25.8 13.4 40.2

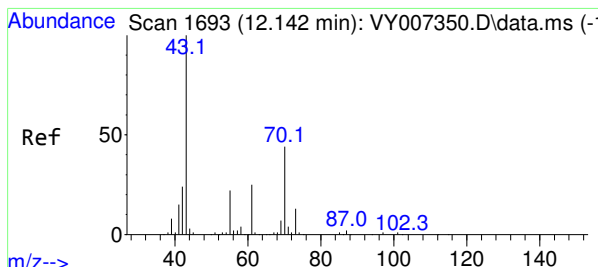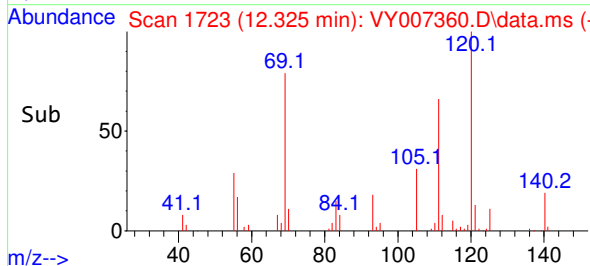

#74
N-ethyl acetate
Concen: 109.96 ug/l
RT: 12.124 min Scan# 1690
Delta R.T. -0.018 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 43 Resp: 152989
Ion Ratio Lower Upper
43 100
70 11.5 28.7 43.1#
55 16.2 17.3 25.9#
61 0.0 17.0 25.6#



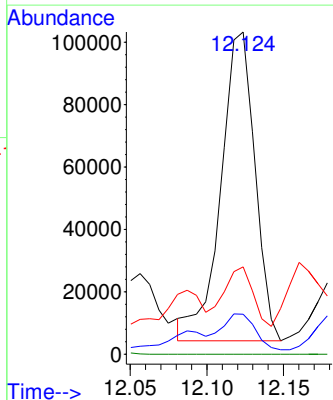





#75
1,1,2,2-Tetrachloroethane
Concen: 15.14 ug/l
RT: 12.556 min Scan# 1
Delta R.T. -0.024 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 83 Resp: 15539
Ion Ratio Lower Upper
83 100
131 0.0 5.6 16.8#
85 90.0 32.3 96.8



#76
1,2,3-Trichloropropane
Concen: 7.91 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. 0.037 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 75 Resp: 5862
Ion Ratio Lower Upper
75 100
77 682.5 0.0 0.0#







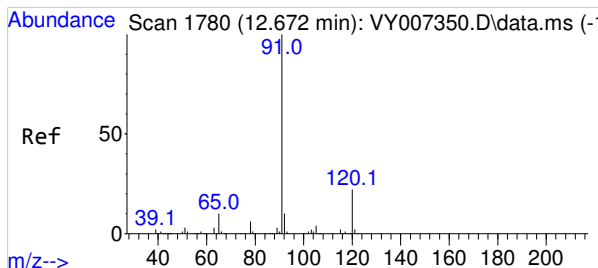

#78
n-propylbenzene
Concen: 135.80 ug/l
RT: 12.666 min Scan# 1
Delta R.T. -0.006 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 91 Resp: 924516
Ion Ratio Lower Upper
91 100
120 22.7 11.3 33.9

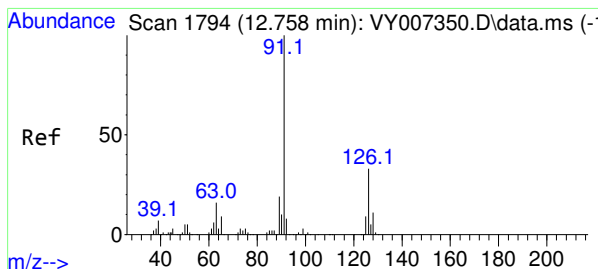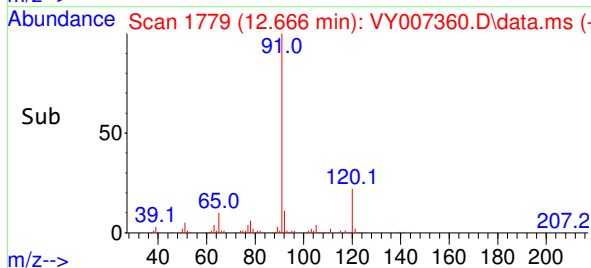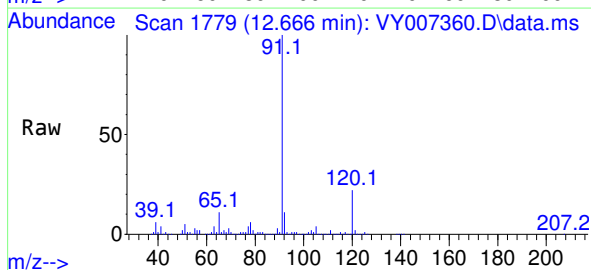

#79
2-Chlorotoluene
Concen: 106.71 ug/l
RT: 12.733 min Scan# 1790
Delta R.T. -0.024 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 91 Resp: 402221
Ion Ratio Lower Upper
91 100
126 0.1 16.9 50.6#


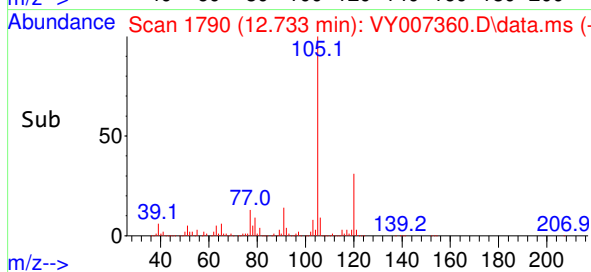

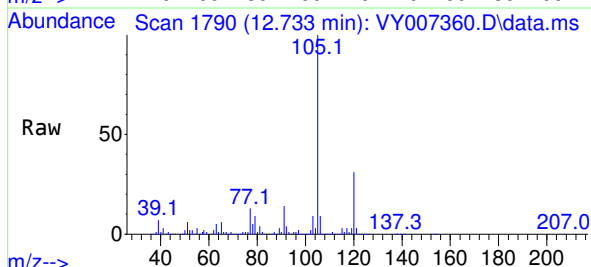




#80
1,3,5-Trimethylbenzene
Concen: 408.65 ug/l
RT: 12.813 min Scan# 1
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion:105 Resp: 1873771
Ion Ratio Lower Upper
105 100
120 47.5 24.4 73.4

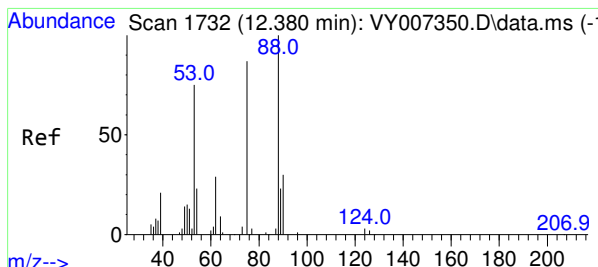

#81
trans-1,4-Dichloro-2-butene
Concen: 8.98 ug/l
RT: 12.325 min Scan# 1723
Delta R.T. -0.055 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 75 Resp: 3279
Ion Ratio Lower Upper
75 100
53 138.7 85.3 127.9#
89 119.1 37.0 55.4#


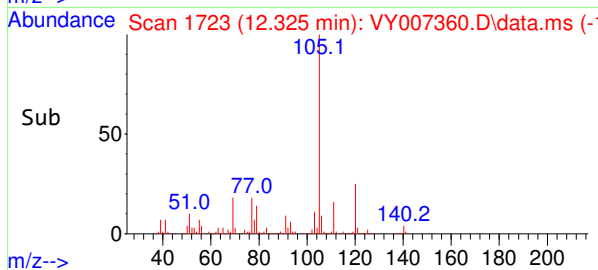




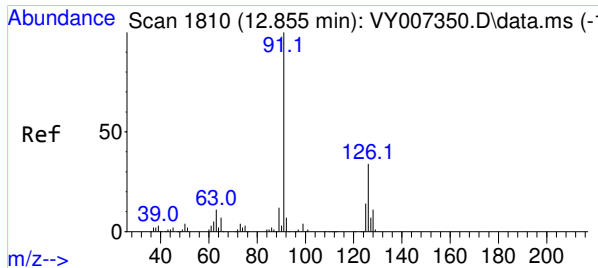

#82
4-Chlorotoluene
Concen: 56.78 ug/l
RT: 12.813 min Scan# 1
Delta R.T. -0.043 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion: 91 Resp: 219815
Ion Ratio Lower Upper
91 100
126 1.7 17.0 51.0#

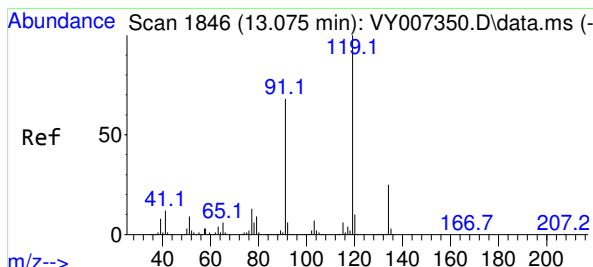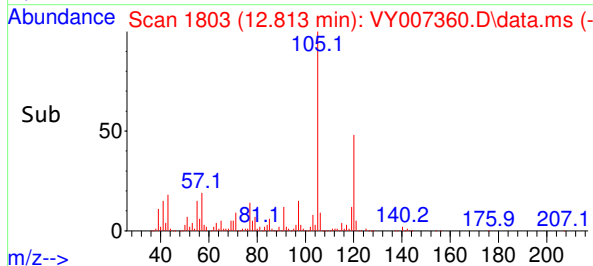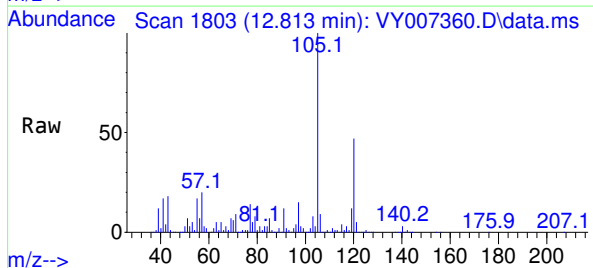

#83
tert-Butylbenzene
Concen: 176.43 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. 0.043 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 119 Resp: 704246
Ion Ratio Lower Upper
119 100
91 96.8 34.8 104.4
134 0.0 13.3 39.9#


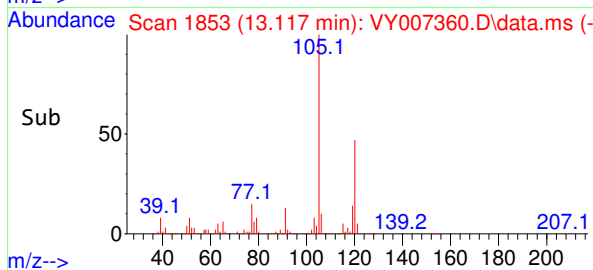

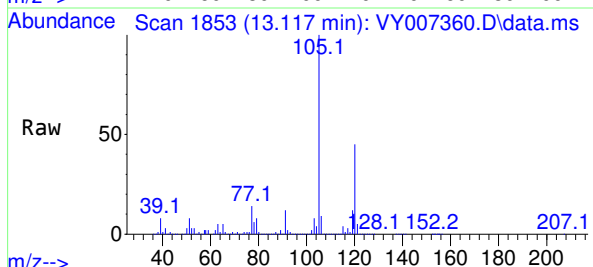




#84
1,2,4-Trimethylbenzene
Concen: 1291.61 ug/l
RT: 13.117 min Scan# 1
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion:105 Resp: 5831172
Ion Ratio Lower Upper
105 100
120 44.9 22.3 66.9

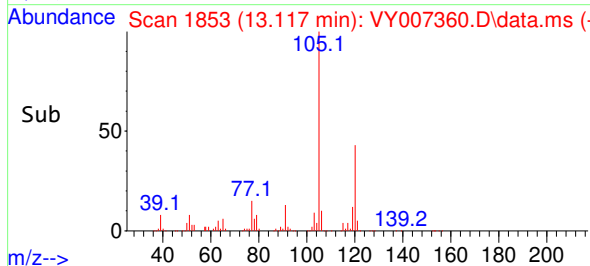

#85
sec-Butylbenzene
Concen: 973.93 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. -0.134 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion:105 Resp: 5831172
Ion Ratio Lower Upper
105 100
134 0.0 10.2 30.4#









#86
p-Isopropyltoluene
Concen: 51.72 ug/l
RT: 13.367 min Scan# 1
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion:	119	Resp:	252253
Ion	Ratio	Lower	Upper
119	100		
134	25.6	13.2	39.5
91	25.7	12.4	37.2

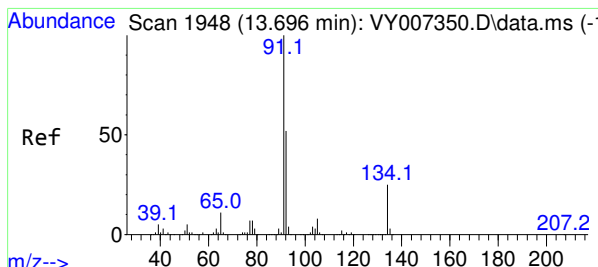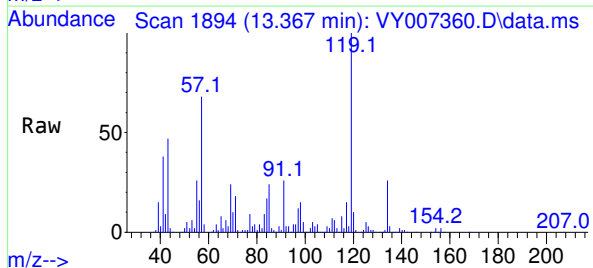

#89
n-Butylbenzene
Concen: 33.93 ug/l
RT: 13.697 min Scan# 1948
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion:	91	Resp:	159292
Ion	Ratio	Lower	Upper
91	100		
92	66.8	26.3	78.9
134	0.0	13.0	38.9#


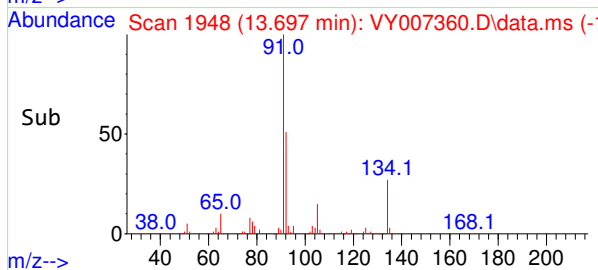

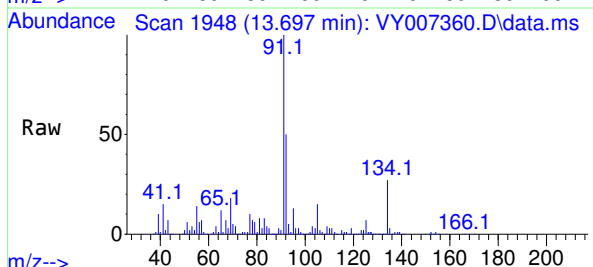




#90
Hexachloroethane
Concen: 72.28 ug/l
RT: 13.971 min Scan# 1
Delta R.T. 0.012 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32




Instrument :
MSVOA_Y
ClientSampleId :
CC-7


Tgt Ion:117 Resp: 66622
Ion Ratio Lower Upper
117 100
201 0.0 43.0 128.8#

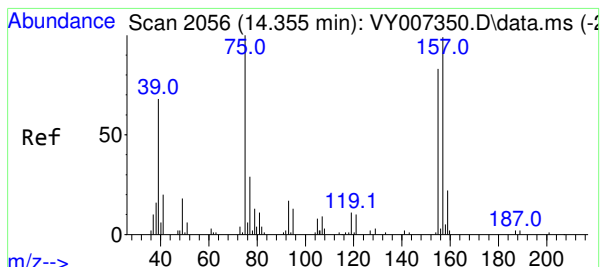

#92
1,2-Dibromo-3-Chloropropane
Concen: 16.84 ug/l
RT: 14.331 min Scan# 2052
Delta R.T. -0.024 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Tgt Ion: 75 Resp: 2809
Ion Ratio Lower Upper
75 100
155 0.0 38.0 113.9#
157 0.0 47.8 143.3#

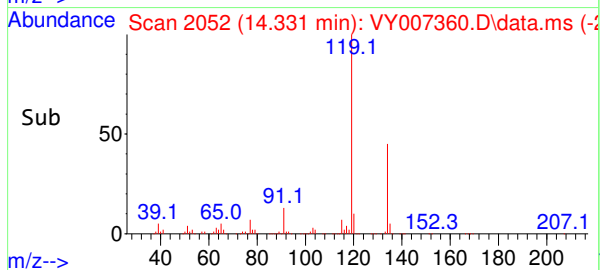

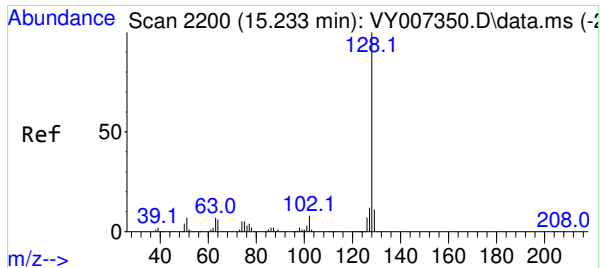

#95
Naphthalene
Concen: 350.24 ug/l
RT: 15.233 min Scan# 2
Delta R.T. 0.000 min
Lab File: VY007360.D
Acq: 02 Feb 2022 17:32

Instrument :
MSVOA_Y
ClientSampleId :
CC-7

Tgt Ion:128 Resp: 870933
Ion Ratio Lower Upper
128 100
127 13.1 11.0 16.4
129 11.0 8.4 12.6

