
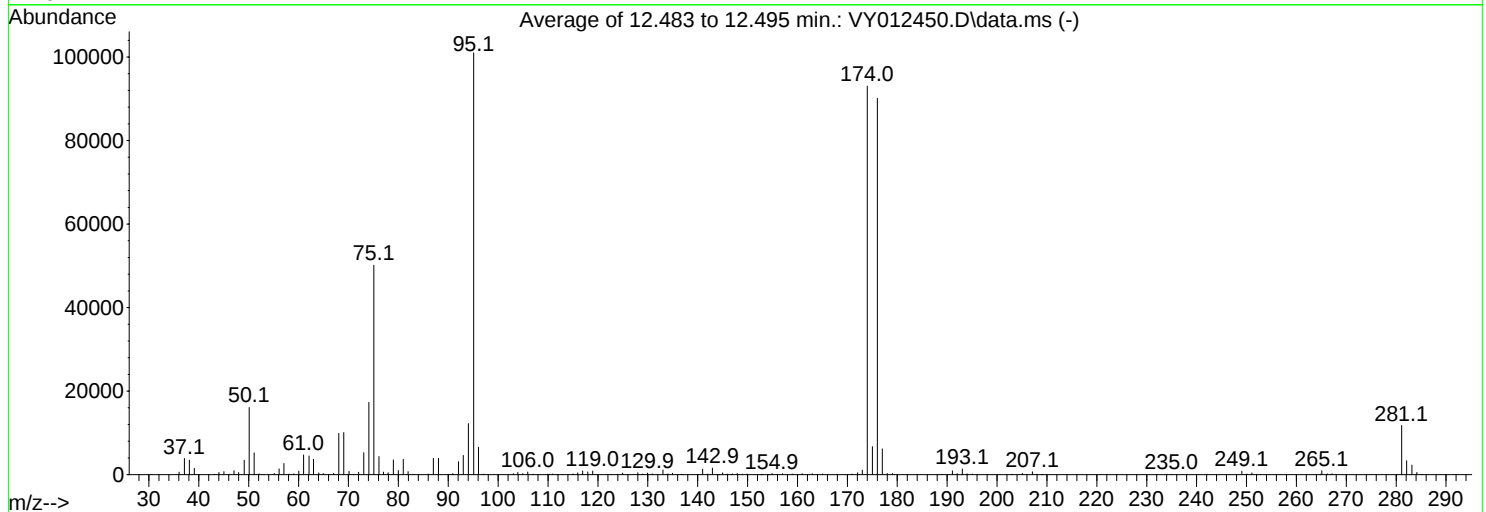


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020223\
Data File : VY012450.D
Acq On : 02 Feb 2023 09:23
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Title : SW846 8260
Last Update : Tue Jan 17 04:31:47 2023

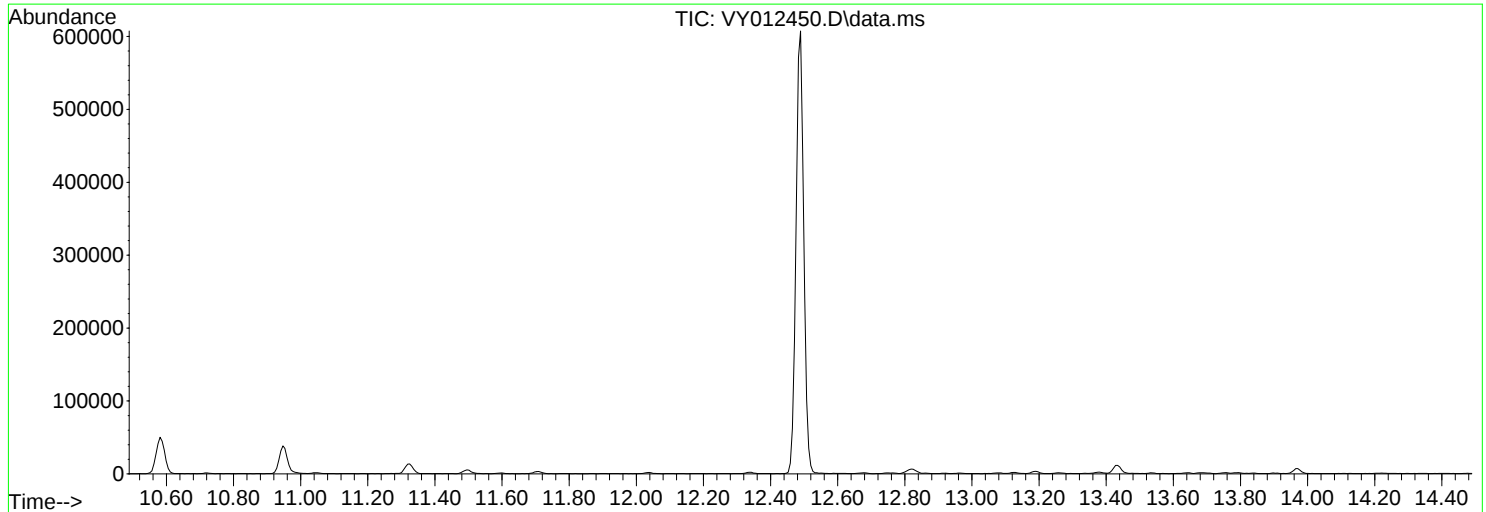

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.9	16103	PASS
75	95	30	60	49.7	50165	PASS
95	95	100	100	100.0	101005	PASS
96	95	5	9	6.5	6580	PASS
173	174	0.00	2	1.1	1066	PASS
174	95	50	100	92.1	93045	PASS
175	174	5	9	7.2	6703	PASS
176	174	95	101	96.9	90117	PASS
177	176	5	9	6.8	6155	PASS