

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020321\
 Data File : VY003980.D
 Acq On : 03 Feb 2021 23:17
 Operator : SY/MD
 Sample : M1291-16
 Misc : 8.67g/5mL/MSVOA_Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU421-004-0002

Quant Time: Feb 04 01:25:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012821S.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 01 00:38:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	82399	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	134786	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	127795	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	63778	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.155	65	55072	60.78	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	121.56%
35) Dibromofluoromethane	7.728	113	43959	55.78	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	111.56%
50) Toluene-d8	10.185	98	164465	53.18	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	106.36%
62) 4-Bromofluorobenzene	12.483	95	61104	54.20	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	108.40%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020321\
Data File : VY003980.D
Acq On : 03 Feb 2021 23:17
Operator : SY/MD
Sample : M1291-16
Misc : 8.67g/5mL/MSVOA_Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU421-004-0002


Quant Time: Feb 04 01:25:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012821S.M
Quant Title : SW846 8260
QLast Update : Mon Feb 01 00:38:02 2021
Response via : Initial Calibration

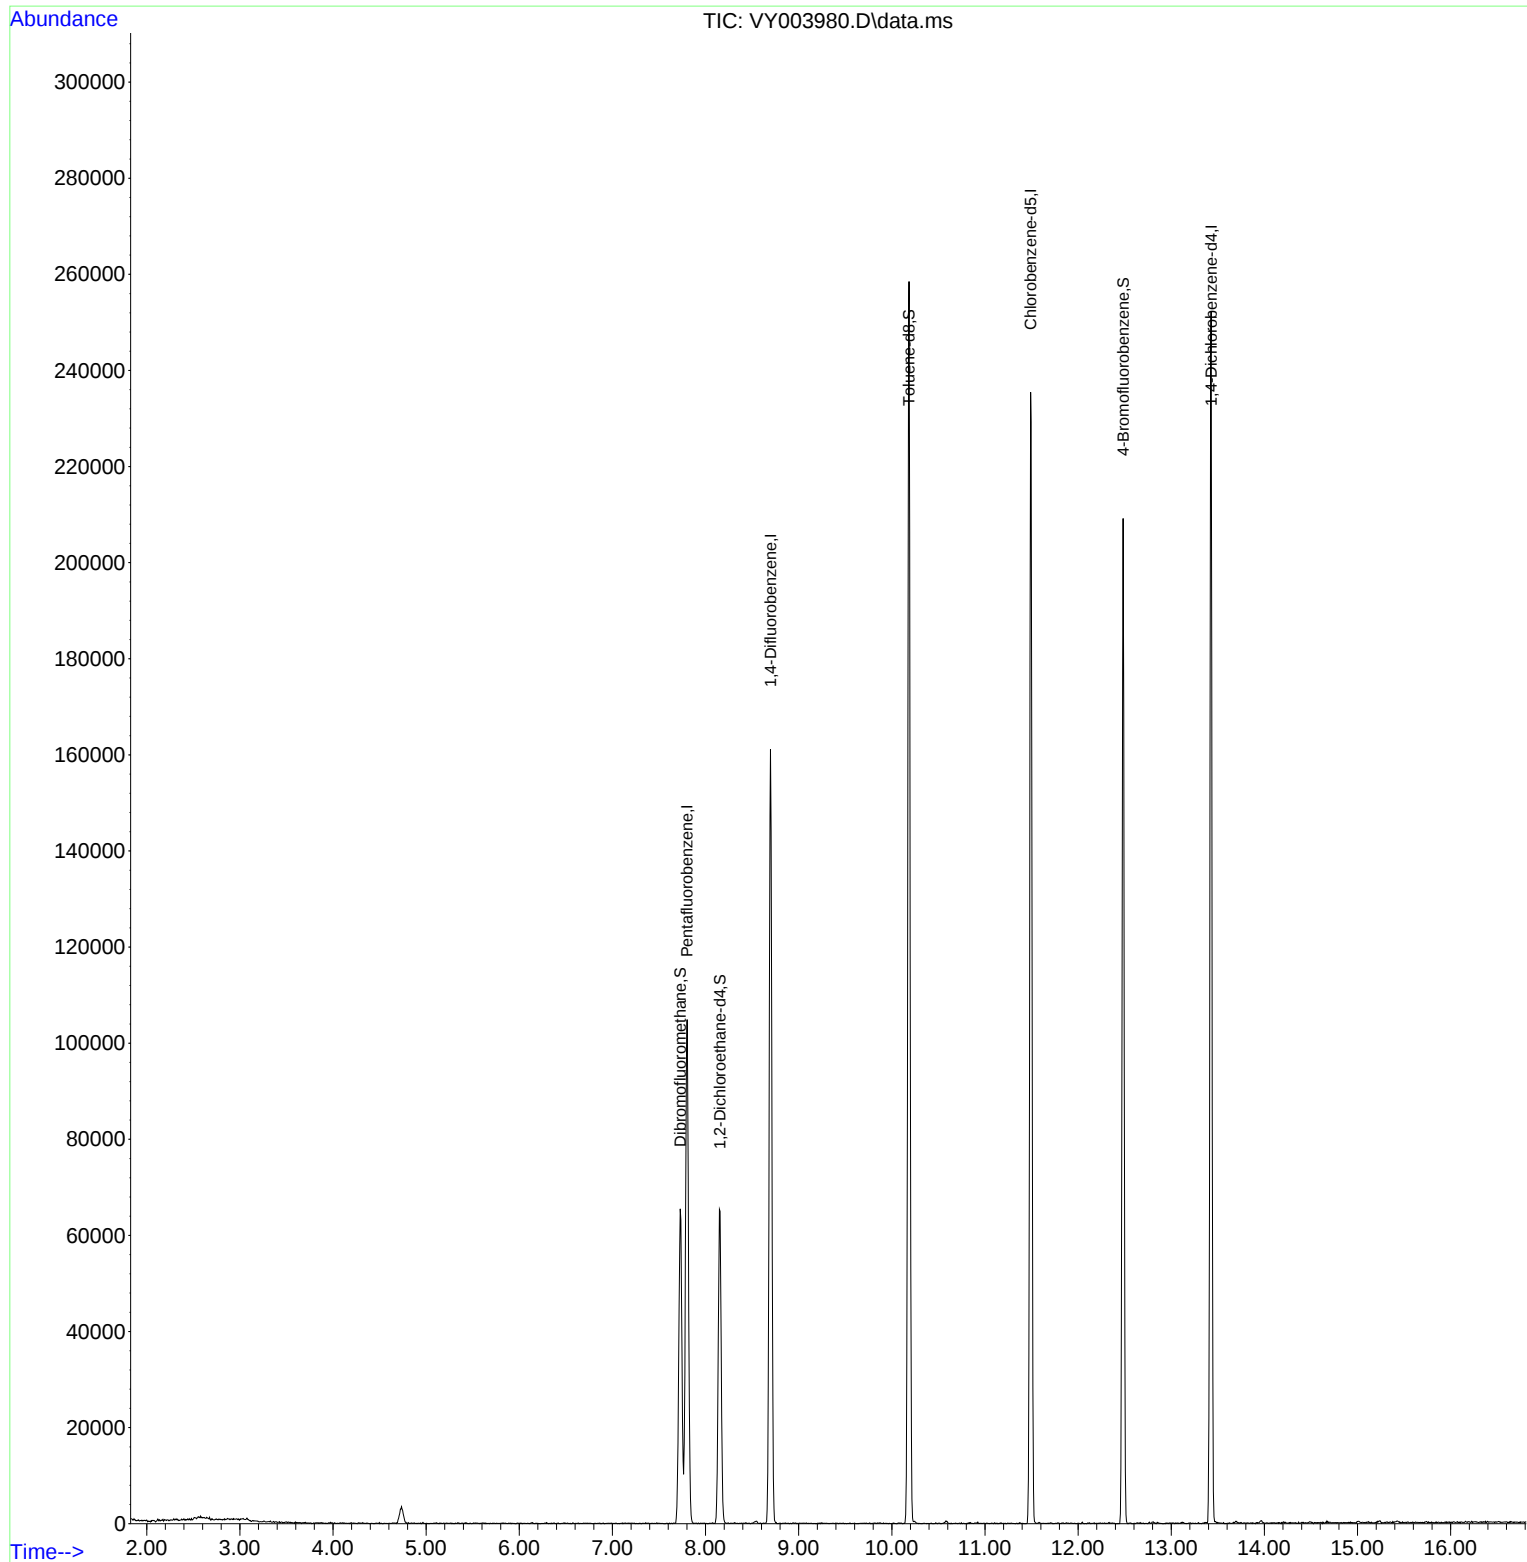



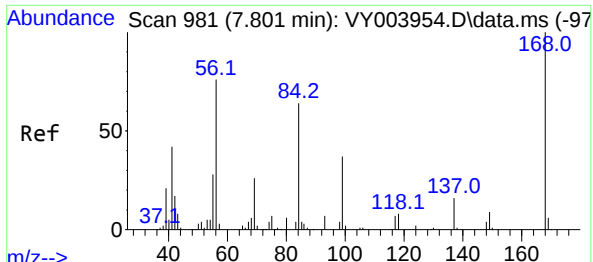


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY003980.D
Acq: 03 Feb 2021 23:17

Instrument :
MSVOA_Y
ClientSampleId :
OU421-004-0002



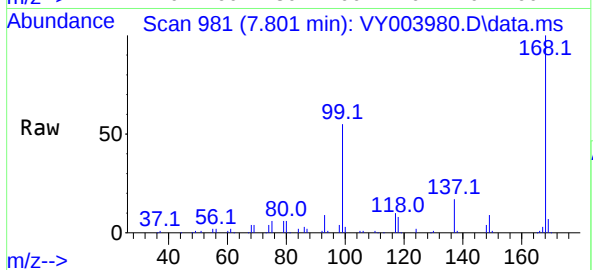



Tgt Ion:168 Resp: 82399
Ion Ratio Lower Upper
168 100
99 55.0 46.1 69.1

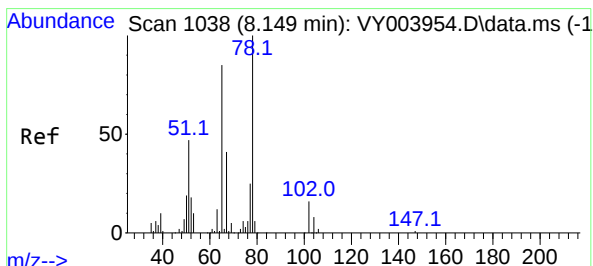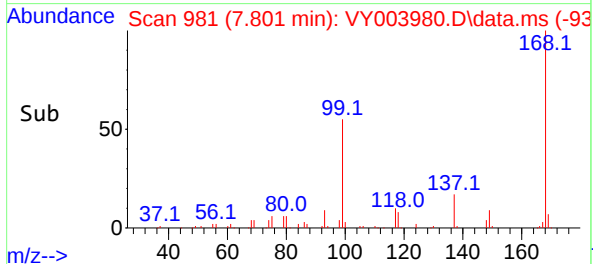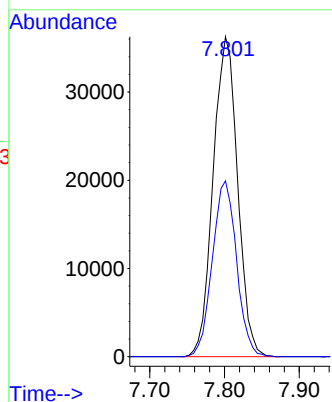

#33
1,2-Dichloroethane-d4
Concen: 60.78 ug/l
RT: 8.155 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY003980.D
Acq: 03 Feb 2021 23:17

Tgt Ion: 65 Resp: 55072
Ion Ratio Lower Upper
65 100
67 48.9 0.0 101.8

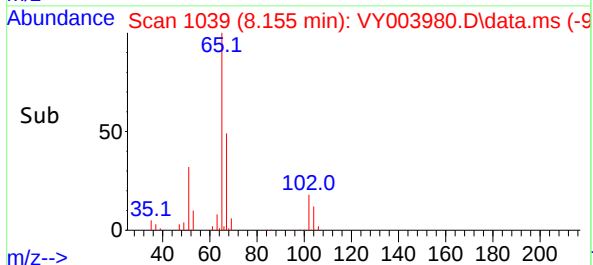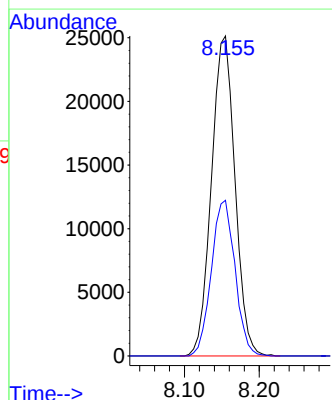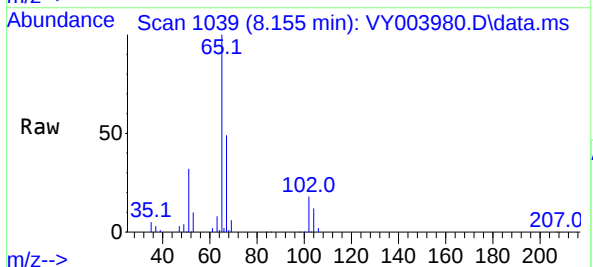

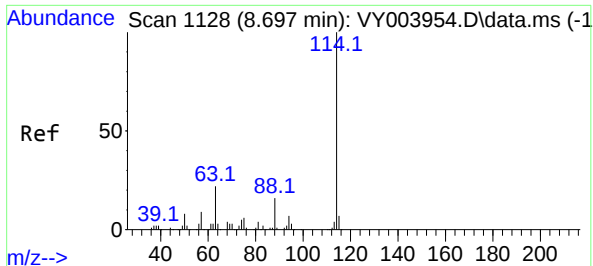

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.697 min Scan# 1128

Delta R.T. 0.000 min

Lab File: VY003980.D

Acq: 03 Feb 2021 23:17





Tgt Ion:114 Resp: 134786

Ion Ratio Lower Upper

114 100

63 21.5 0.0 47.2

88 16.5 0.0 30.2

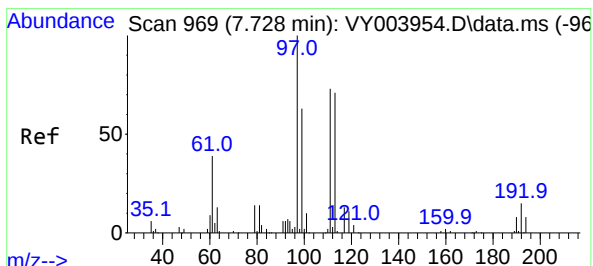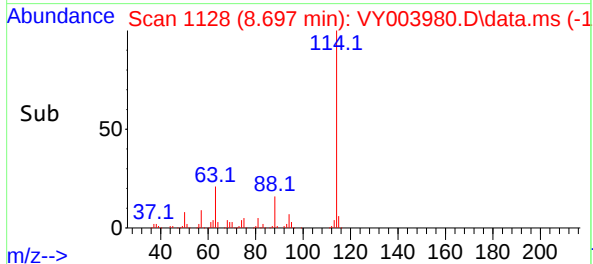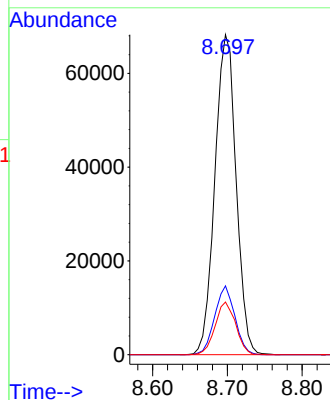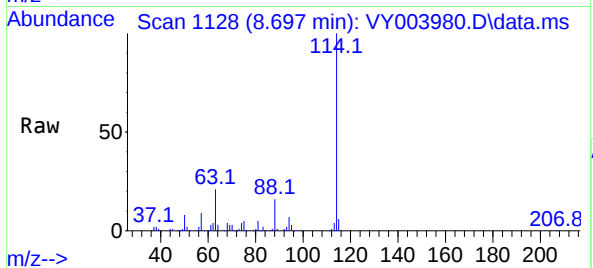

#35

Dibromofluoromethane

Concen: 55.78 ug/l

RT: 7.728 min Scan# 969

Delta R.T. 0.000 min

Lab File: VY003980.D

Acq: 03 Feb 2021 23:17




Tgt Ion:113 Resp: 43959


Ion Ratio Lower Upper

113 100

111 104.6 82.2 123.4

192 22.9 18.3 27.5


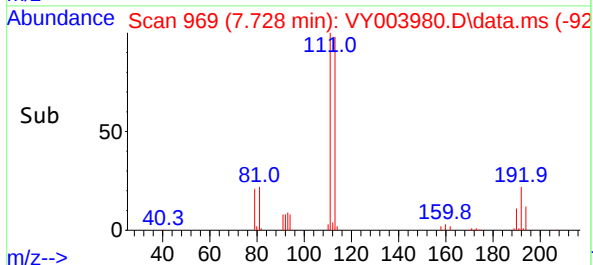
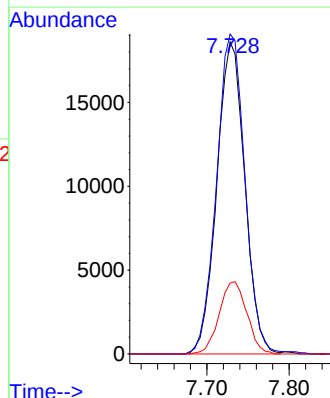
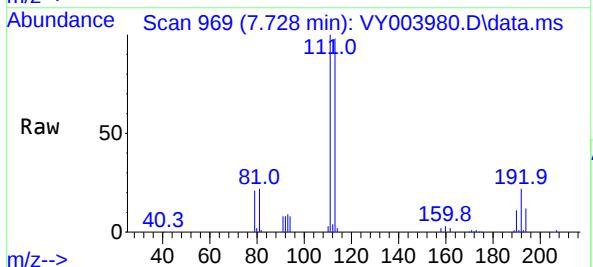


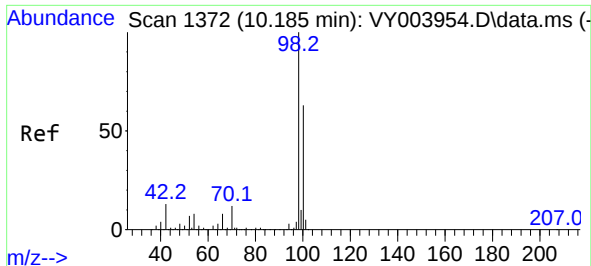

#50
Toluene-d8
Concen: 53.18 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY003980.D
Acq: 03 Feb 2021 23:17




Instrument :
MSVOA_Y
ClientSampleId :
OU421-004-0002


Tgt Ion: 98 Resp: 164465
Ion Ratio Lower Upper
98 100
100 64.5 50.5 75.7

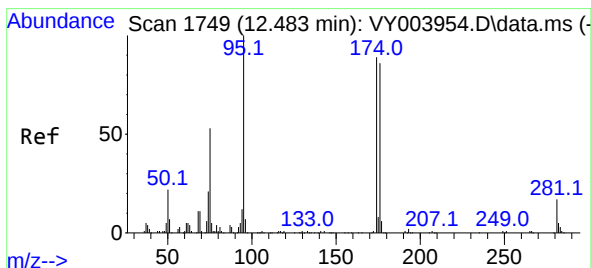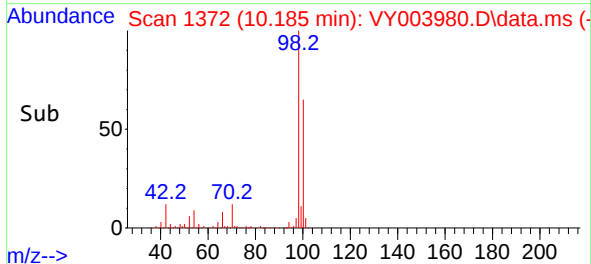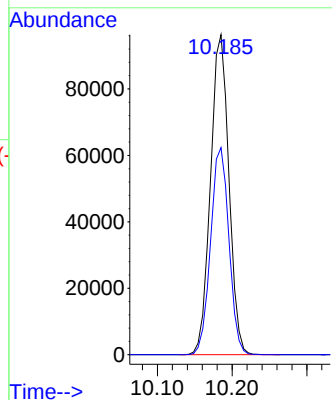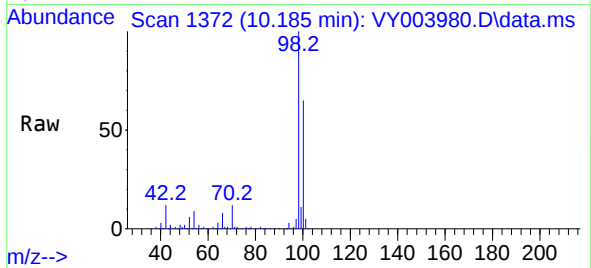

#62
4-Bromofluorobenzene
Concen: 54.20 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY003980.D
Acq: 03 Feb 2021 23:17

Tgt Ion: 95 Resp: 61104
Ion Ratio Lower Upper
95 100
174 89.2 0.0 184.4
176 86.0 0.0 177.2


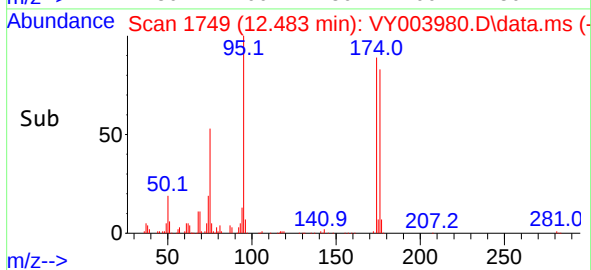
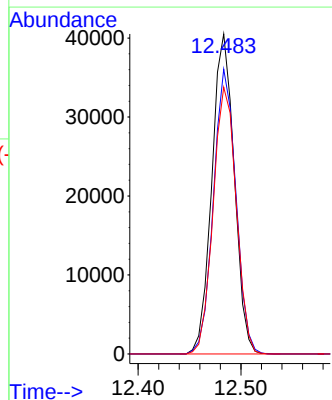
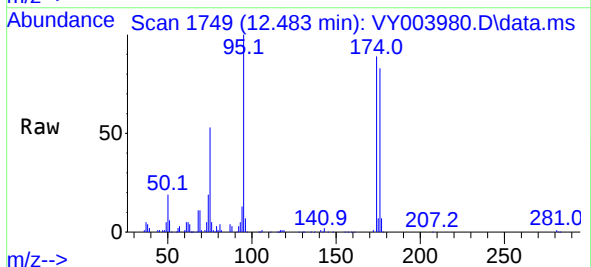


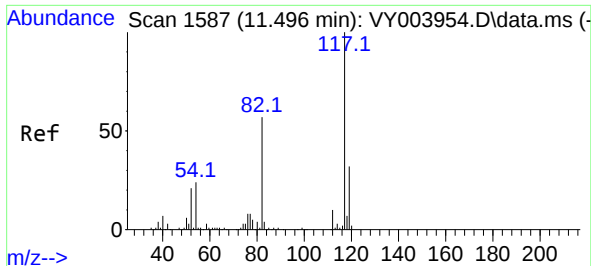

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY003980.D
Acq: 03 Feb 2021 23:17

Instrument :
MSVOA_Y
ClientSampleId :
OU421-004-0002

Tgt Ion:	117	Resp:	127795
Ion	Ratio	Lower	Upper
117	100		
82	54.9	44.3	66.5
119	30.9	25.0	37.6

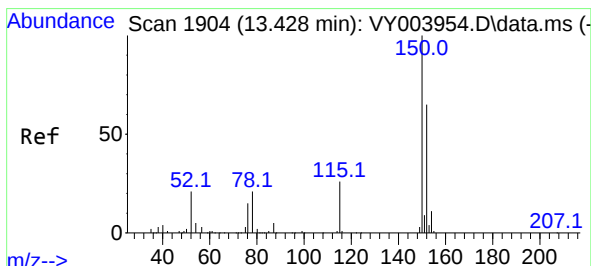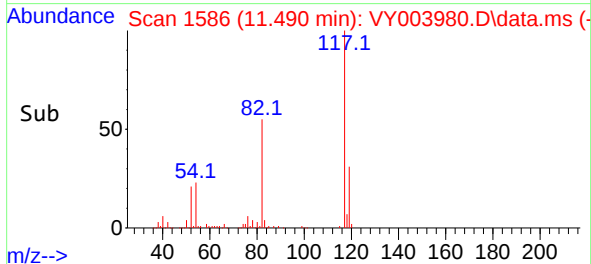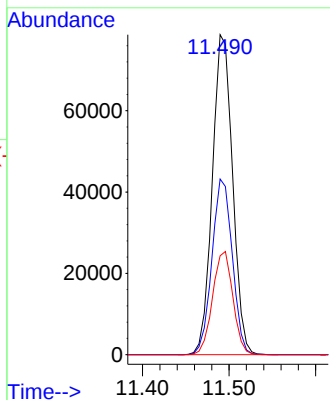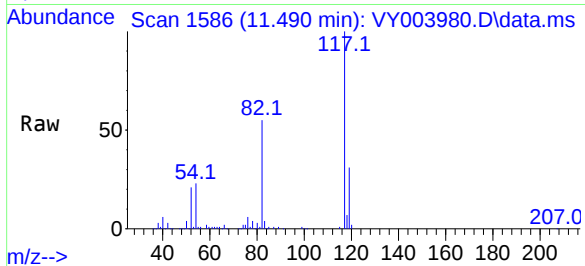

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY003980.D
Acq: 03 Feb 2021 23:17

Tgt Ion:	152	Resp:	63778
Ion	Ratio	Lower	Upper
152	100		
115	56.7	28.2	84.6
150	155.0	0.0	356.2

