
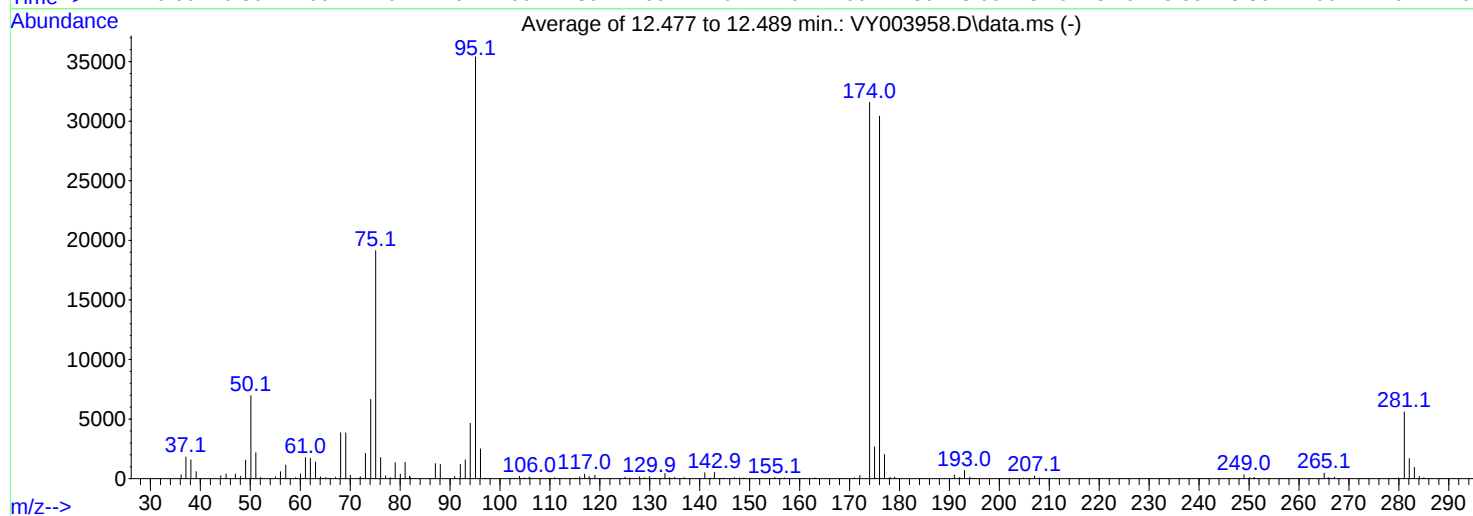


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020321\
 Data File : VY003958.D
 Acq On : 03 Feb 2021 14:04
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y0128215.M
 Title : SW846 8260
 Last Update : Mon Feb 01 00:38:02 2021

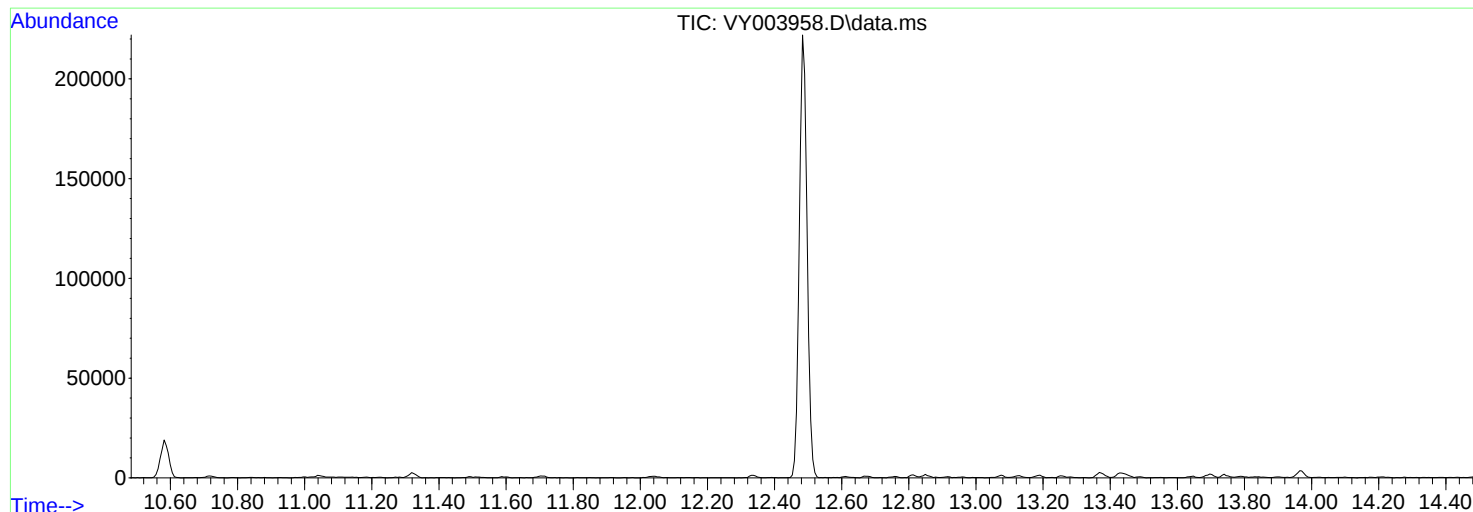

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	6968	PASS
75	95	30	60	54.1	19141	PASS
95	95	100	100	100.0	35400	PASS
96	95	5	9	7.0	2494	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.2	31581	PASS
175	174	5	9	8.4	2661	PASS
176	174	95	101	96.3	30424	PASS
177	176	5	9	6.7	2031	PASS