

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020323\
 Data File : VY012483.D
 Acq On : 03 Feb 2023 17:34
 Operator : KP/MD
 Sample : 01414-06
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SASP2-123-2(75-80)

Quant Time: Feb 04 00:12:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 04:31:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	83219	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	134112	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	126037	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	54140	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	44300	65.436	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	130.880%
35) Dibromofluoromethane	7.716	113	39118	55.086	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.180%
50) Toluene-d8	10.179	98	158227	65.665	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	131.340%
62) 4-Bromofluorobenzene	12.483	95	47175	47.125	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	94.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020323\
Data File : VY012483.D
Acq On : 03 Feb 2023 17:34
Operator : KP/MD
Sample : 01414-06
Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SASP2-123-2(75-80)

Quant Time: Feb 04 00:12:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 04:31:47 2023
Response via : Initial Calibration




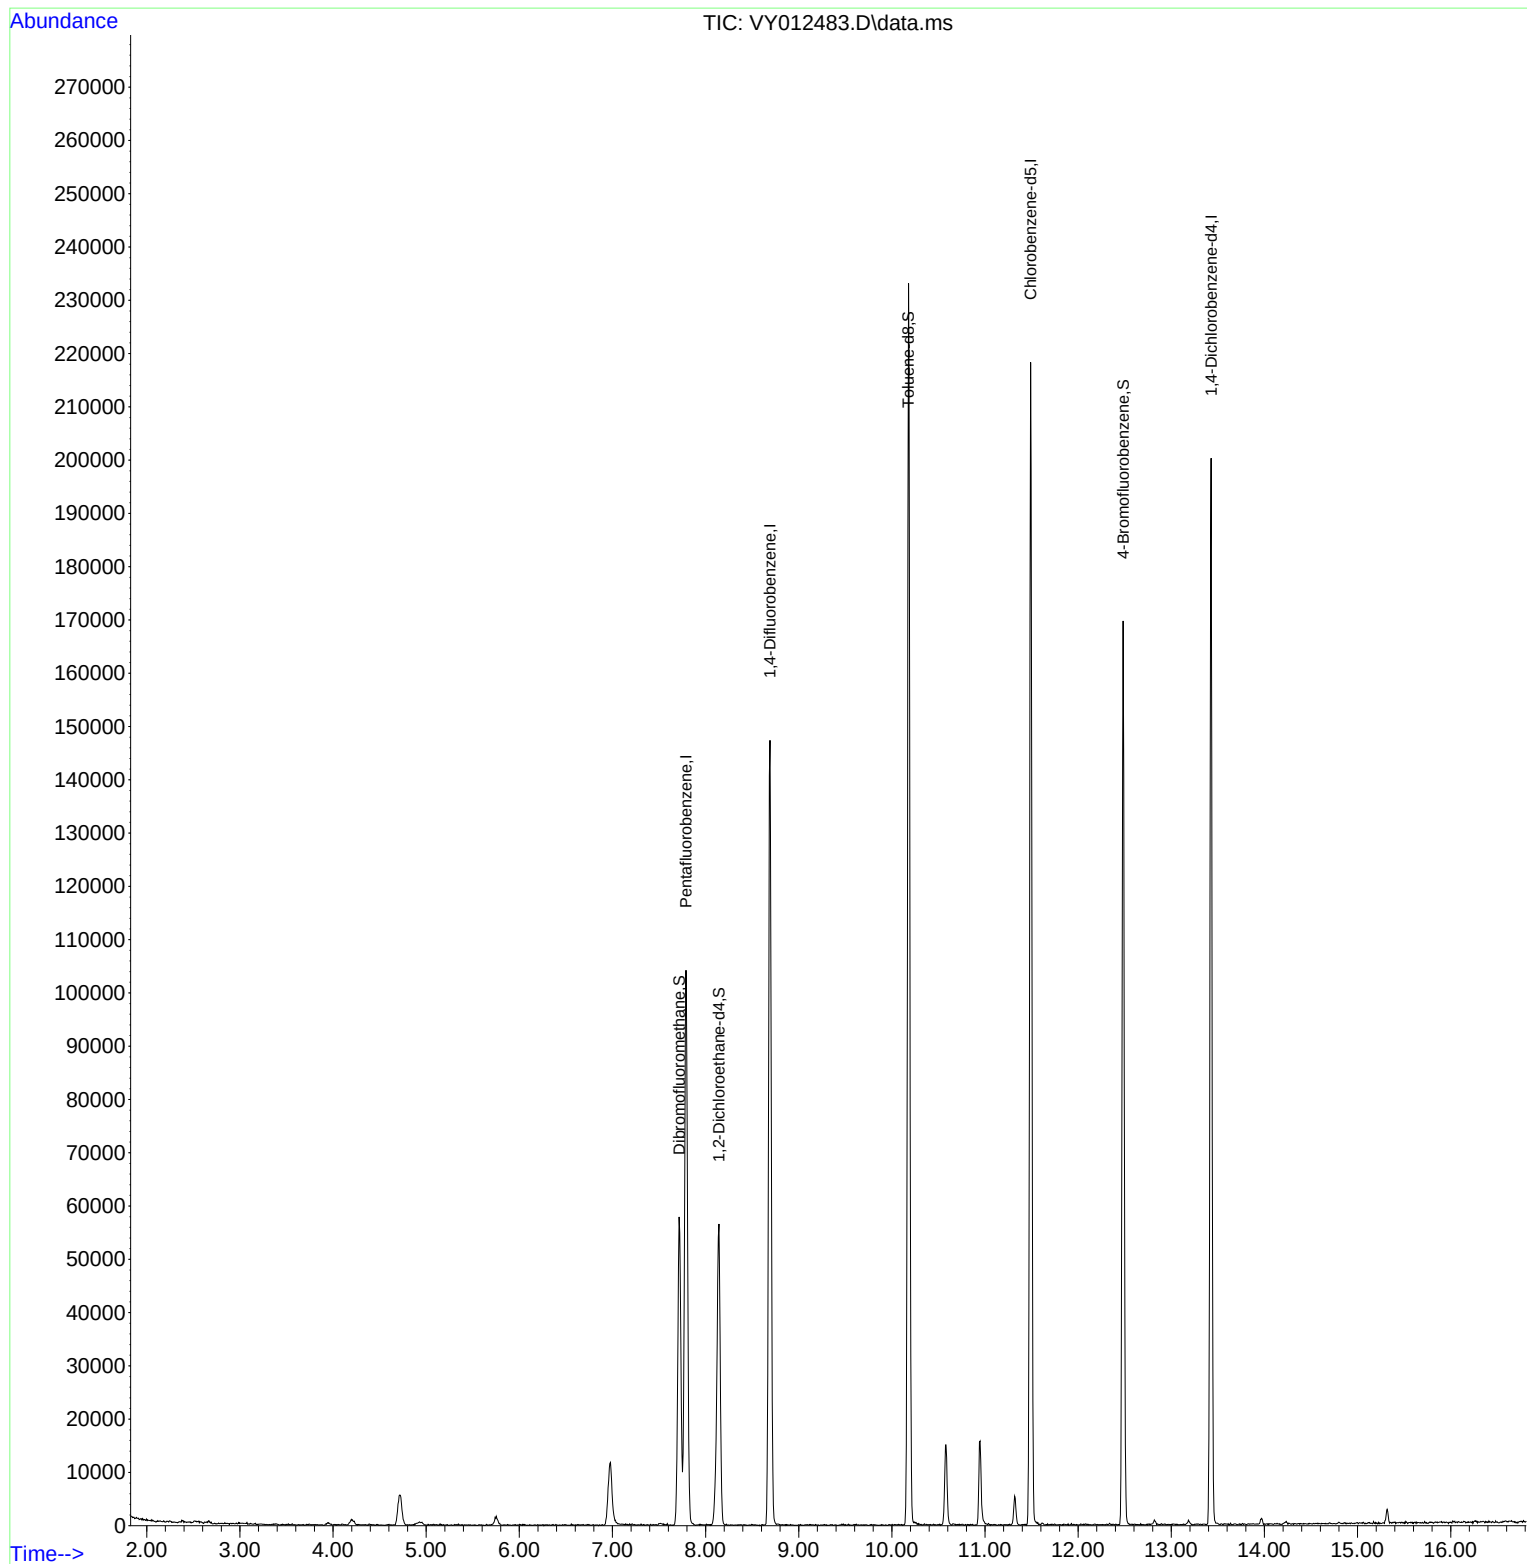


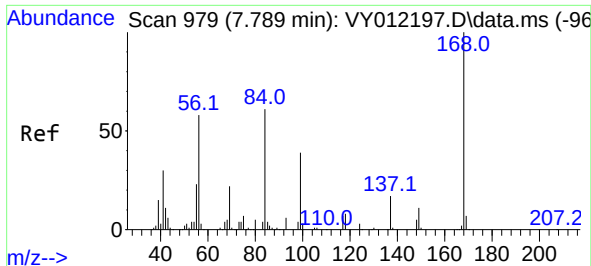

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012483.D
Acq: 03 Feb 2023 17:34




Instrument :
MSVOA_Y
ClientSampleId :
SASP2-123-2(75-80)


Tgt Ion:168 Resp: 83219
Ion Ratio Lower Upper
168 100
99 53.3 44.0 66.0

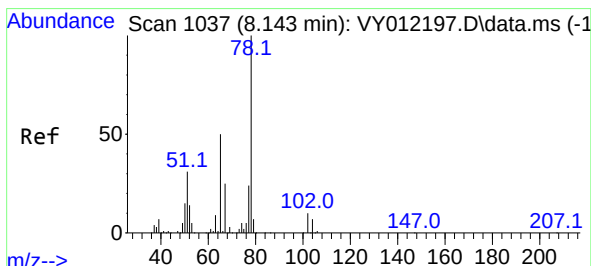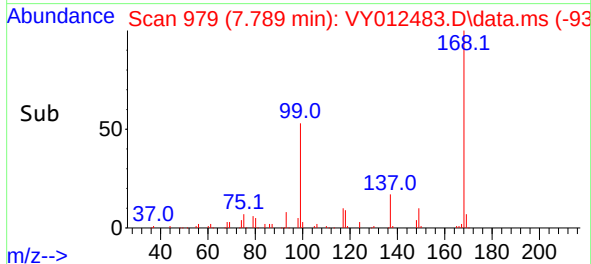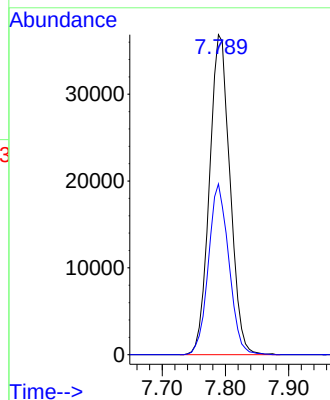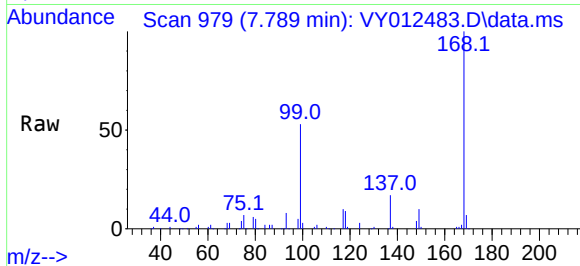

#33
1,2-Dichloroethane-d4
Concen: 65.436 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY012483.D
Acq: 03 Feb 2023 17:34

Tgt Ion: 65 Resp: 44300
Ion Ratio Lower Upper
65 100
67 49.8 0.0 103.2


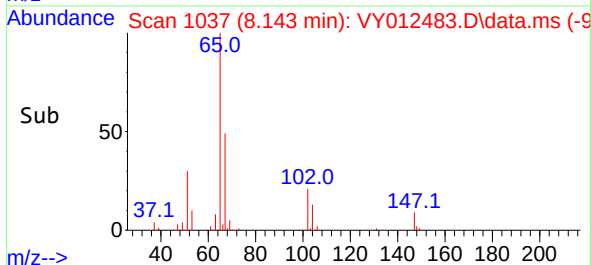
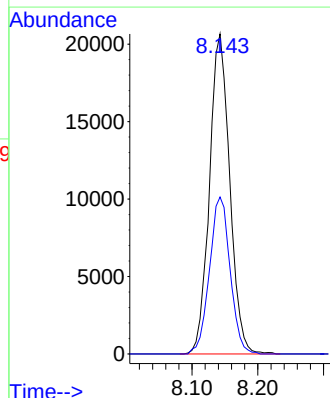
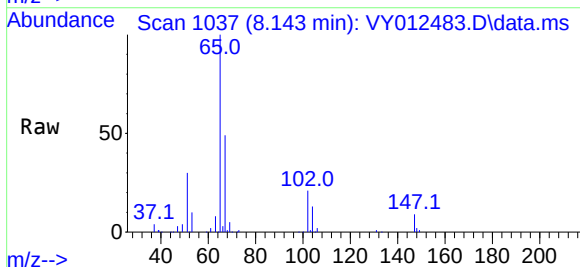


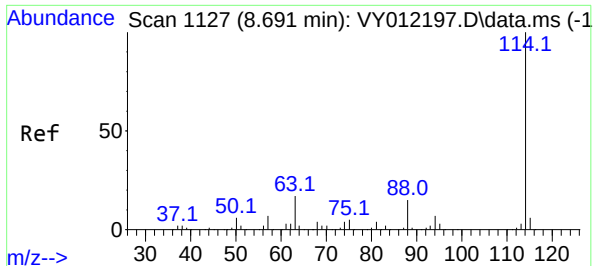

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY012483.D
Acq: 03 Feb 2023 17:34




Instrument :
MSVOA_Y
ClientSampleId :
SASP2-123-2(75-80)


Tgt Ion:114 Resp: 134112
Ion Ratio Lower Upper
114 100
63 17.2 0.0 39.6
88 14.5 0.0 32.2

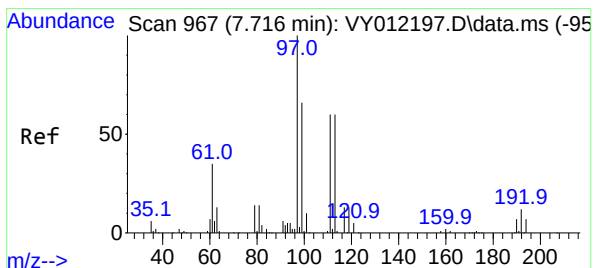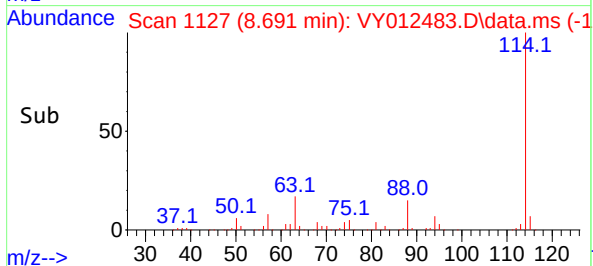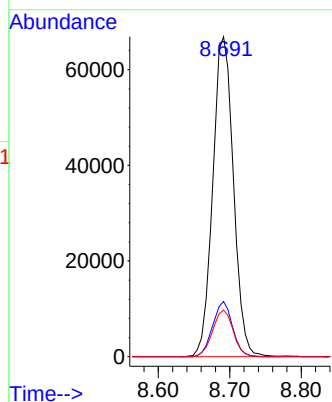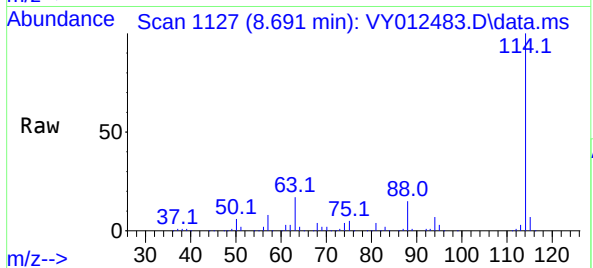

#35
Dibromofluoromethane
Concen: 55.086 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY012483.D
Acq: 03 Feb 2023 17:34

Tgt Ion:113 Resp: 39118
Ion Ratio Lower Upper
113 100
111 101.2 83.0 124.4
192 21.4 16.0 24.0


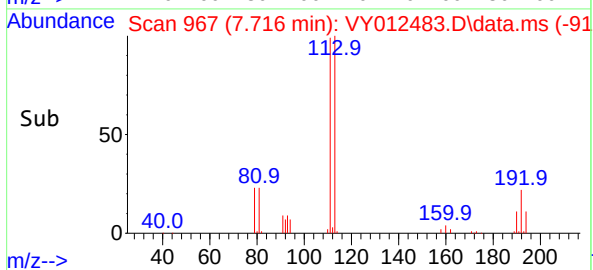
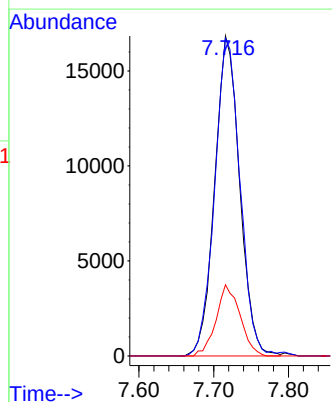
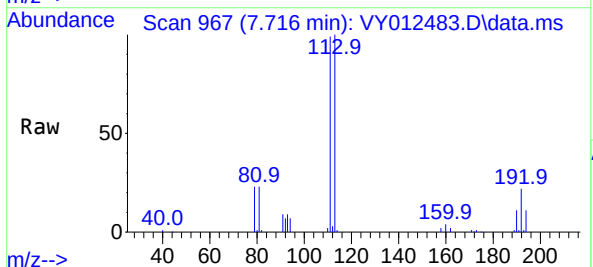


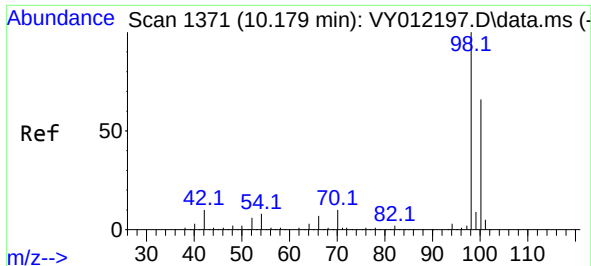

#50
Toluene-d8
Concen: 65.665 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY012483.D
Acq: 03 Feb 2023 17:34




Instrument :
MSVOA_Y
ClientSampleId :
SASP2-123-2(75-80)


Tgt Ion: 98 Resp: 158227
Ion Ratio Lower Upper
98 100
100 64.3 51.9 77.9

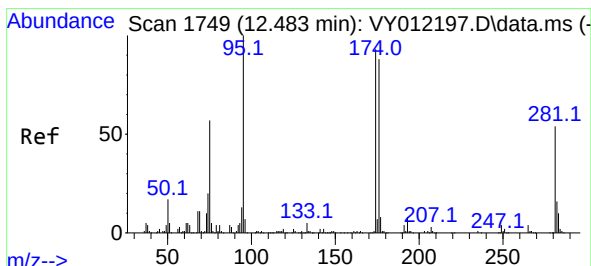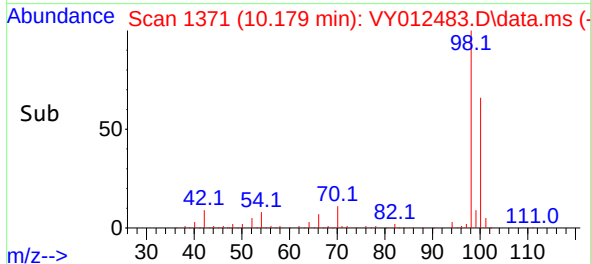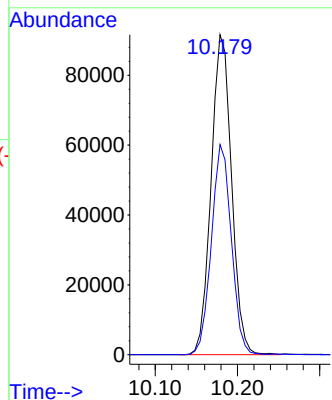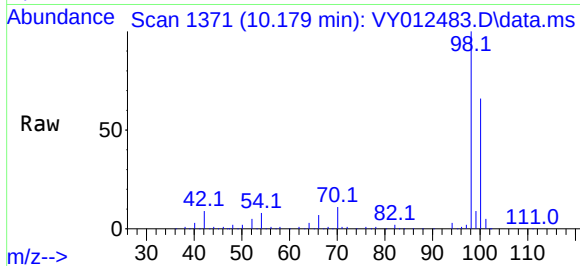

#62
4-Bromofluorobenzene
Concen: 47.125 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012483.D
Acq: 03 Feb 2023 17:34

Tgt Ion: 95 Resp: 47175
Ion Ratio Lower Upper
95 100
174 94.9 0.0 172.0
176 93.2 0.0 167.6


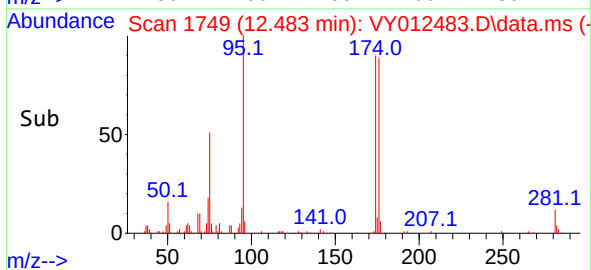
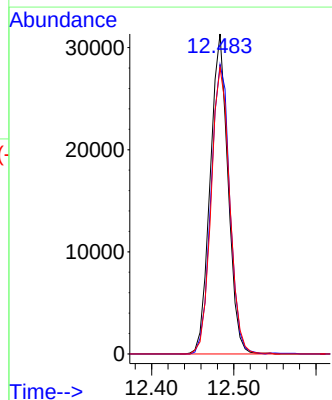
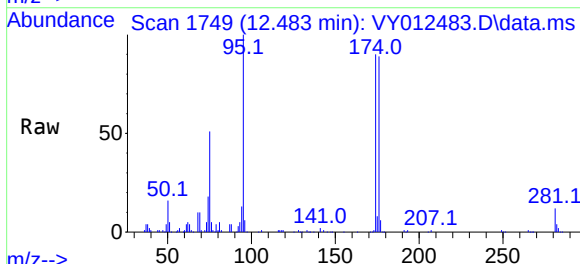


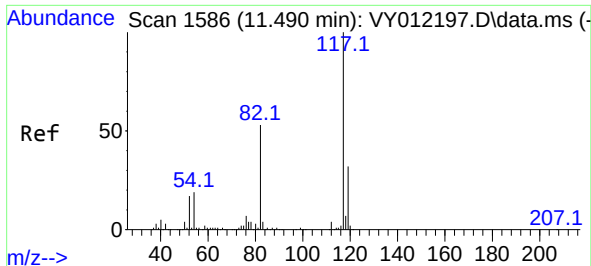

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.001 min
Lab File: VY012483.D
Acq: 03 Feb 2023 17:34

Instrument :
MSVOA_Y
ClientSampleId :
SASP2-123-2(75-80)

Tgt Ion:117 Resp: 126037
Ion Ratio Lower Upper
117 100
82 52.3 44.8 67.2
119 32.4 25.4 38.2

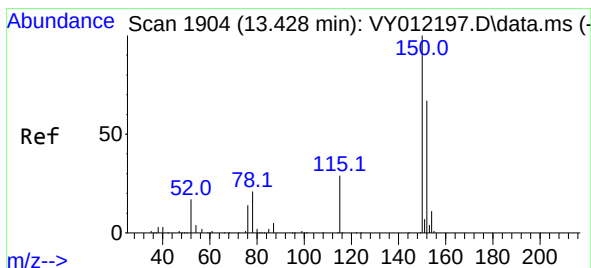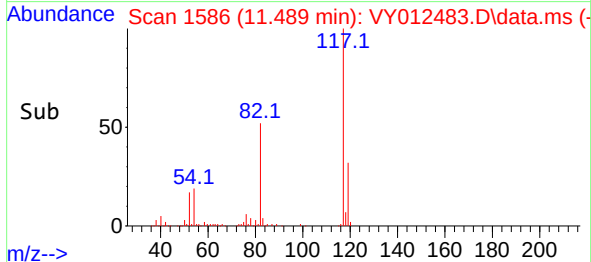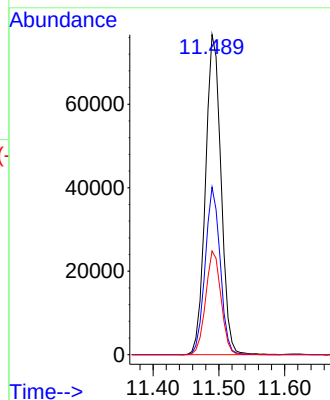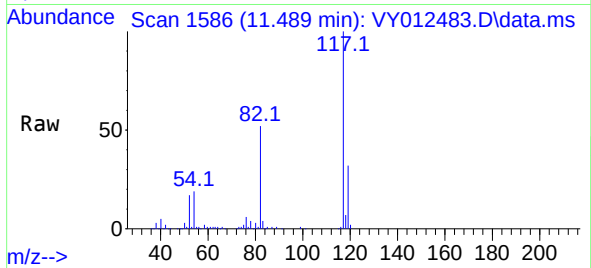

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY012483.D
Acq: 03 Feb 2023 17:34

Tgt Ion:152 Resp: 54140
Ion Ratio Lower Upper
152 100
115 55.6 29.1 87.3
150 157.5 0.0 342.6

