
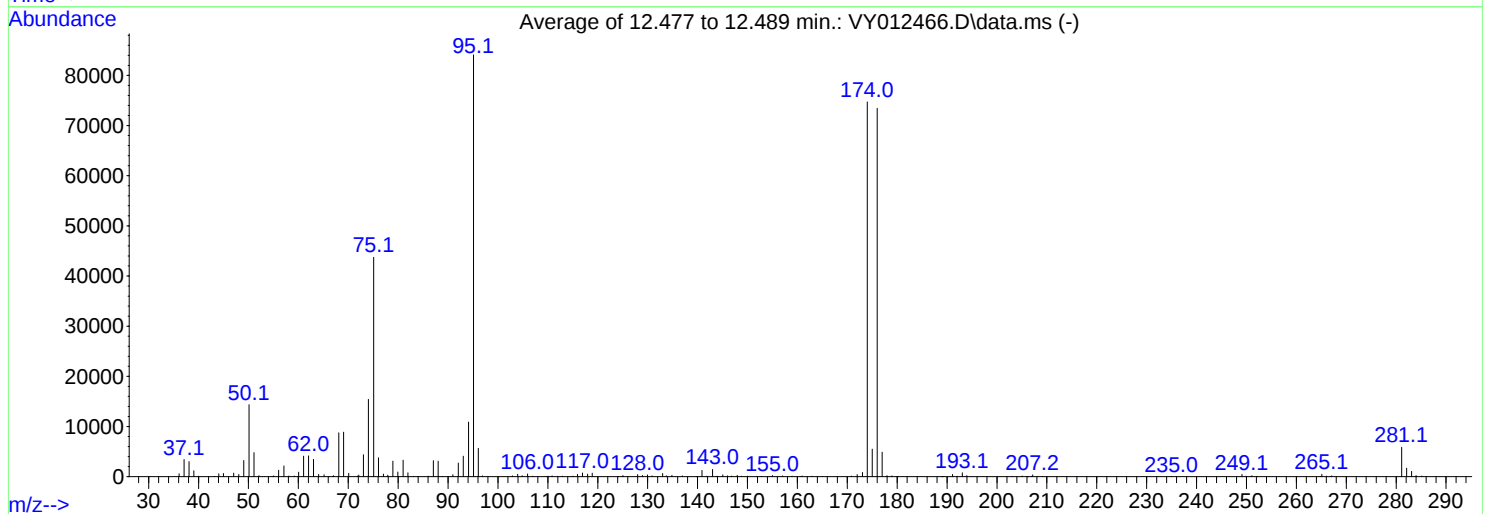


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020323\
Data File : VY012466.D
Acq On : 03 Feb 2023 09:07
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Title : SW846 8260
Last Update : Tue Jan 17 04:31:47 2023

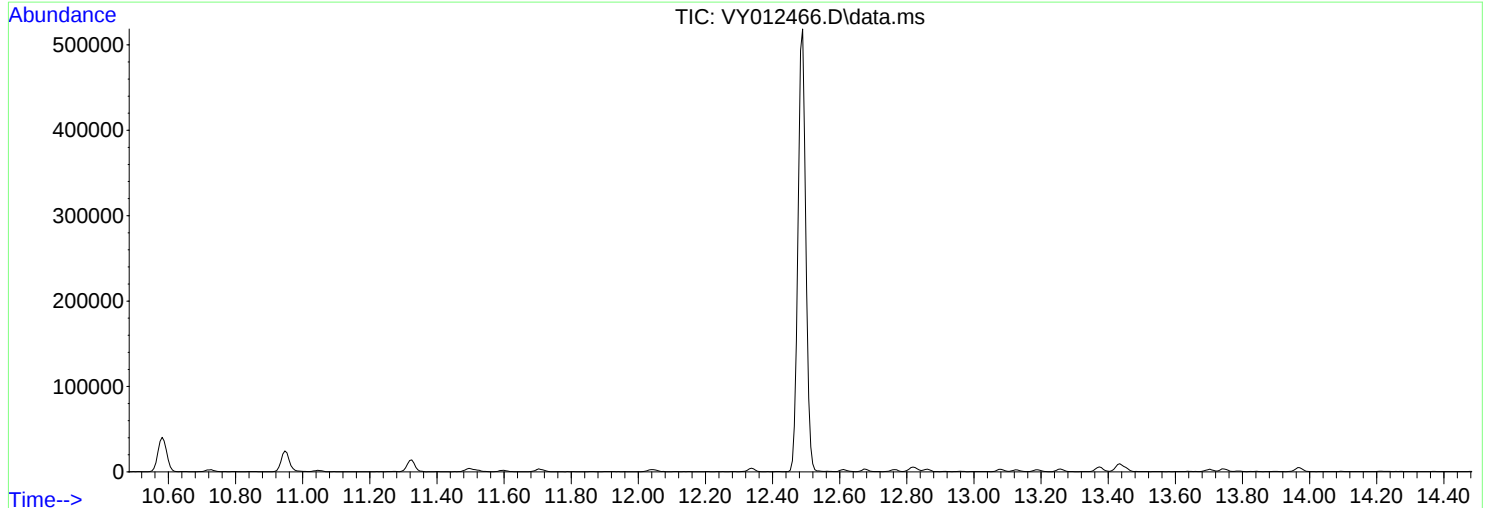

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	14374	PASS
75	95	30	60	52.0	43728	PASS
95	95	100	100	100.0	84099	PASS
96	95	5	9	6.7	5652	PASS
173	174	0.00	2	1.1	836	PASS
174	95	50	100	88.9	74728	PASS
175	174	5	9	7.4	5504	PASS
176	174	95	101	98.3	73443	PASS
177	176	5	9	6.6	4872	PASS