

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY020420\
 Data File : VY001496.D
 Acq On : 04 Feb 2020 18:50
 Operator : SY/MD
 Sample : L1329-22
 Misc : 5.05G/5ML/MSVOA Y/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 628-629

Quant Time: Feb 05 05:50:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 04 15:10:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.82	168	122015	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	214556	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	165488	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.43	152	47568	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.16	65	66845	54.41	ug/l	0.00
Spiked Amount			Recovery	=	108.82%	
35) Dibromofluoromethane	7.74	113	64728	52.32	ug/l	0.00
Spiked Amount			Recovery	=	104.64%	
50) Toluene-d8	10.19	98	235159	50.24	ug/l	0.00
Spiked Amount			Recovery	=	100.48%	
62) 4-Bromofluorobenzene	12.49	95	69829	37.87	ug/l	0.00
Spiked Amount			Recovery	=	75.74%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.96	59	3195	Below Cal	#	80
16) Acetone	3.98	43	5160	14.520	ug/l	95
25) 2-Butanone	7.00	43	4614	10.008	ug/l #	78
29) Tetrahydrofuran	7.38	42	574	2.077	ug/l #	66
31) Cyclohexane	7.81	56	2699	1.128	ug/l #	4
36) 1,1-Dichloropropene	7.81	75	9956	5.072	ug/l #	48
37) Ethyl Acetate	7.00	43	4614	4.856	ug/l #	74
38) Carbon Tetrachloride	7.81	117	12351	6.504	ug/l #	16
51) 4-Methyl-2-Pentanone	10.08	43	31216	33.693	ug/l	97
59) 2-Hexanone	10.85	43	1104	1.639	ug/l	74
68) m/p-Xylenes	11.70	106	5543	2.458	ug/l	98
69) o-Xylene	12.03	106	3427	1.612	ug/l	95
74) N-amyl acetate	12.12	43	4750	5.039	ug/l #	44
75) 1,1,2,2-Tetrachloroethane	12.55	83	709	1.029	ug/l #	26
76) 1,2,3-Trichloropropane	12.49	75	34404	67.255	ug/l #	100
78) n-propylbenzene	12.67	91	8984	2.069	ug/l	98
80) 1,3,5-Trimethylbenzene	12.81	105	9721	3.182	ug/l	96
81) trans-1,4-Dichloro-2-buten	12.49	75	34404	130.135	ug/l #	16
84) 1,2,4-Trimethylbenzene	13.13	105	41401	13.691	ug/l	97
85) sec-Butylbenzene	13.26	105	6340	1.746	ug/l	90
86) p-Isopropyltoluene	13.38	119	3869	1.209	ug/l	96
89) n-Butylbenzene	13.70	91	14696	4.655	ug/l #	75
90) Hexachloroethane	13.97	117	2207	3.594	ug/l #	16
92) 1,2-Dibromo-3-Chloropropan	14.34	75	208	1.635	ug/l #	3
95) Naphthalene	15.24	128	15269	7.070	ug/l #	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY020420\
Data File : VY001496.D
Acq On : 04 Feb 2020 18:50
Operator : SY/MD
Sample : L1329-22
Misc : 5.05G/5ML/MSVOA Y/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
628-629

Quant Time: Feb 05 05:50:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 04 15:10:08 2020
Response via : Initial Calibration

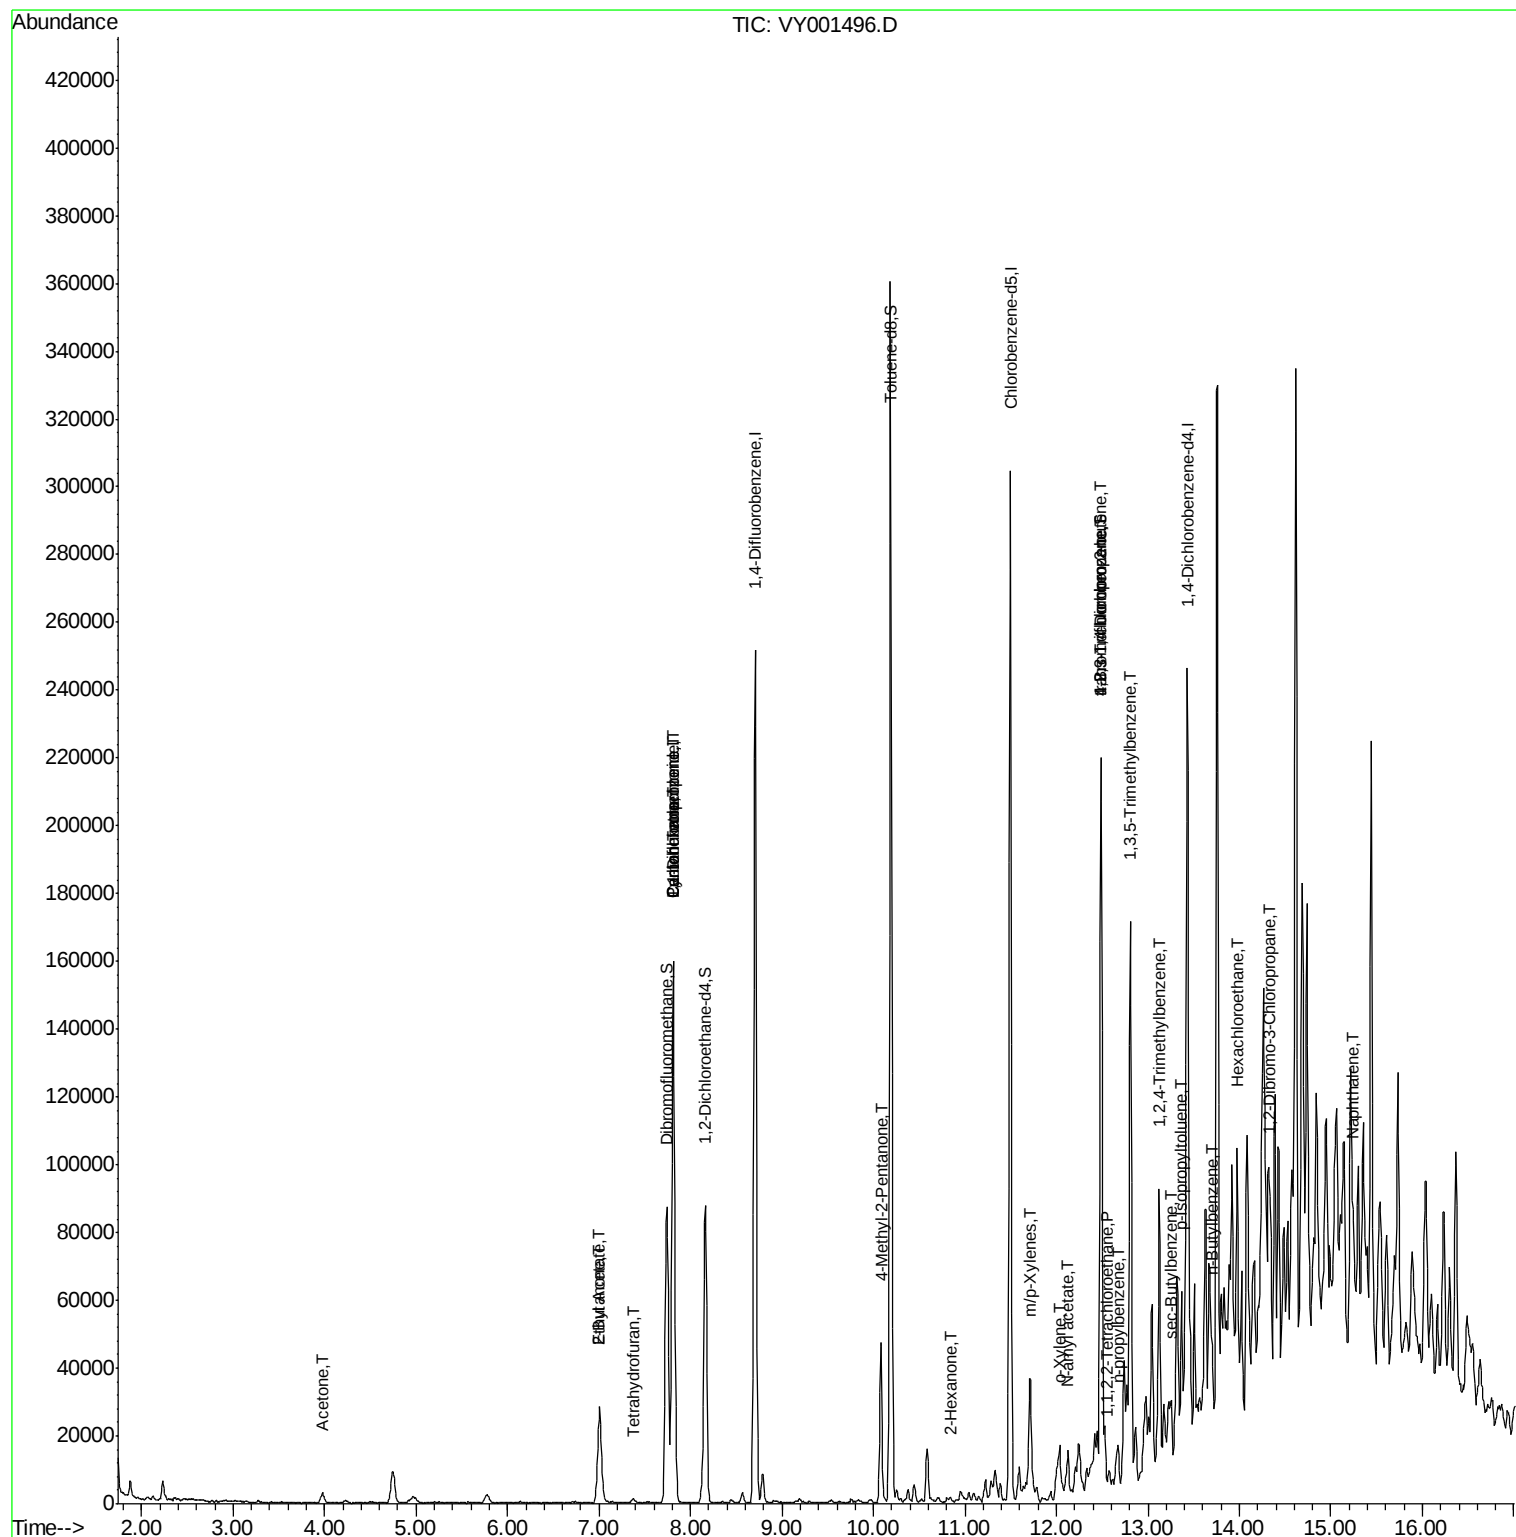

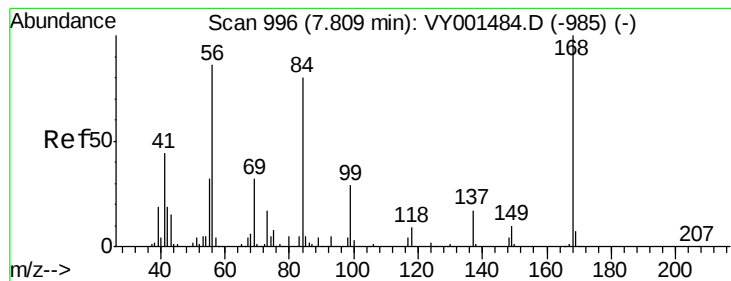

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.82 min Scan# 997

Delta R.T. 0.01 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50

Instrument :

MSVOA_Y

ClientSampleId :


628-629

Tot Ion:168 Resp: 122015

Ion Ratio Lower Upper

168 100

99 56.1 48.2 72.4



Abundance Ion 167.90 (167.60 to 168.60): VY001484.D (-985) (-)

Ion 98.90 (98.60 to 99.60): VY001484.D (-985) (-)

7.82

60000

50000

40000



30000

20000

10000

0

Time-->

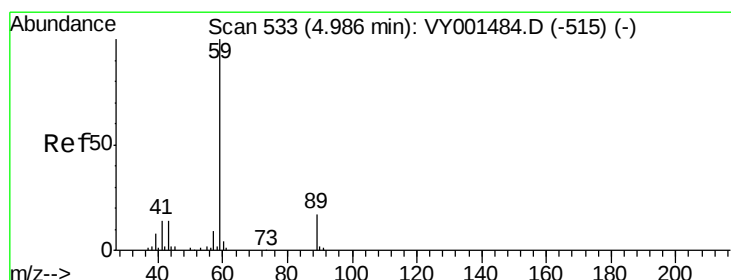

#11

Tert butyl alcohol

Concen: Below Cal

RT: 4.96 min Scan# 529

Delta R.T. -0.02 min

Lab File: VY001496.D


Acq: 04 Feb 2020 18:50

Tgt Ion: 59 Resp: 3195

Ion Ratio Lower Upper

59 100

57 1.4 7.0 10.6#

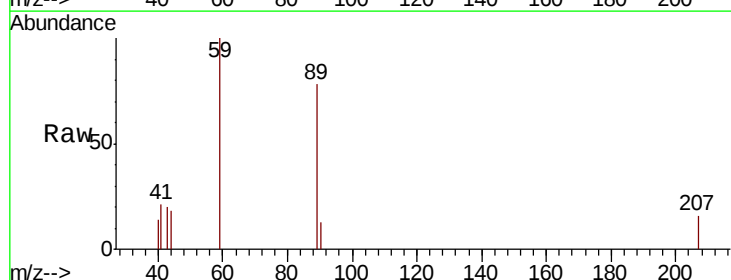

Abundance Ion 59.00 (58.70 to 59.70): VY001484.D (-515) (-)

Ion 57.00 (56.70 to 57.70): VY001484.D (-515) (-)

4.96

800


600


400

200

0

Time-->

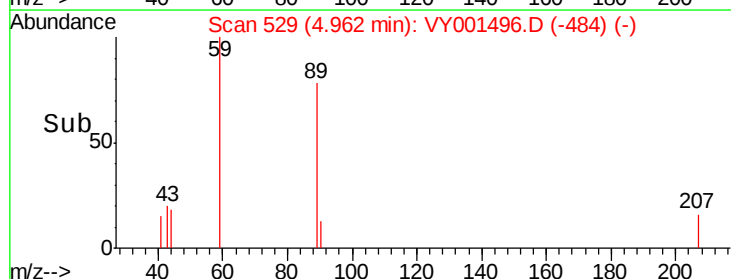

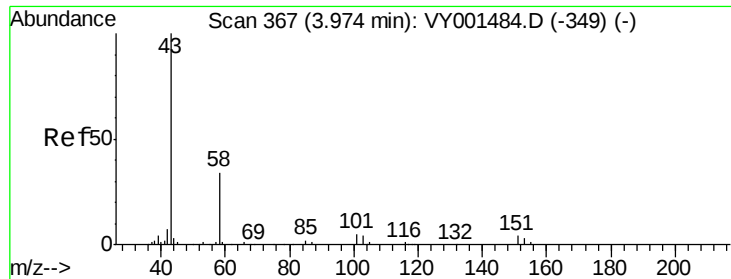

#16

Acetone

Concen: 14.520 ug/l

RT: 3.98 min Scan# 368

Delta R.T. 0.01 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50

Instrument :

MSVOA_Y

ClientSampleId :


628-629

Tot Ion: 43 Resp: 5160

Ion Ratio Lower Upper

43 100

58 31.4 27.5 41.3



Abundance Ion 43.00 (42.70 to 43.70): VY0

Ion 58.00 (57.70 to 58.70): VY0

2000

1500



1000

500

0

3.90 4.00 4.10

Time-->

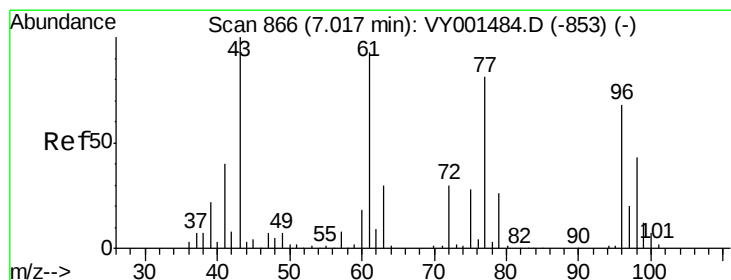

#25

2-Butanone

Concen: 10.008 ug/l

RT: 7.00 min Scan# 864

Delta R.T. -0.01 min

Lab File: VY001496.D


Acq: 04 Feb 2020 18:50

Tgt Ion: 43 Resp: 4614

Ion Ratio Lower Upper

43 100

72 17.8 23.8 35.8#



Abundance Ion 43.00 (42.70 to 43.70): VY0

Ion 72.00 (71.70 to 72.70): VY0

1500


1000


500

0

6.90 7.00 7.10

Time-->









#29
Tetrahydrofuran
Concen: 2.077 ug/l
RT: 7.38 min Scan# 925
Delta R.T. 0.01 min
Lab File: VY001496.D
Acq: 04 Feb 2020 18:50




Instrument :
MSVOA_Y
ClientSampleId :
628-629


Tot Ion: 42 Resp: 574
Ion Ratio Lower Upper
42 100
72 7.1 37.8 56.6#
71 39.9 34.8 52.2

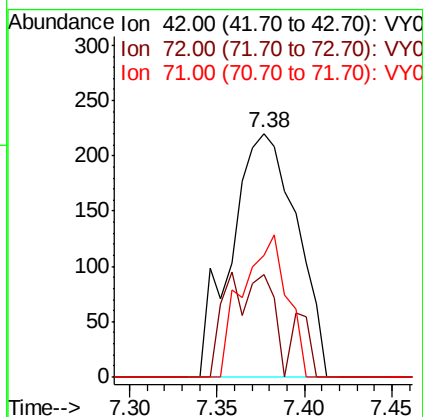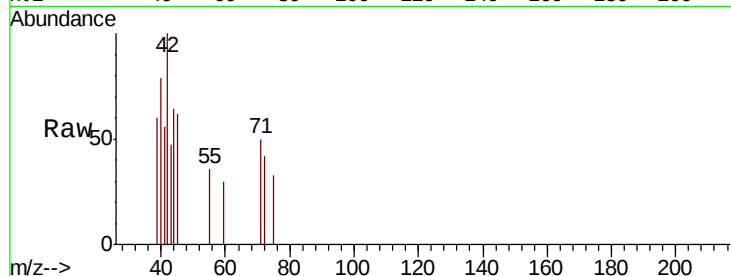

#31
Cyclohexane
Concen: 1.128 ug/l
RT: 7.81 min Scan# 996
Delta R.T. 0.00 min
Lab File: VY001496.D
Acq: 04 Feb 2020 18:50

Tgt Ion: 56 Resp: 2699
Ion Ratio Lower Upper
56 100
69 162.0 29.6 44.4#
84 139.6 73.6 110.4#



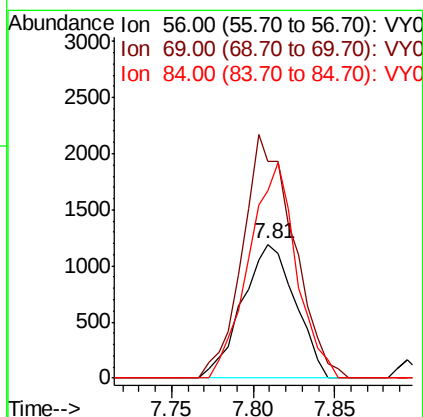



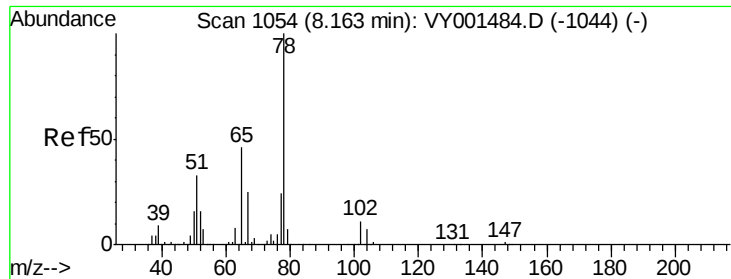

#33
 1,2-Dichloroethane-d4
 Concen: 54.411 ug/l
 RT: 8.16 min Scan# 1054
 Delta R.T. 0.00 min
 Lab File: VY001496.D
 Acq: 04 Feb 2020 18:50




Instrument :
 MSVOA_Y
 ClientSampleId :
 628-629


Tot Ion: 65 Resp: 66845
 Ion Ratio Lower Upper
 65 100
 67 53.7 0.0 108.6

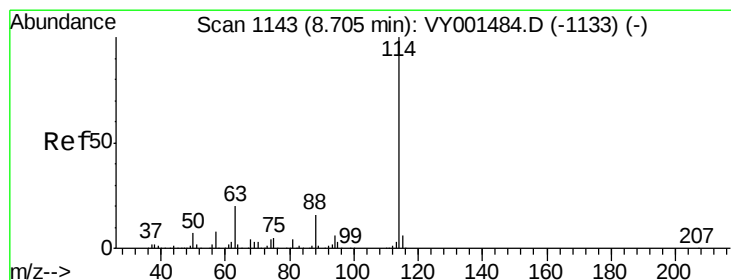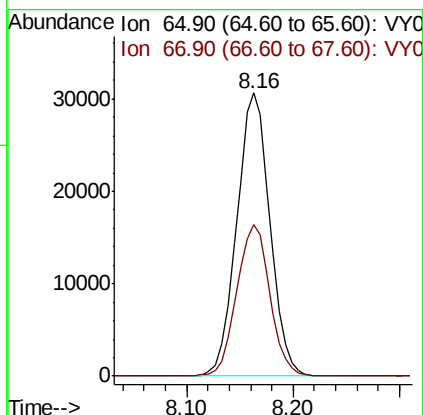

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.71 min Scan# 1143
 Delta R.T. 0.00 min
 Lab File: VY001496.D
 Acq: 04 Feb 2020 18:50

Tgt Ion: 114 Resp: 214556
 Ion Ratio Lower Upper
 114 100
 63 20.1 0.0 39.8
 88 15.9 0.0 32.6


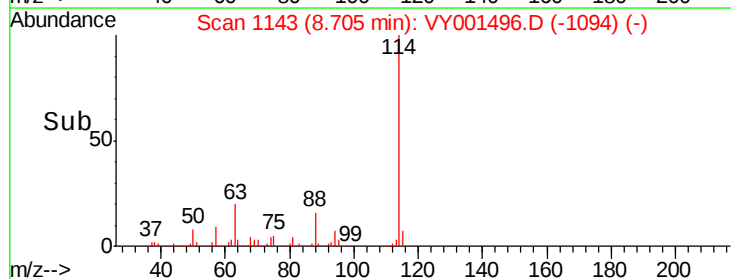
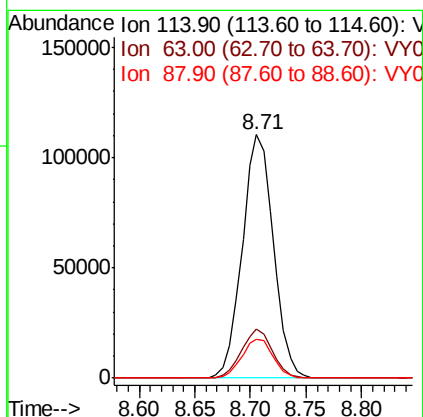
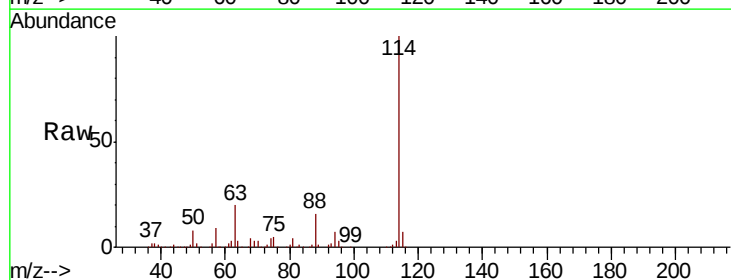




#35
 Dibromofluoromethane
 Concen: 52.317 ug/l
 RT: 7.74 min Scan# 985
 Delta R.T. 0.00 min
 Lab File: VY001496.D
 Acq: 04 Feb 2020 18:50




Instrument :
 MSVOA_Y
 ClientSampleId :
 628-629


Tot Ion:113 Resp: 64728
 Ion Ratio Lower Upper
 113 100
 111 102.3 82.9 124.3
 192 18.4 14.6 22.0

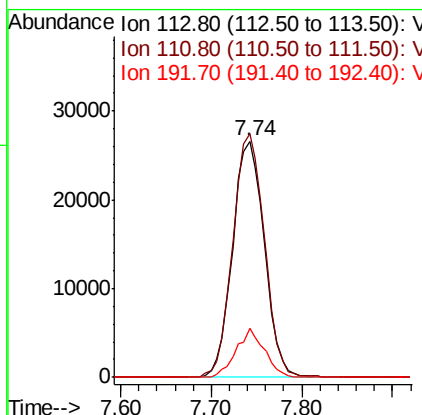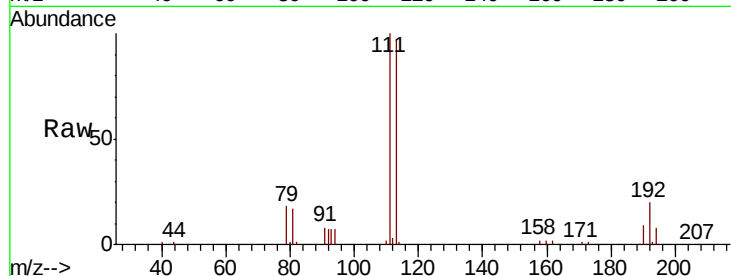

#36
 1,1-Dichloropropene
 Concen: 5.072 ug/l
 RT: 7.81 min Scan# 996
 Delta R.T. -0.13 min
 Lab File: VY001496.D
 Acq: 04 Feb 2020 18:50

Tgt Ion: 75 Resp: 9956
 Ion Ratio Lower Upper
 75 100
 110 8.4 18.2 54.6#
 77 0.0 25.0 37.4#

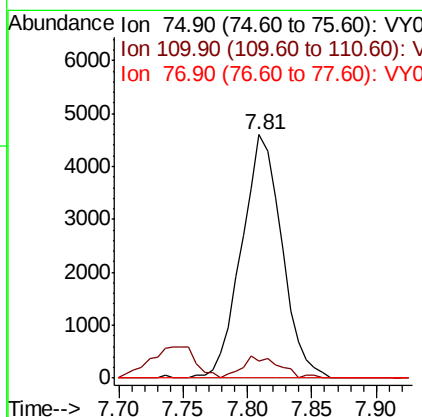

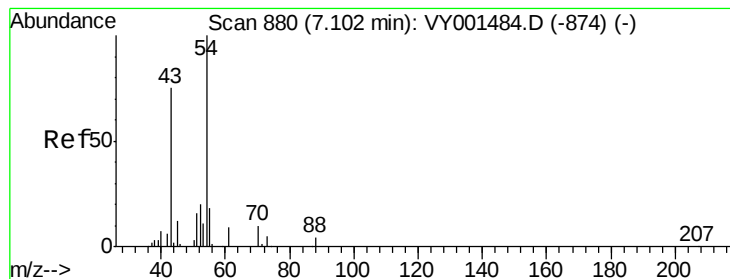

#37

Ethyl Acetate

Concen: 4.856 ug/l

RT: 7.00 min Scan# 864

Delta R.T. -0.10 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50

Instrument :

MSVOA_Y

ClientSampleId :

628-629


Tot Ion: 43 Resp: 4614

Ion Ratio Lower Upper

43 100

61 24.0 12.0 18.0#




70 0.6 10.2 15.4#



Abundance Ion 43.00 (42.70 to 43.70): VY001496.D (-864) (-)

Ion 60.90 (60.60 to 61.60): VY001496.D (-864) (-)

Ion 70.00 (69.70 to 70.70): VY001496.D (-864) (-)

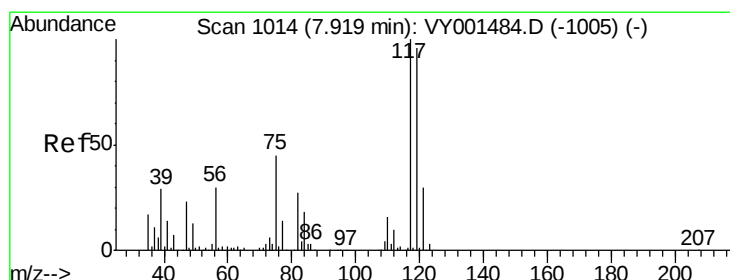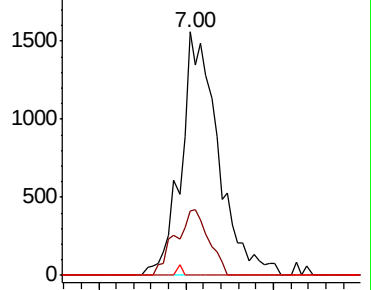

#38

Carbon Tetrachloride

Concen: 6.504 ug/l

RT: 7.81 min Scan# 996

Delta R.T. -0.11 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50


Tgt Ion: 117 Resp: 12351

Ion Ratio Lower Upper

117 100

119 5.5 76.4 114.6#



121 0.0 24.2 36.4#




Abundance Ion 116.80 (116.50 to 117.50): VY001496.D (-965) (-)

Ion 118.80 (118.50 to 119.50): VY001496.D (-965) (-)

Ion 120.80 (120.50 to 121.50): VY001496.D (-965) (-)

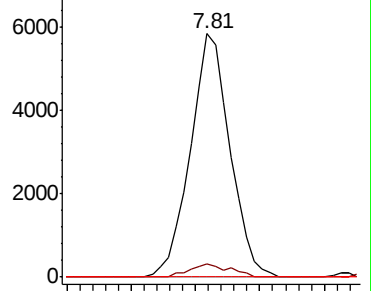

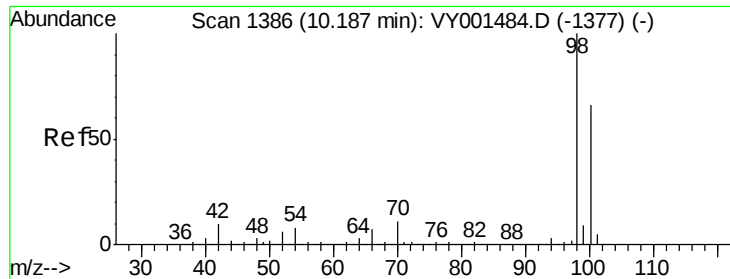

#50

Toluene-d8

Concen: 50.237 ug/l

RT: 10.19 min Scan# 1386

Delta R.T. 0.00 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50

Instrument :

MSVOA_Y

ClientSampleId :


628-629

Tot Ion: 98 Resp: 235159

Ion Ratio Lower Upper




98 100

100 65.8 53.0 79.6

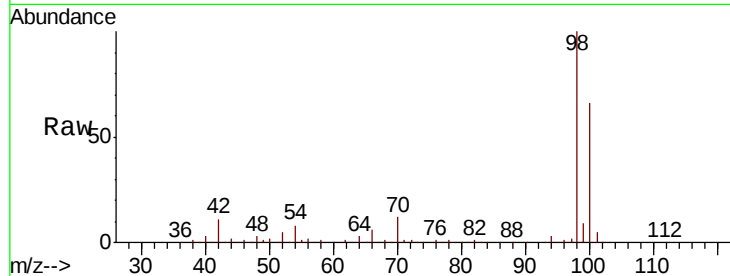

Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY

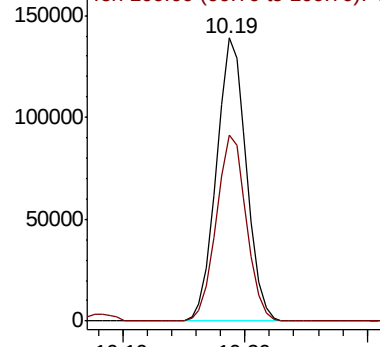

#51

4-Methyl-2-Pentanone

Concen: 33.693 ug/l

RT: 10.08 min Scan# 1369

Delta R.T. 0.00 min

Lab File: VY001496.D


Acq: 04 Feb 2020 18:50

Tgt Ion: 43 Resp: 31216

Ion Ratio Lower Upper



43 100


58 40.6 33.9 50.9



Abundance Ion 43.00 (42.70 to 43.70): VY0

Ion 58.00 (57.70 to 58.70): VY0

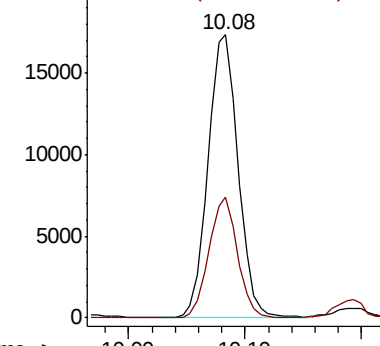

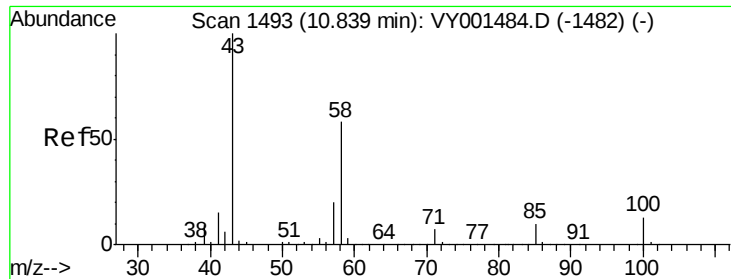

#59

2-Hexanone

Concen: 1.639 ug/l

RT: 10.85 min Scan# 1494

Delta R.T. 0.01 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50

Instrument :

MSVOA_Y

ClientSampled :





628-629

Tot Ion: 43 Resp: 1104

Ion Ratio Lower Upper

43 100

58 38.7 29.0 87.0

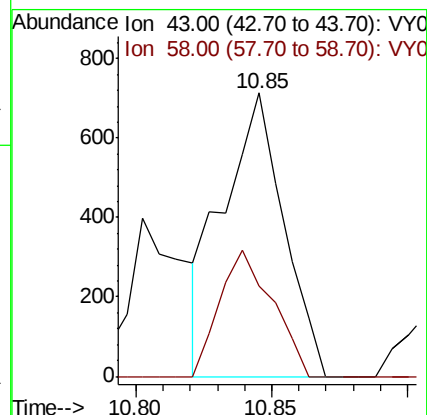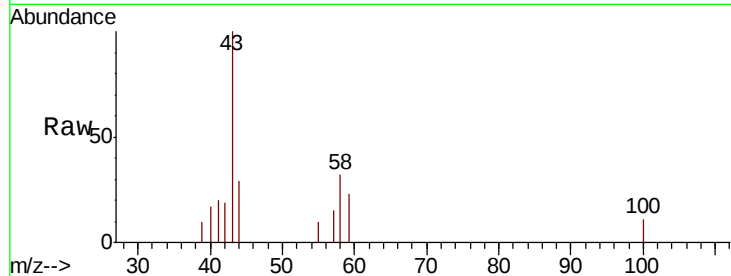

#62

4-Bromofluorobenzene

Concen: 37.867 ug/l

RT: 12.49 min Scan# 1763

Delta R.T. 0.00 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50




Tgt Ion: 95 Resp: 69829


Ion Ratio Lower Upper

95 100

174 72.6 0.0 141.4

176 68.7 0.0 135.4

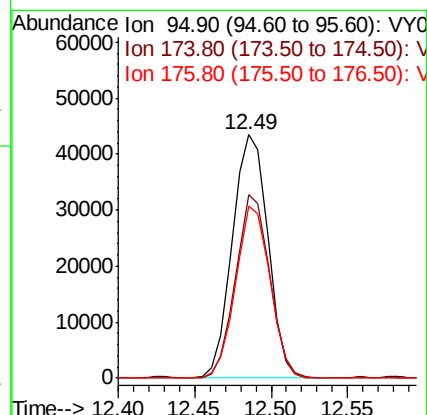


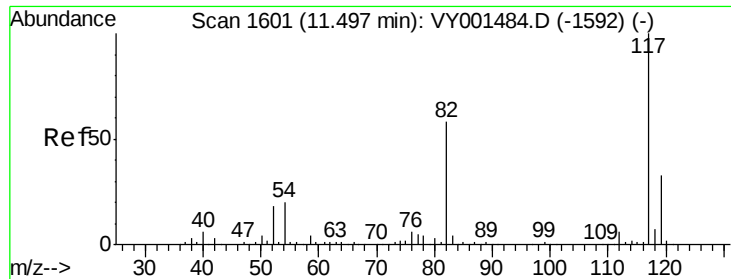




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1601
Delta R.T. 0.00 min
Lab File: VY001496.D
Acq: 04 Feb 2020 18:50

Instrument :
MSVOA_Y
ClientSampled :
628-629

Tot Ion:117 Resp: 165488
Ion Ratio Lower Upper
117 100
82 56.3 46.1 69.1
119 32.4 26.1 39.1

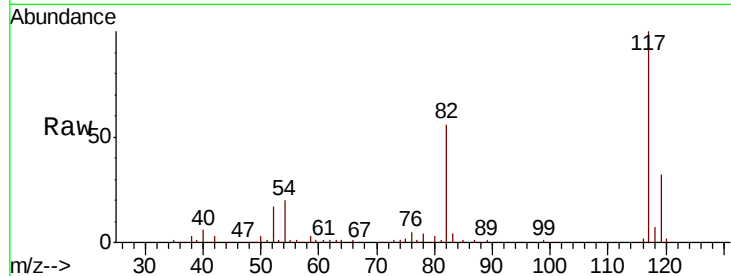


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

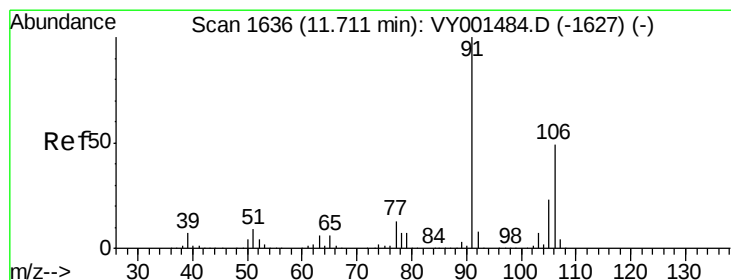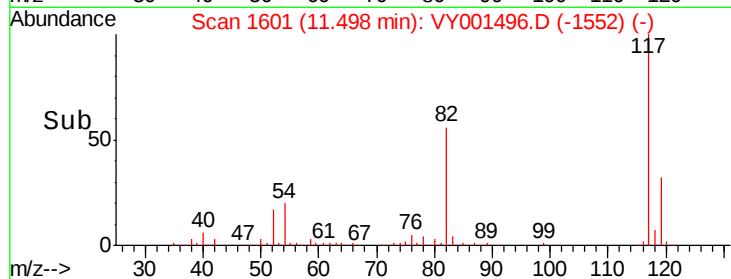
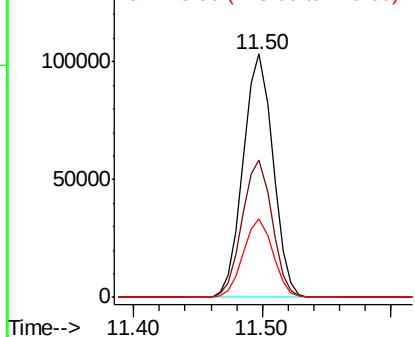



#68
m/p-Xylenes
Concen: 2.458 ug/l
RT: 11.70 min Scan# 1635
Delta R.T. -0.01 min
Lab File: VY001496.D
Acq: 04 Feb 2020 18:50

Tgt Ion:106 Resp: 5543
Ion Ratio Lower Upper
106 100
91 207.9 163.6 245.4



Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VY0



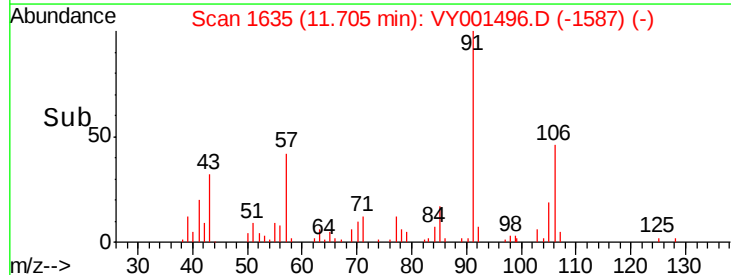
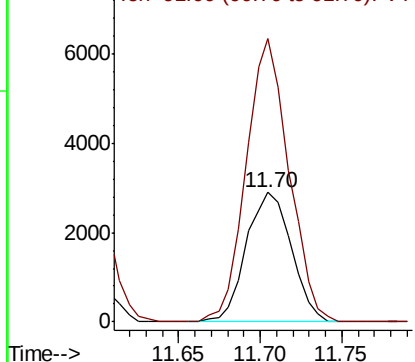


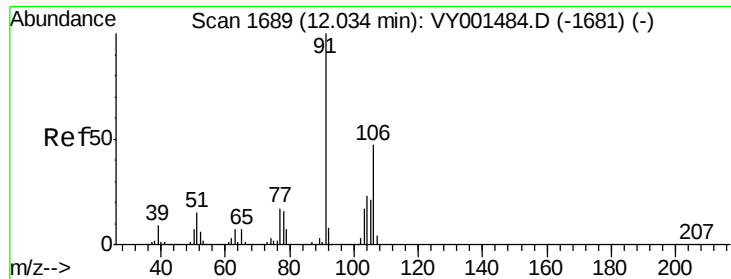

#69
o-Xylene
Concen: 1.612 ug/l
RT: 12.03 min Scan# 1689
Delta R.T. 0.00 min
Lab File: VY001496.D
Acq: 04 Feb 2020 18:50




Instrument :
MSVOA_Y
ClientSampled :
628-629


Tot Ion:106 Resp: 3427
Ion Ratio Lower Upper
106 100
91 204.7 106.0 318.0

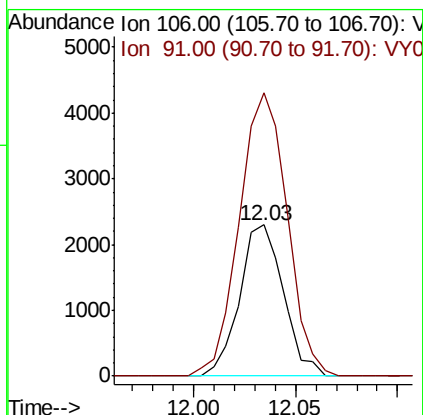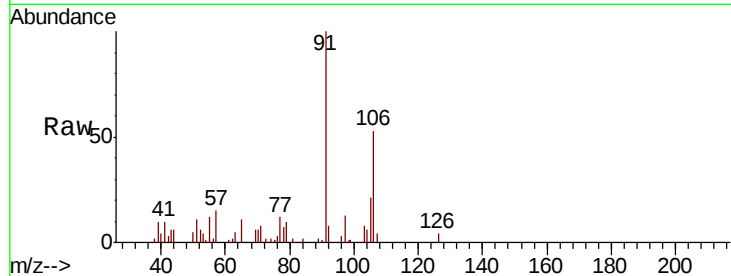

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.43 min Scan# 1918
Delta R.T. 0.00 min
Lab File: VY001496.D
Acq: 04 Feb 2020 18:50

Tgt Ion:152 Resp: 47568
Ion Ratio Lower Upper
152 100
115 63.2 31.4 94.3
150 157.4 0.0 346.8

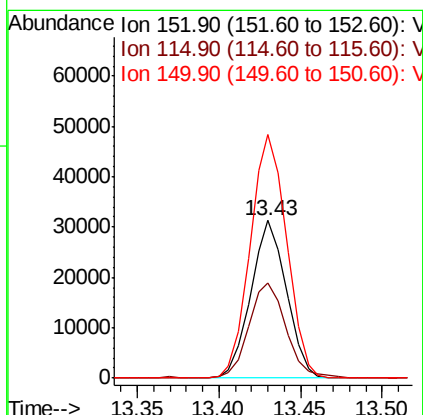



#74

N-amvl acetate

Concen: 5.039 ug/l

RT: 12.12 min Scan# 1703

Delta R.T. -0.03 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50

Instrument :

MSVOA_Y

ClientSampleId :

628-629

Tot Ion: 43 Resp: 4750


Ion Ratio Lower Upper

43 100

70 4.7 37.2 55.8#

55 0.0 18.8 28.2#

61 0.0 21.4 32.2#



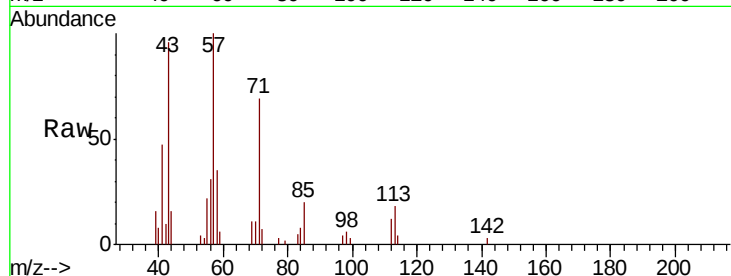


Abundance Ion 43.00 (42.70 to 43.70): VY0

Ion 70.00 (69.70 to 70.70): VY0

Ion 55.00 (54.70 to 55.70): VY0

Ion 61.00 (60.70 to 61.70): VY0

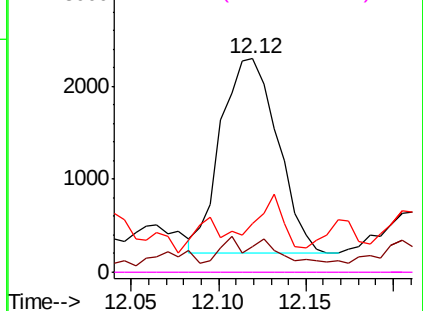

#75

1,1,2,2-Tetrachloroethane

Concen: 1.029 ug/l

RT: 12.55 min Scan# 1774

Delta R.T. -0.04 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50


Tgt Ion: 83 Resp: 709

Ion Ratio Lower Upper

83 100

131 0.0 5.4 16.2#



85 0.0 32.0 96.0#




Abundance Ion 82.90 (82.60 to 83.60): VY0

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): VY0

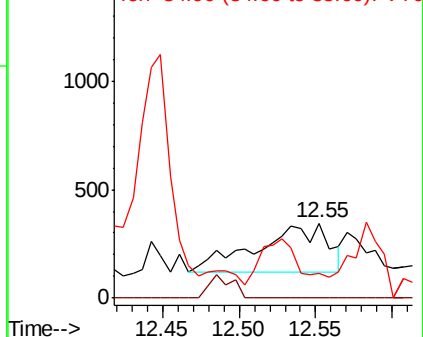

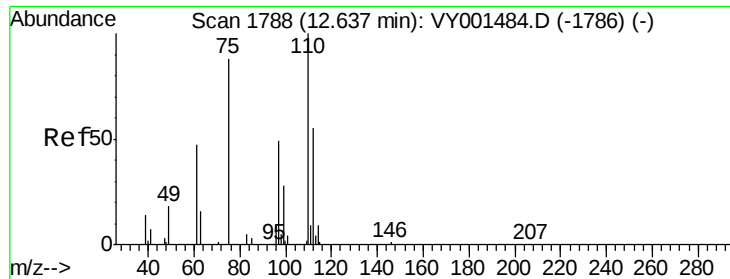

#76

1,2,3-Trichloropropane

Concen: 67.255 ug/l

RT: 12.49 min Scan# 1763

Delta R.T. -0.15 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50

Instrument :

MSVOA_Y

ClientSampleId :


628-629

Tot Ion: 75 Resp: 34404

Ion Ratio Lower Upper

75 100

77 1.4 0.0 0.0#

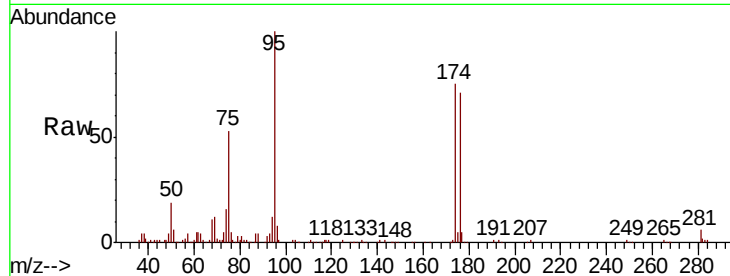

Abundance Ion 74.90 (74.60 to 75.60): VY0

Ion 77.00 (76.70 to 77.70): VY0

12.49

25000

20000

15000



10000

5000

0

Time-->

12.40 12.45 12.50 12.55



#78

n-propylbenzene

Concen: 2.069 ug/l

RT: 12.67 min Scan# 1794

Delta R.T. 0.00 min

Lab File: VY001496.D


Acq: 04 Feb 2020 18:50

Tgt Ion: 91 Resp: 8984

Ion Ratio Lower Upper

91 100

120 23.5 11.4 34.2



Abundance Ion 91.00 (90.70 to 91.70): VY0

Ion 120.00 (119.70 to 120.70): V

12.67

6000


4000


2000

0

Time-->

12.60 12.65 12.70





#80

1,3,5-Trimethylbenzene

Concen: 3.182 ug/l

RT: 12.81 min Scan# 1817

Delta R.T. -0.01 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50

Instrument :

MSVOA_Y

ClientSampleId :


628-629

Tot Ion:105 Resp: 9721

Ion Ratio Lower Upper

105 100

120 50.5 24.1 72.2

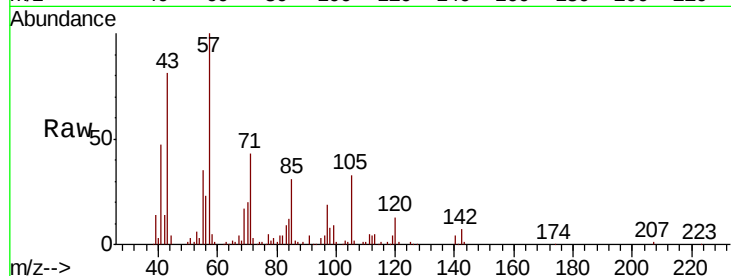

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

8000

6000

4000

2000



0

12.80

12.81

12.85

Time-->



#81

trans-1,4-Dichloro-2-butene

Concen: 130.135 ug/l

RT: 12.49 min Scan# 1763

Delta R.T. 0.10 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50


Tgt Ion: 75 Resp: 34404

Ion Ratio Lower Upper

75 100

53 0.5 67.7 101.5#

89 0.1 34.6 52.0#



Abundance Ion 74.90 (74.60 to 75.60): VY0

Ion 53.00 (52.70 to 53.70): VY0

Ion 88.90 (88.60 to 89.60): VY0

30000

25000

20000

15000

10000

5000

0


12.40


12.45

12.49

12.55

Time-->









#84
1,2,4-Trimethylbenzene
Concen: 13.691 ug/l
RT: 13.13 min Scan# 1868
Delta R.T. 0.00 min
Lab File: VY001496.D
Acq: 04 Feb 2020 18:50




Instrument :
MSVOA_Y
ClientSampleId :
628-629


Tot Ion:105 Resp: 41401
Ion Ratio Lower Upper
105 100
120 46.7 22.4 67.0

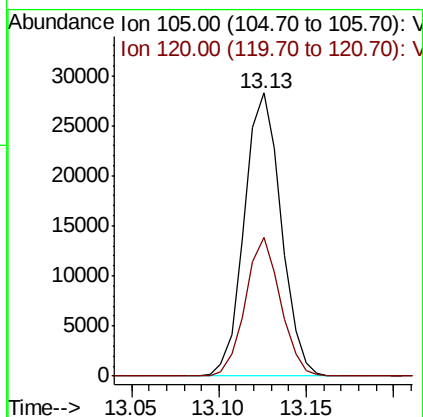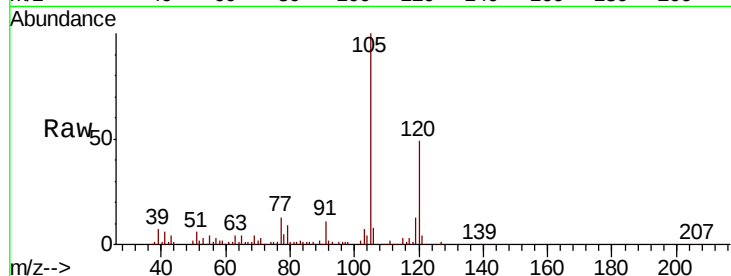

#85
sec-Butylbenzene
Concen: 1.746 ug/l
RT: 13.26 min Scan# 1890
Delta R.T. 0.00 min
Lab File: VY001496.D
Acq: 04 Feb 2020 18:50

Tgt Ion:105 Resp: 6340
Ion Ratio Lower Upper
105 100
134 24.7 10.0 29.8



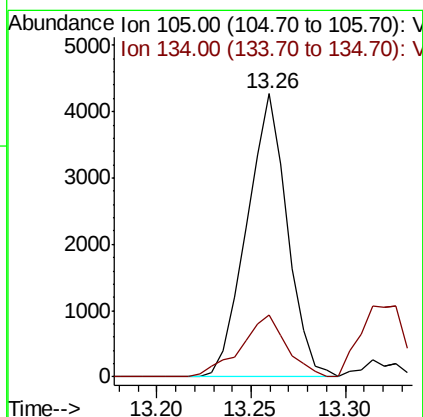





#86
 p-Isopropyltoluene
 Concen: 1.209 ug/l
 RT: 13.38 min Scan# 1909
 Delta R.T. 0.00 min
 Lab File: VY001496.D
 Acq: 04 Feb 2020 18:50




Instrument :
 MSVOA_Y
 ClientSampleId :
 628-629


Tot Ion	Ratio	Lower	Upper
119	100		
134	27.1	13.3	39.8
91	27.8	12.2	36.6

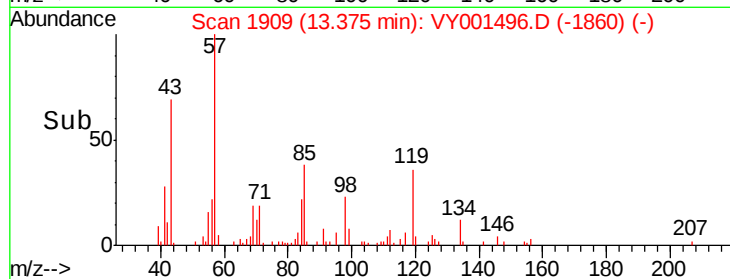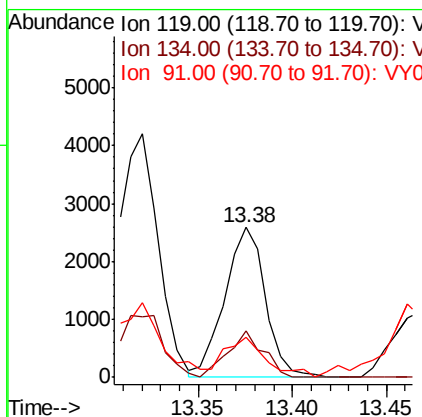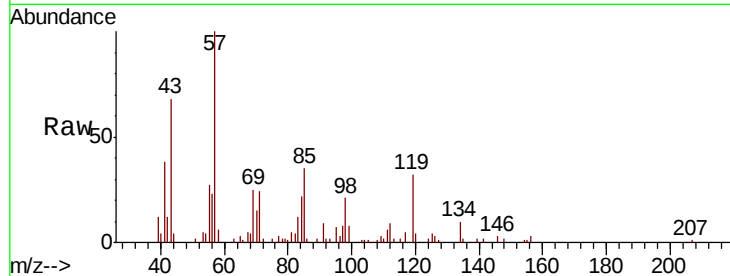

#89
 n-Butylbenzene
 Concen: 4.655 ug/l
 RT: 13.70 min Scan# 1963
 Delta R.T. 0.00 min
 Lab File: VY001496.D
 Acq: 04 Feb 2020 18:50

Tgt Ion	Ratio	Lower	Upper
91	100		
92	45.3	27.3	81.9
134	0.0	13.0	38.9#

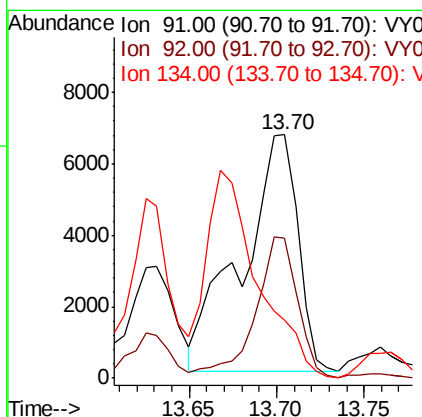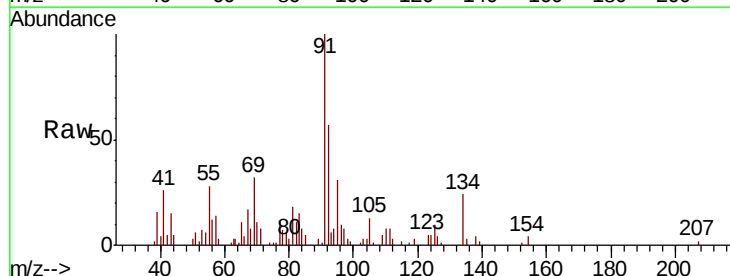



#90

Hexachloroethane

Concen: 3.594 ug/l

RT: 13.97 min Scan# 2007

Delta R.T. 0.01 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50

Instrument :

MSVOA_Y

ClientSampleId :


628-629

Tot Ion:117 Resp: 2207

Ion Ratio Lower Upper




117 100

201 0.0 34.1 102.3#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

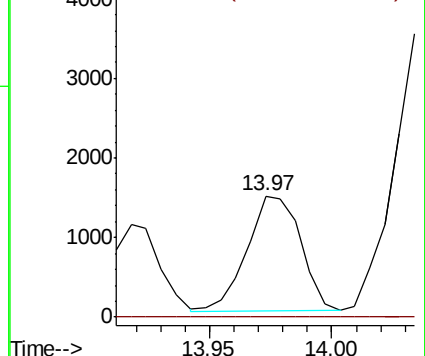

#92

1,2-Dibromo-3-Chloropropane

Concen: 1.635 ug/l

RT: 14.34 min Scan# 2067

Delta R.T. -0.02 min

Lab File: VY001496.D

Acq: 04 Feb 2020 18:50


Tgt Ion: 75 Resp: 208

Ion Ratio Lower Upper

75 100

155 0.0 40.7 122.1#



157 0.0 52.3 157.1#




Abundance Ion 74.90 (74.60 to 75.60): VY0

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V

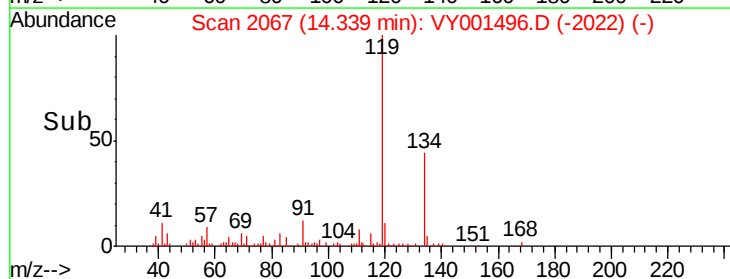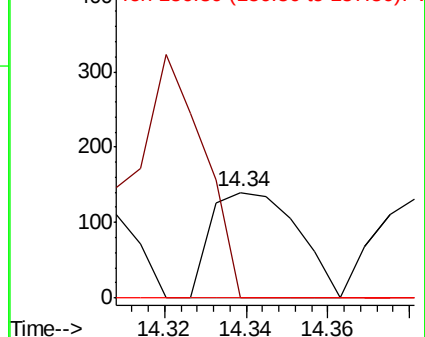




#95
Naphthalene
Concen: 7.070 ug/l
RT: 15.24 min Scan# 2215
Delta R.T. 0.00 min
Lab File: VY001496.D
Acq: 04 Feb 2020 18:50

Instrument :
MSVOA_Y
ClientSampleId :
628-629

Tot Ion	Ratio	Lower	Upper
128	100		
127	20.6	10.1	15.1#
129	16.2	8.9	13.3#

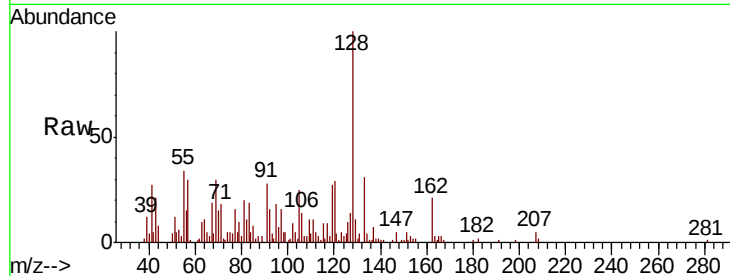

Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

