
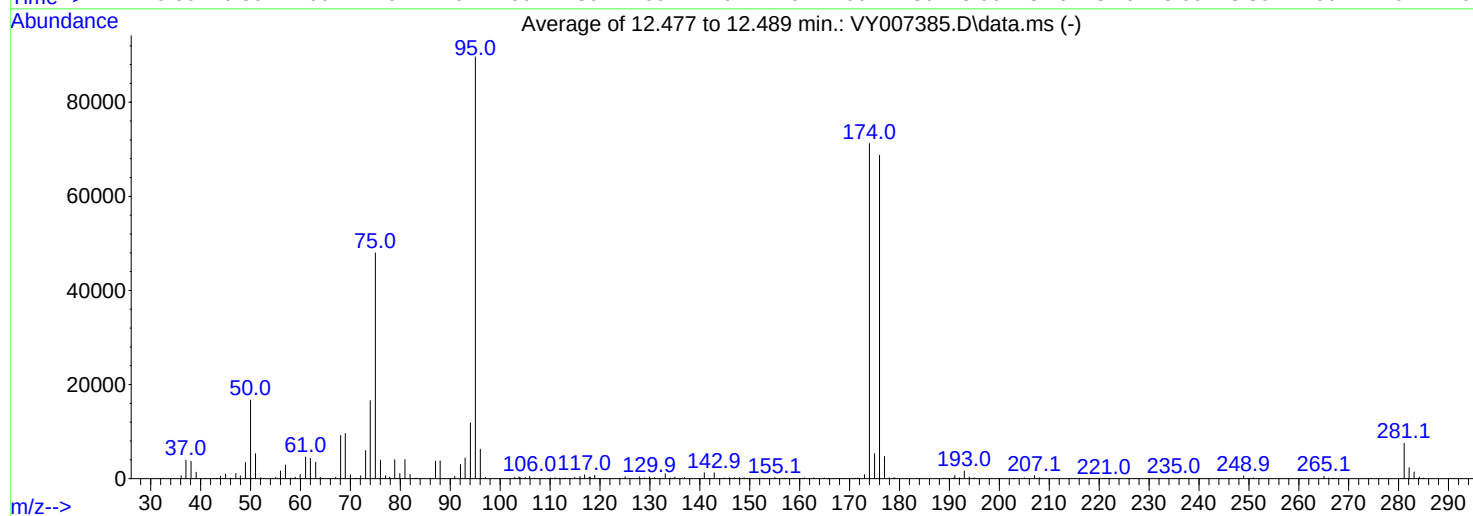


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020422\
 Data File : VY007385.D
 Acq On : 04 Feb 2022 09:31
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020222S.M
 Title : SW846 8260
 Last Update : Thu Feb 03 04:36:48 2022

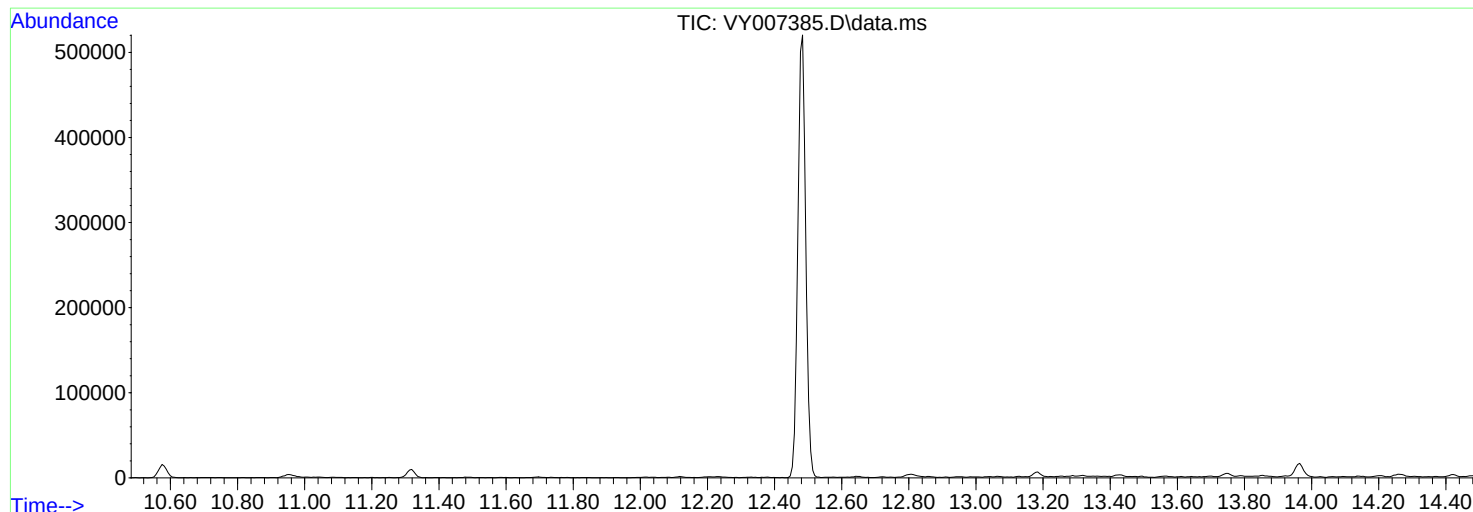

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	16702	PASS
75	95	30	60	53.5	47987	PASS
95	95	100	100	100.0	89648	PASS
96	95	5	9	7.0	6252	PASS
173	174	0.00	2	1.2	847	PASS
174	95	50	100	79.4	71211	PASS
175	174	5	9	7.4	5295	PASS
176	174	95	101	96.5	68723	PASS
177	176	5	9	6.9	4731	PASS