
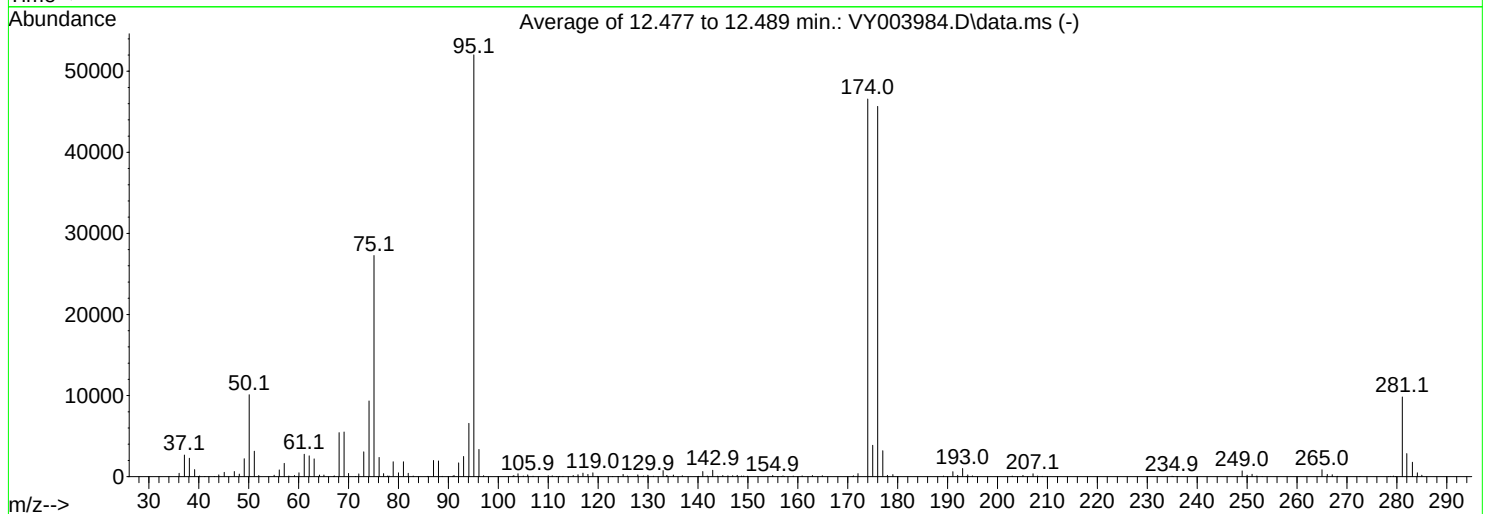


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020521\
 Data File : VY003984.D
 Acq On : 05 Feb 2021 09:39
 Operator : SY/MD
 Sample : BFB98
 Misc : 5.00g/10mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB980

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\SFAMYL012621SMA.M
 Title : VOC Analysis
 Last Update : Sat Feb 06 03:42:14 2021

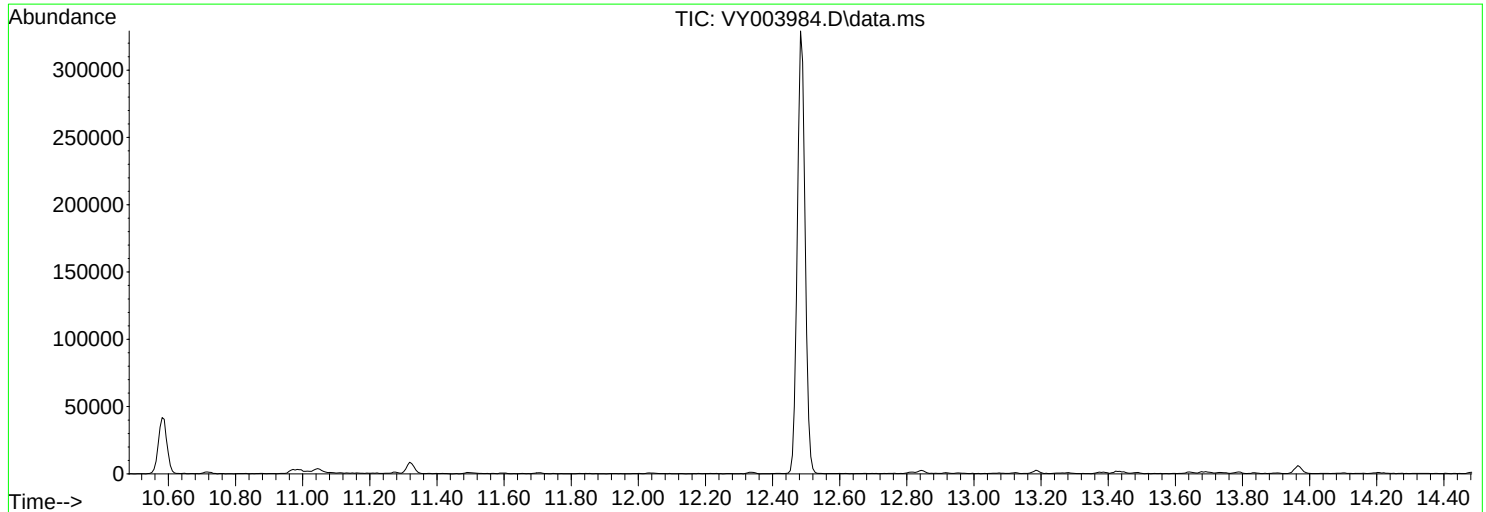

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	10103	PASS
75	95	30	80	52.4	27269	PASS
95	95	100	100	100.0	52021	PASS
96	95	5	9	6.5	3364	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.5	46576	PASS
175	174	5	9	8.3	3867	PASS
176	174	95	105	98.0	45656	PASS
177	176	5	10	7.0	3199	PASS

m/z	Abundance
44.00	107.0
207.10	113.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB980

m/z	Abundance
36.10	470.0
37.10	2411.0
38.10	2256.0
39.10	877.0
39.90	73.0
40.30	62.0
44.00	345.0
45.10	533.0
47.10	479.0
48.10	428.0
49.10	2219.0
50.10	9656.0
51.10	2914.0
52.00	107.0
55.10	227.0
56.10	742.0
57.10	1637.0
58.00	94.0
59.10	92.0
60.10	571.0
61.10	2818.0
62.10	2461.0
63.10	2024.0
64.10	226.0
65.20	211.0
67.00	143.0
68.10	4947.0
69.10	5102.0
70.00	427.0
72.10	241.0
73.10	2394.0
74.10	8576.0
75.10	24648.0
76.10	2289.0
77.00	405.0
79.00	1746.0
80.00	479.0
81.00	1675.0
82.00	356.0
87.00	1683.0
88.00	1752.0
88.70	57.0
90.90	208.0
92.00	1505.0
93.00	2265.0
94.10	5830.0
95.10	47104.0
96.10	2787.0
97.00	131.0
102.90	152.0
103.90	342.0
105.90	156.0
110.00	60.0
110.90	54.0
115.10	186.0
116.00	195.0
117.00	447.0
118.00	265.0
118.90	398.0
119.90	53.0
124.90	115.0
128.00	219.0
128.80	82.0
129.90	148.0
133.00	435.0
133.60	70.0
135.00	186.0
136.90	99.0
140.10	98.0
141.00	638.0
141.90	87.0
143.00	688.0
144.00	53.0
144.90	193.0
146.00	76.0
146.90	61.0
147.90	108.0
149.10	75.0
149.90	77.0
154.90	137.0
156.70	87.0
157.10	78.0
159.10	73.0
160.90	68.0
162.90	70.0
164.90	74.0
170.90	122.0
172.10	357.0
174.00	37192.0
175.00	3142.0
176.00	36648.0
177.00	2707.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB980

178.10	88.0
179.10	178.0
191.00	251.0
192.10	67.0
193.00	534.0
193.80	141.0
194.90	83.0
207.10	353.0
208.10	84.0
235.20	75.0
248.90	223.0
250.00	109.0
251.00	124.0
265.00	566.0
266.20	125.0
267.10	118.0
278.30	50.0
279.70	75.0
281.00	4277.0
282.00	1371.0
283.10	822.0
284.20	200.0
285.00	54.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB980

m/z	Abundance
36.10	375.0
37.10	3103.0
38.10	2355.0
39.20	987.0
40.10	103.0
43.10	56.0
44.10	333.0
45.10	496.0
47.10	781.0
48.10	259.0
49.10	2436.0
50.10	11680.0
51.10	3736.0
51.90	215.0
55.10	182.0
56.10	1009.0
57.10	1837.0
58.10	91.0
59.20	152.0
60.00	452.0
61.10	3128.0
62.10	2732.0
63.10	2346.0
64.10	199.0
65.00	216.0
67.20	188.0
68.10	6056.0
69.10	6240.0
70.00	491.0
72.00	436.0
73.00	3356.0
74.10	10625.0
75.10	31136.0
76.10	2644.0
77.00	472.0
78.10	220.0
78.90	1928.0
80.00	526.0
81.00	2192.0
81.90	431.0
82.90	86.0
87.00	2255.0
88.00	1879.0
88.80	84.0
91.10	274.0
92.10	2041.0
93.10	2855.0
94.10	7409.0
95.10	59232.0
96.10	4045.0
97.10	99.0
103.10	179.0
103.90	405.0
105.00	148.0
105.90	246.0
106.90	69.0
110.00	141.0
110.80	130.0
111.70	51.0
112.90	59.0
115.00	123.0
116.00	307.0
117.00	439.0
117.90	217.0
119.00	666.0
119.90	67.0
122.90	67.0
124.00	66.0
125.00	301.0
125.80	68.0
128.00	271.0
129.10	85.0
130.00	229.0
131.10	98.0
132.90	712.0
133.70	309.0
135.00	210.0
136.90	144.0
140.90	566.0
141.80	63.0
142.90	847.0
143.90	78.0
145.00	134.0
146.00	80.0
147.00	141.0
147.80	189.0
148.70	113.0
149.20	77.0
149.90	105.0
155.00	194.0
157.00	159.0
159.00	67.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB980

160.90	135.0
162.90	200.0
164.90	88.0
171.10	106.0
172.00	387.0
174.00	53152.0
175.00	4440.0
176.00	50872.0
177.00	3807.0
177.90	204.0
179.10	258.0
189.20	69.0
191.10	741.0
191.90	109.0
193.00	817.0
194.00	231.0
195.00	100.0
203.00	132.0
205.20	93.0
207.10	444.0
208.10	66.0
209.00	50.0
234.90	80.0
249.00	663.0
250.10	159.0
251.00	419.0
252.00	97.0
264.90	669.0
266.00	302.0
266.90	237.0
268.10	102.0
272.60	50.0
279.30	62.0
281.10	9494.0
282.10	2691.0
283.10	1786.0
284.00	471.0
285.10	218.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB980

m/z	Abundance
36.00	431.0
37.10	2507.0
38.10	2193.0
39.10	722.0
40.10	92.0
41.20	73.0
44.10	305.0
45.10	544.0
47.10	642.0
48.10	241.0
49.10	1969.0
50.10	8972.0
51.10	2764.0
52.10	108.0
55.00	124.0
56.10	749.0
57.10	1440.0
58.10	65.0
59.10	166.0
60.00	377.0
61.10	2365.0
62.10	2517.0
63.10	2203.0
64.20	169.0
65.00	153.0
67.10	101.0
68.10	5254.0
69.10	5207.0
70.00	294.0
71.40	59.0
72.00	330.0
73.10	3451.0
74.10	8806.0
75.10	26024.0
76.10	2193.0
77.00	256.0
77.80	243.0
78.90	1812.0
80.00	428.0
81.00	1633.0
81.90	438.0
83.00	136.0
85.90	114.0
87.00	2038.0
88.00	2203.0
91.10	176.0
92.00	1518.0
93.10	2372.0
94.10	6475.0
95.10	49728.0
96.10	3261.0
97.10	116.0
103.10	231.0
104.00	297.0
105.00	106.0
105.90	270.0
107.00	111.0
110.00	95.0
110.70	108.0
112.20	97.0
113.00	67.0
114.90	112.0
115.80	239.0
116.90	446.0
118.00	345.0
118.90	387.0
125.00	430.0
125.90	159.0
127.90	180.0
129.10	177.0
129.90	189.0
131.00	78.0
133.10	1093.0
133.90	256.0
135.10	198.0
136.80	90.0
141.00	691.0
141.90	93.0
143.00	810.0
143.90	73.0
145.00	116.0
146.00	138.0
147.00	137.0
147.80	185.0
148.70	109.0
149.20	83.0
155.00	129.0
156.90	54.0
157.30	58.0
159.00	113.0
160.80	104.0
162.90	178.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB980

164.90	187.0
171.20	180.0
172.00	374.0
174.00	49384.0
175.00	4018.0
176.00	49448.0
177.00	3083.0
177.90	182.0
179.00	315.0
180.00	63.0
189.10	162.0
191.00	825.0
192.00	302.0
193.00	1694.0
194.10	443.0
195.00	140.0
202.90	119.0
205.10	413.0
206.10	58.0
207.10	588.0
208.00	100.0
208.90	68.0
235.00	91.0
236.00	56.0
249.00	1250.0
250.00	276.0
251.00	328.0
251.90	119.0
253.00	88.0
265.00	1289.0
266.00	378.0
267.10	370.0
278.70	95.0
279.30	164.0
281.10	15740.0
282.00	4484.0
283.10	2736.0
284.10	782.0
284.90	282.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB980