

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY020620\
 Data File : VY001529.D
 Acq On : 06 Feb 2020 14:41
 Operator : SY/MD
 Sample : L1360-02RE
 Misc : 16.13G/5ML/MSVOA Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-2RE

Quant Time: Feb 07 04:24:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 04 15:10:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.82	168	166516	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	298114	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	258665	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.43	152	110390	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.16	65	107233	63.96	ug/l	0.00
Spiked Amount			Recovery	=	127.92%	
35) Dibromofluoromethane	7.74	113	89277	51.93	ug/l	0.00
Spiked Amount			Recovery	=	103.86%	
50) Toluene-d8	10.19	98	348730	53.62	ug/l	0.00
Spiked Amount			Recovery	=	107.24%	
62) 4-Bromofluorobenzene	12.49	95	118331	46.18	ug/l	0.00
Spiked Amount			Recovery	=	92.36%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY020620\
Data File : VY001529.D
Acq On : 06 Feb 2020 14:41
Operator : SY/MD
Sample : L1360-02RE
Misc : 16.13G/5ML/MSVOA Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-2RE

Quant Time: Feb 07 04:24:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 04 15:10:08 2020
Response via : Initial Calibration

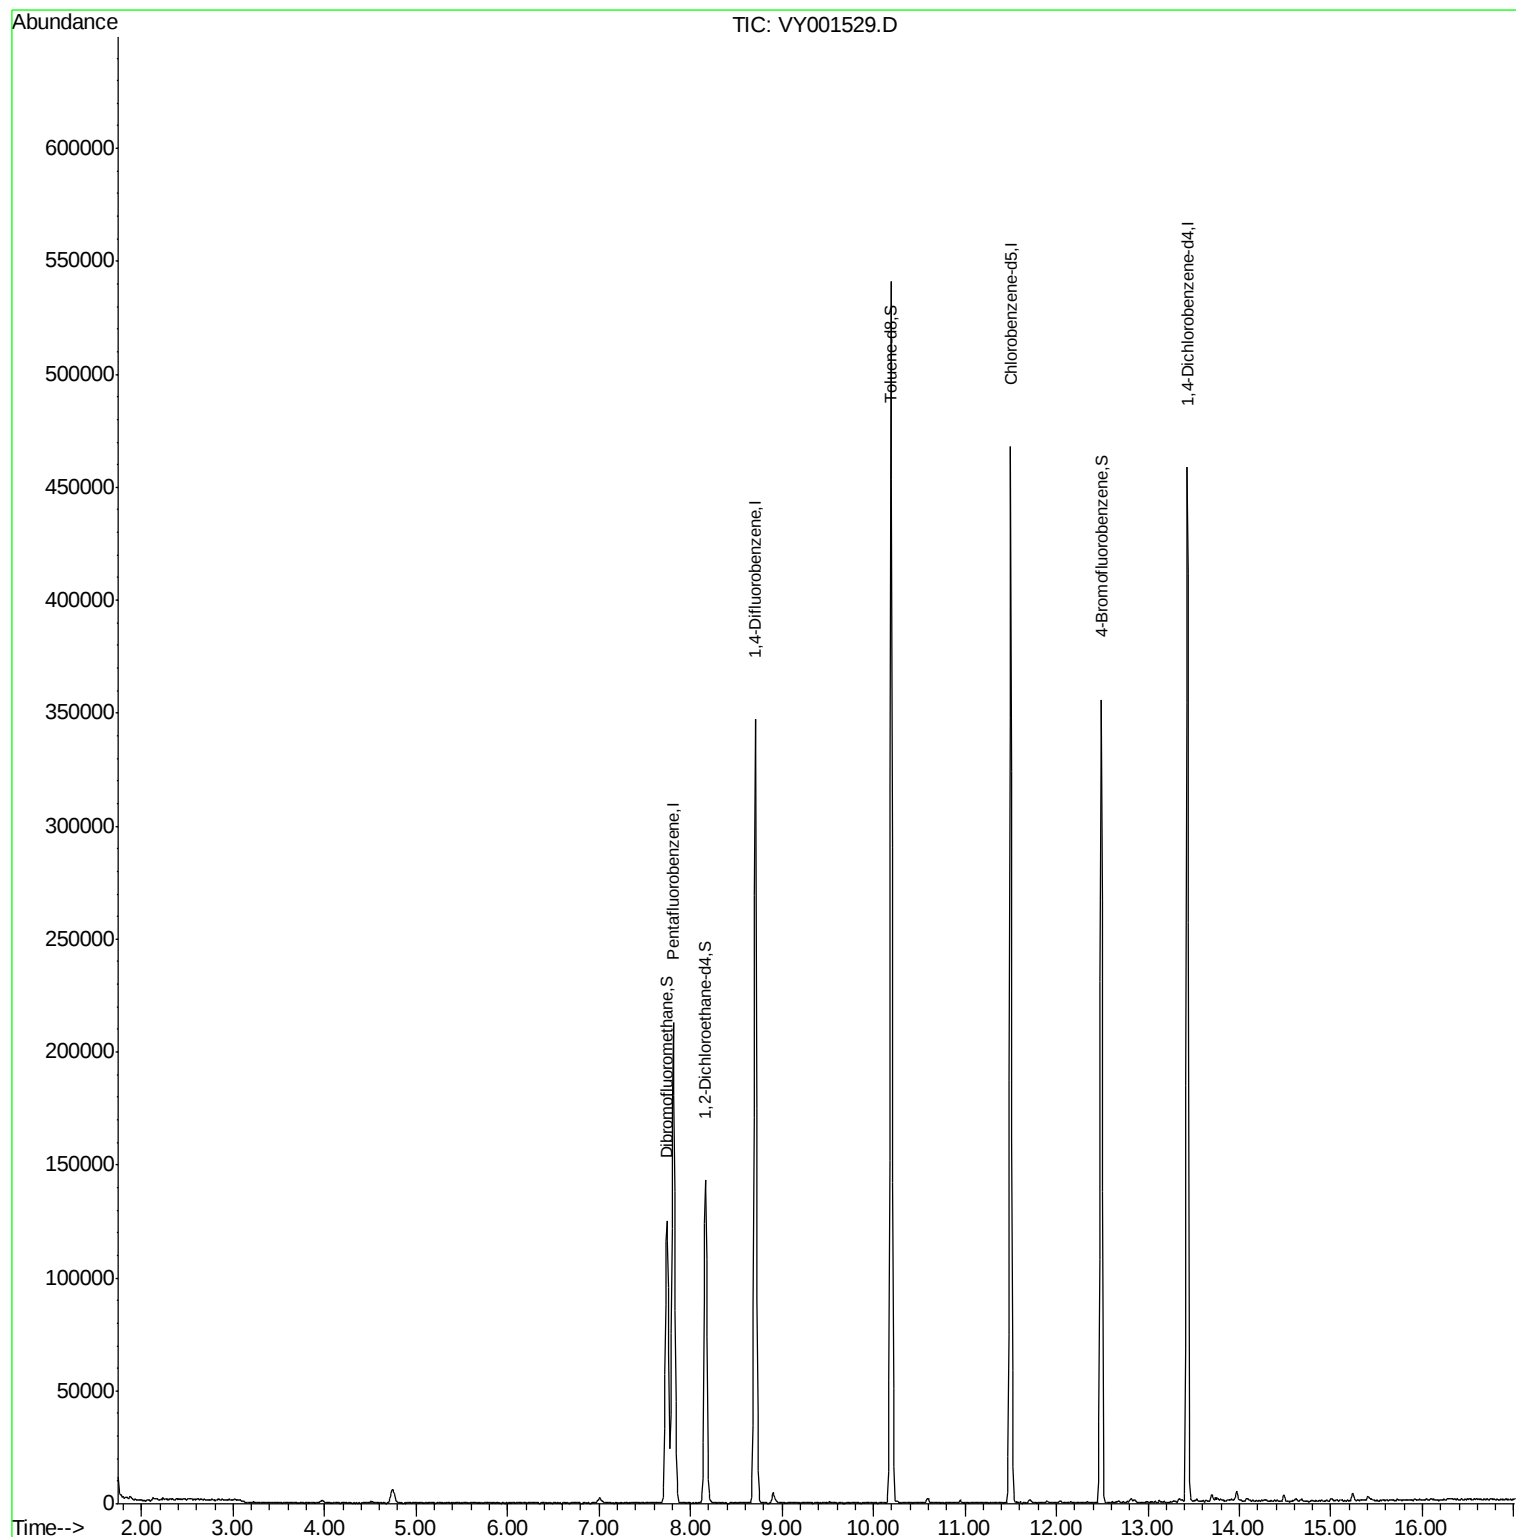

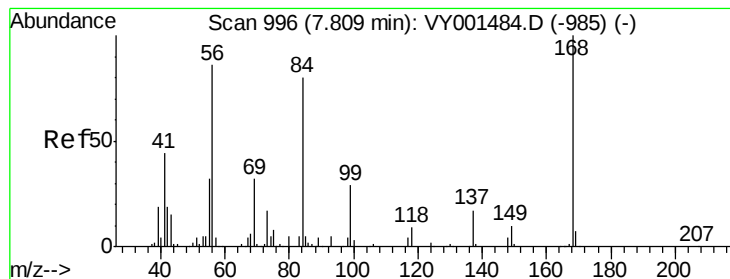

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.82 min Scan# 997

Delta R.T. 0.01 min

Lab File: VY001529.D

Acq: 06 Feb 2020 14:41

Instrument :

MSVOA_Y

ClientSampleId :


TP-2RE

Tot Ion:168 Resp: 166516




Ion Ratio Lower Upper

168 100

99 54.9 48.2 72.4

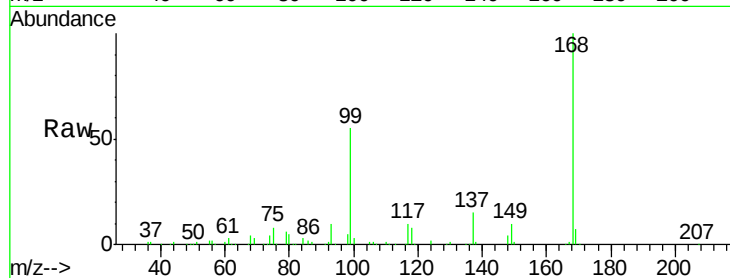

Abundance Ion 167.90 (167.60 to 168.60): VY001529.D (-947) (-)

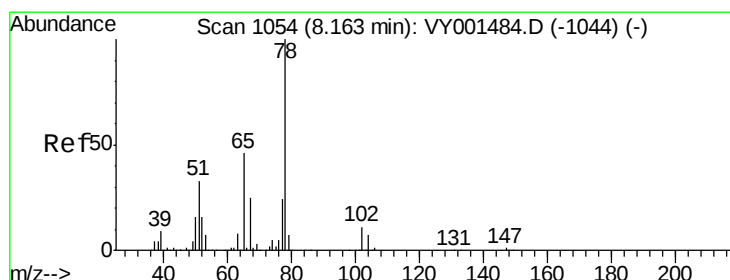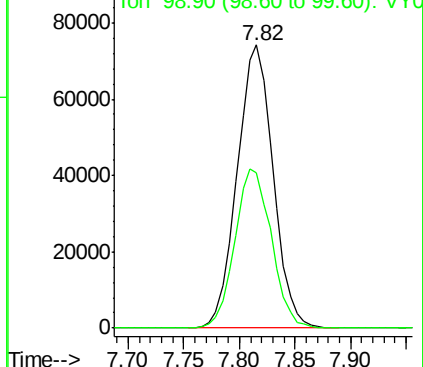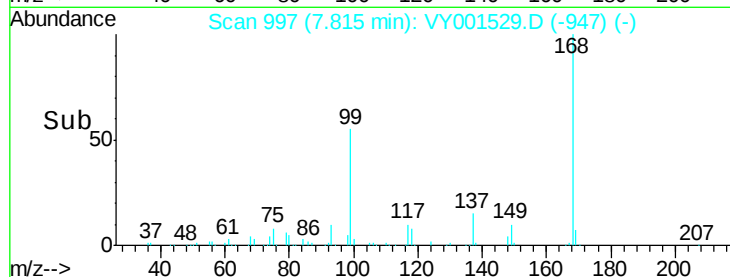

#33

1,2-Dichloroethane-d4

Concen: 63.960 ug/l

RT: 8.16 min Scan# 1054

Delta R.T. 0.00 min

Lab File: VY001529.D


Acq: 06 Feb 2020 14:41

Tgt Ion: 65 Resp: 107233



Ion Ratio Lower Upper


65 100

67 55.3 0.0 108.6

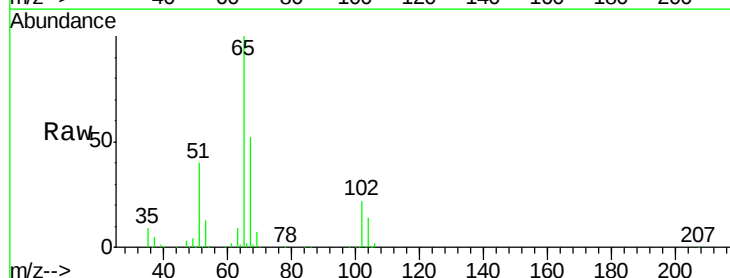

Abundance Ion 64.90 (64.60 to 65.60): VY001529.D (-1005) (-)



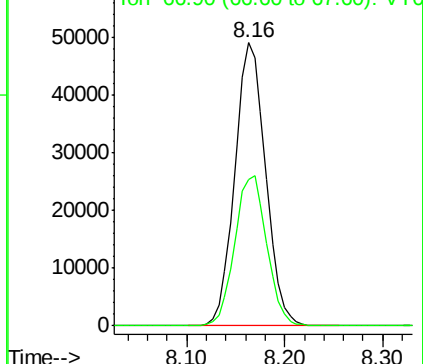
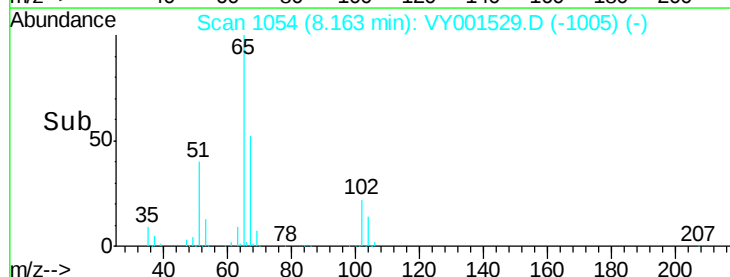


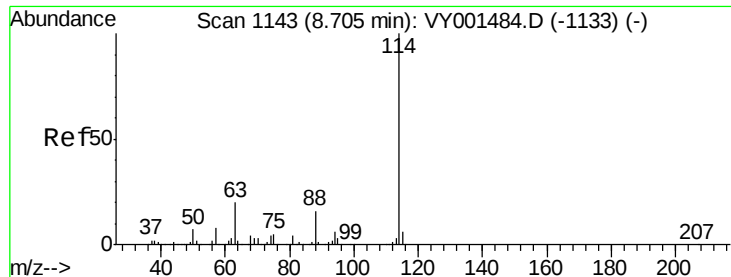

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.71 min Scan# 1144
 Delta R.T. 0.01 min
 Lab File: VY001529.D
 Acq: 06 Feb 2020 14:41




Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-2RE


Tot Ion	Ratio	Lower	Upper
114	100		
63	19.2	0.0	39.8
88	16.0	0.0	32.6

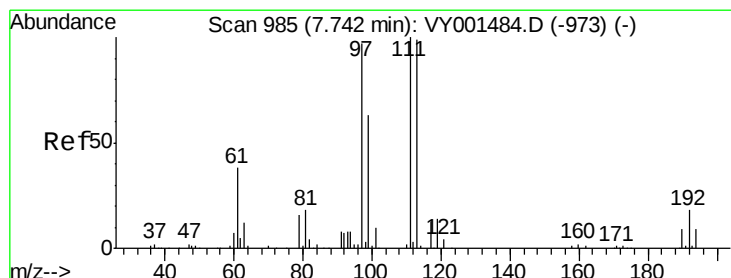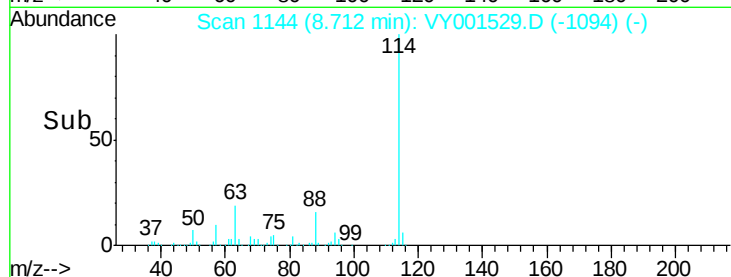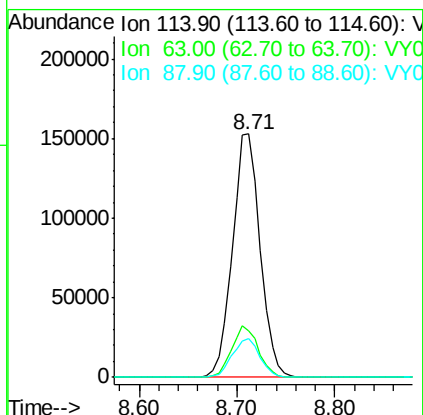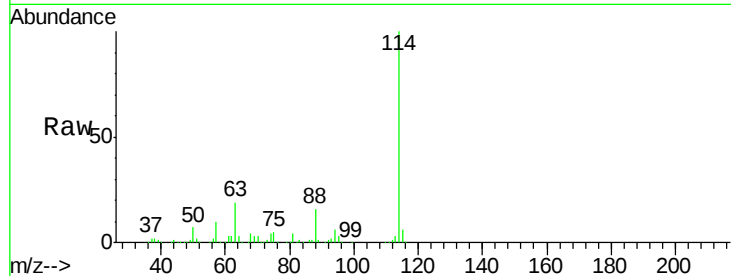

#35
 Dibromofluoromethane
 Concen: 51.933 ug/l
 RT: 7.74 min Scan# 985
 Delta R.T. 0.00 min
 Lab File: VY001529.D
 Acq: 06 Feb 2020 14:41

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.8	82.9	124.3
192	18.7	14.6	22.0

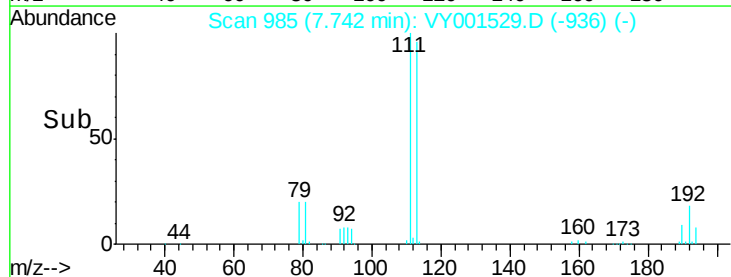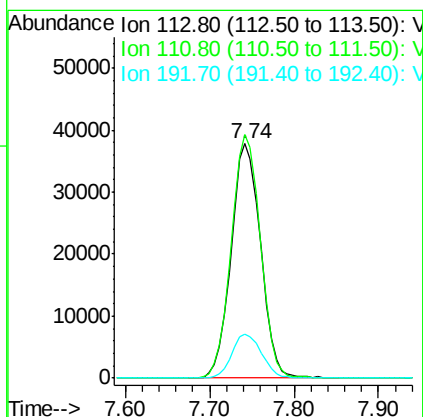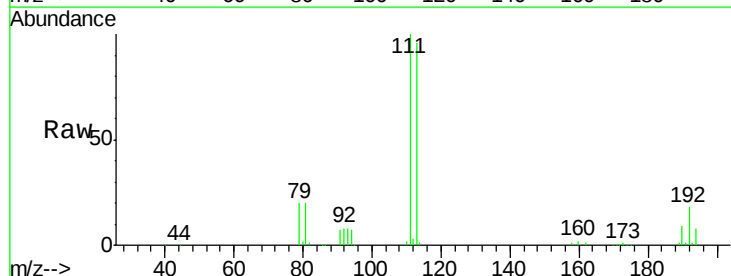

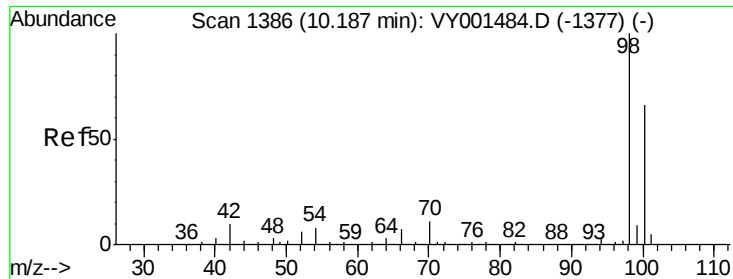

#50

Toluene-d8

Concen: 53.618 ug/l

RT: 10.19 min Scan# 1387

Delta R.T. 0.01 min

Lab File: VY001529.D

Acq: 06 Feb 2020 14:41

Instrument :

MSVOA_Y

ClientSampleId :


TP-2RE

Tot Ion: 98 Resp: 348730

Ion Ratio Lower Upper

98 100

100 65.1 53.0 79.6

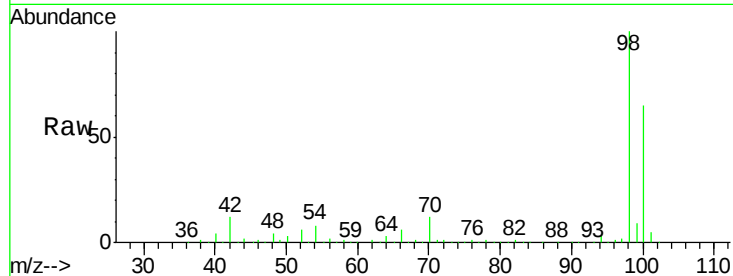

Abundance Ion 98.00 (97.70 to 98.70): VY001484.D (-1377) (-)

Ion 100.00 (99.70 to 100.70): VY001484.D (-1377) (-)

10.19

200000



150000

100000

50000

0

Time-->

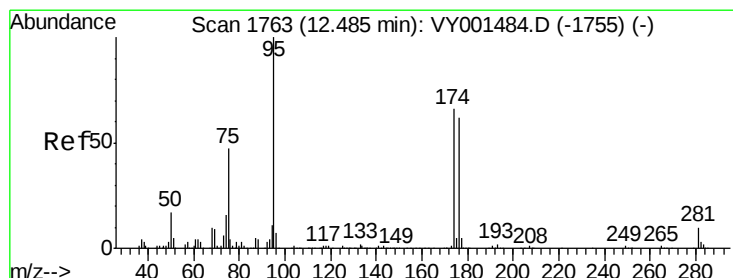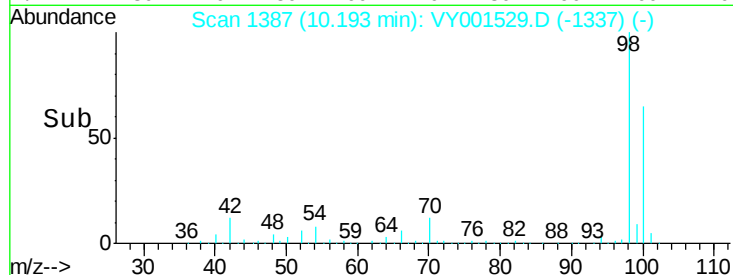

#62

4-Bromofluorobenzene

Concen: 46.183 ug/l

RT: 12.49 min Scan# 1764

Delta R.T. 0.01 min

Lab File: VY001529.D

Acq: 06 Feb 2020 14:41


Tgt Ion: 95 Resp: 118331

Ion Ratio Lower Upper

95 100

174 73.8 0.0 141.4

176 72.9 0.0 135.4

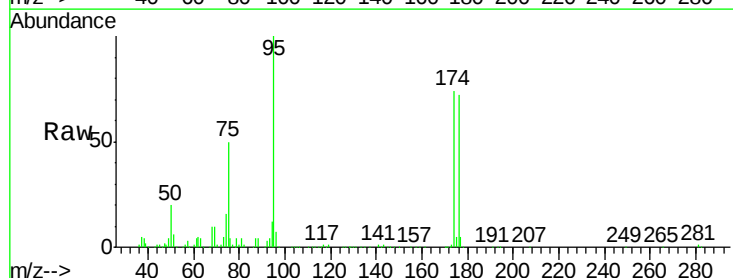

Abundance Ion 94.90 (94.60 to 95.60): VY001484.D (-1755) (-)

Ion 173.80 (173.50 to 174.50): VY001484.D (-1755) (-)

Ion 175.80 (175.50 to 176.50): VY001484.D (-1755) (-)

100000

80000


60000


40000

20000

0

Time-->

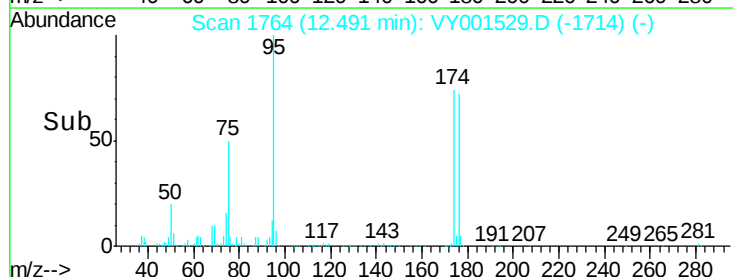


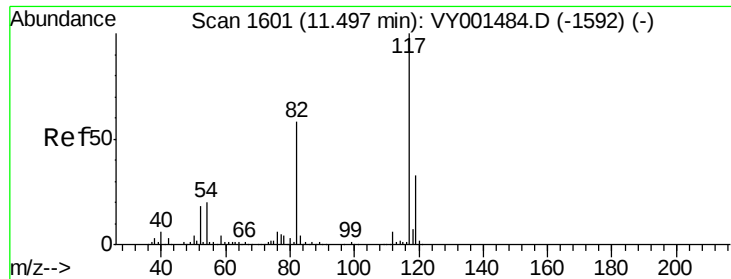




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1602
Delta R.T. 0.01 min
Lab File: VY001529.D
Acq: 06 Feb 2020 14:41

Instrument :
MSVOA_Y
ClientSampled :
TP-2RE

Tot Ion:117 Resp: 258665
Ion Ratio Lower Upper
117 100
82 53.1 46.1 69.1
119 32.0 26.1 39.1

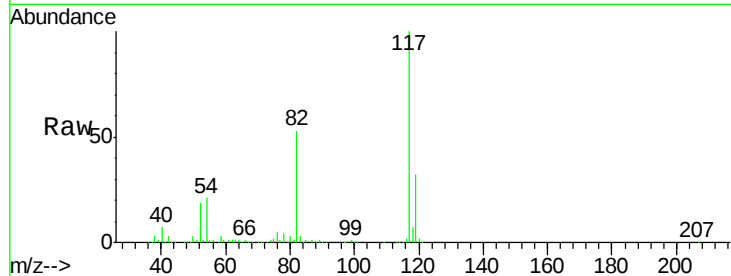


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

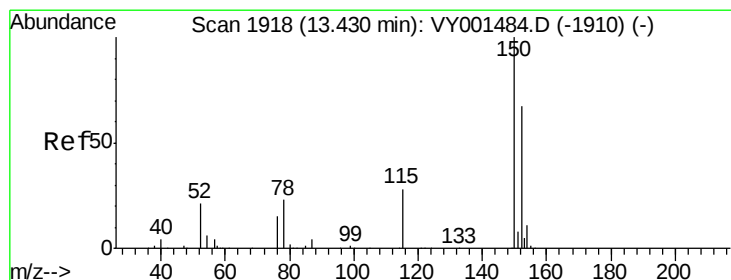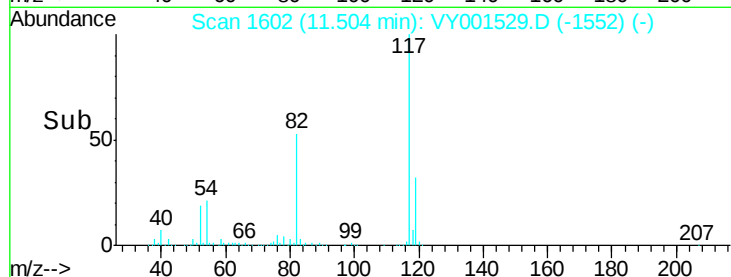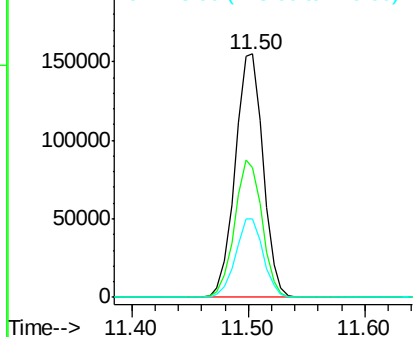

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.43 min Scan# 1918
Delta R.T. 0.00 min
Lab File: VY001529.D
Acq: 06 Feb 2020 14:41

Tgt Ion:152 Resp: 110390
Ion Ratio Lower Upper
152 100
115 59.8 31.4 94.3
150 158.4 0.0 346.8

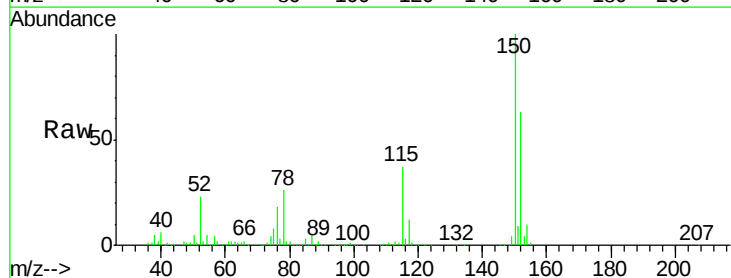

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

