

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020624\
 Data File : VY017271.D
 Acq On : 06 Feb 2024 17:47
 Operator : SY/MD
 Sample : P1358-05
 Misc : 5.06g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RT5149

Quant Time: Feb 07 00:10:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020124S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 02 00:56:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.795	168	74430	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	139836	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	126074	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.434	152	48319	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	43475	65.385	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 130.760%	
35) Dibromofluoromethane	7.722	113	43499	57.613	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 115.220%	
50) Toluene-d8	10.185	98	168799	61.404	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 122.800%	
62) 4-Bromofluorobenzene	12.489	95	53400	59.299	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 118.600%	
Target Compounds						
20) Methylene Chloride	4.722	84	8005	6.988	ug/l	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020624\
Data File : VY017271.D
Acq On : 06 Feb 2024 17:47
Operator : SY/MD
Sample : P1358-05
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RT5149

Quant Time: Feb 07 00:10:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020124S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 02 00:56:04 2024
Response via : Initial Calibration




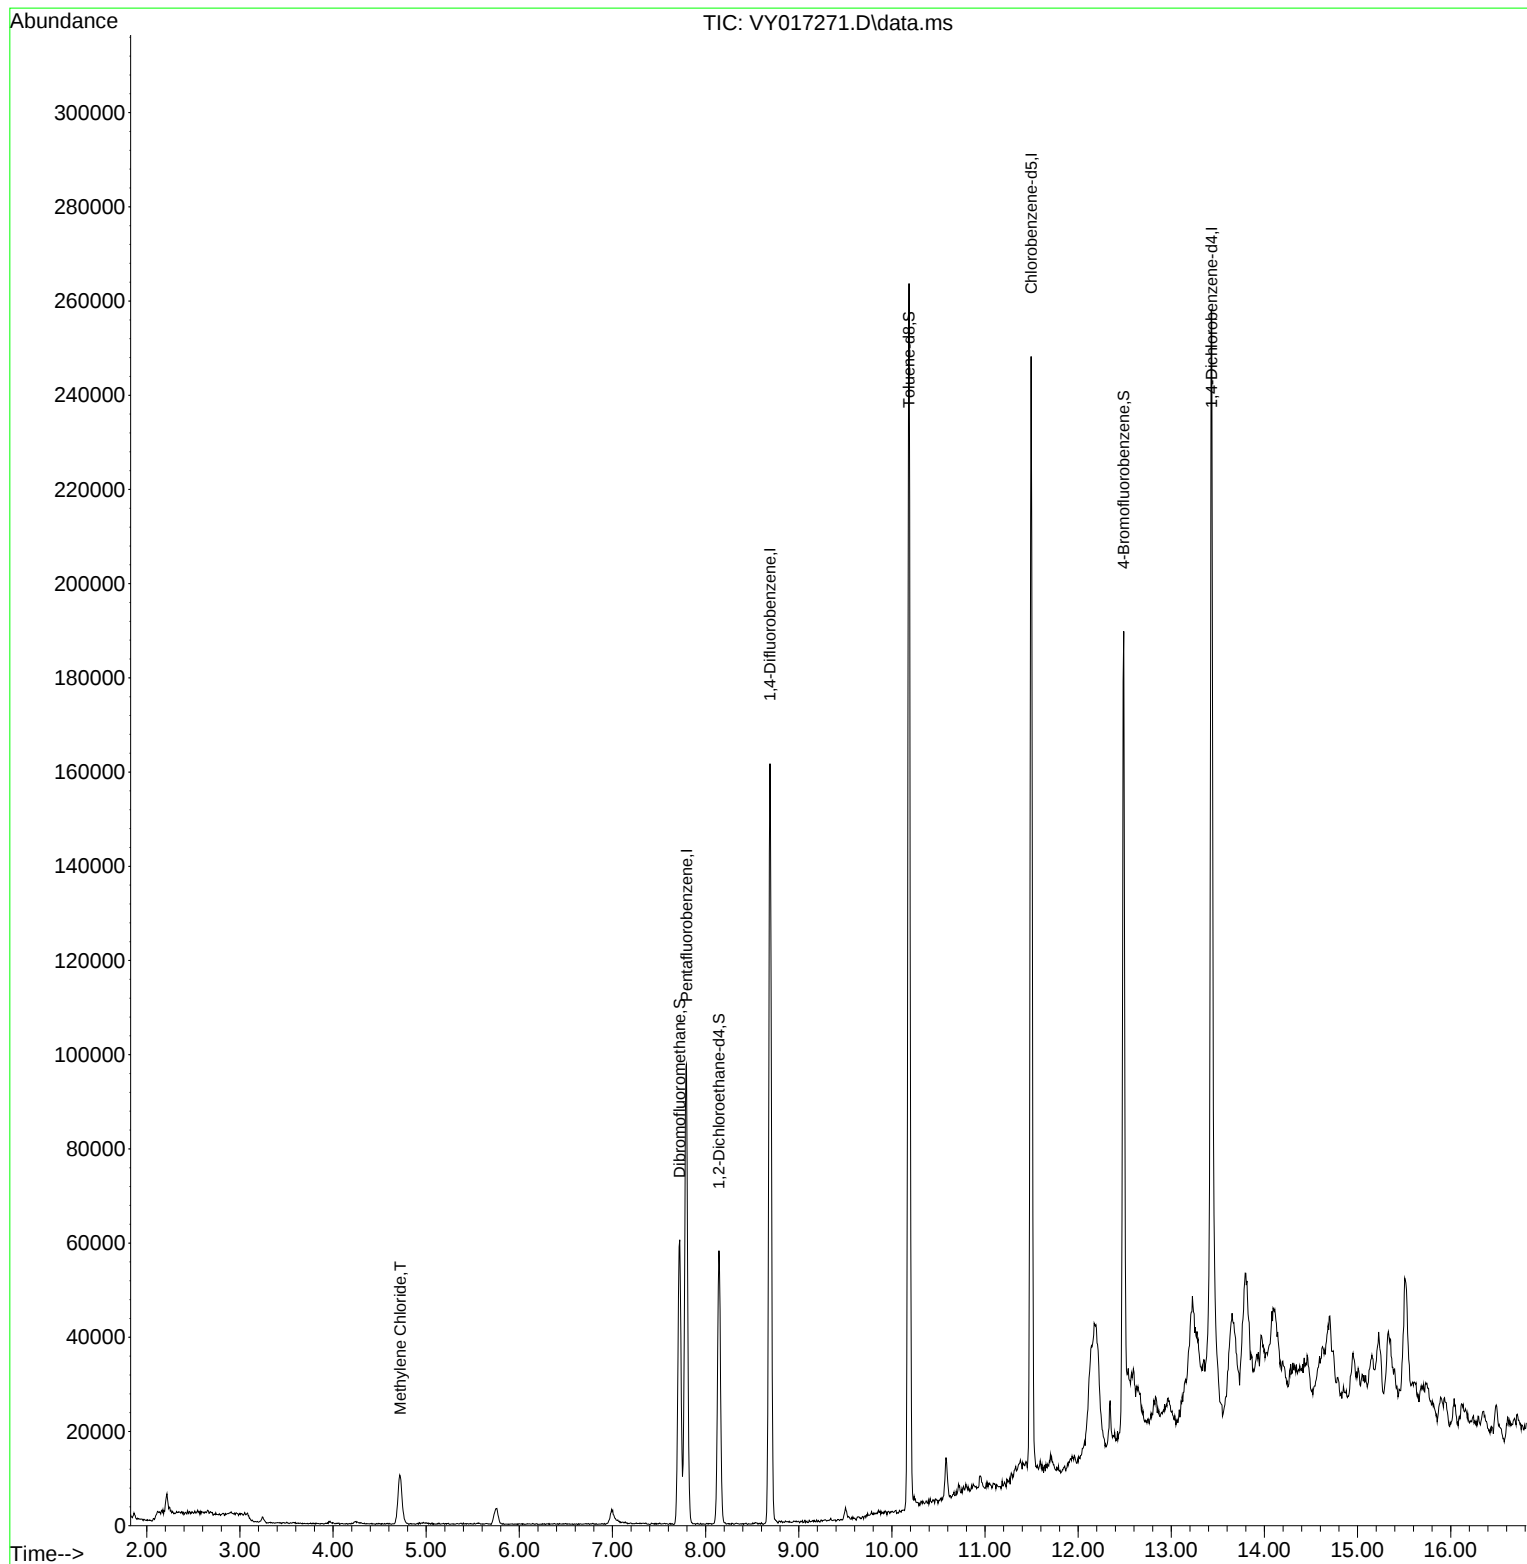


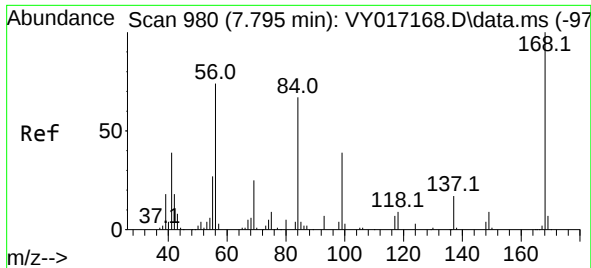

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.000 min
Lab File: VY017271.D
Acq: 06 Feb 2024 17:47




Instrument :
MSVOA_Y
ClientSampleId :
RT5149


Tgt Ion:168 Resp: 74430
Ion Ratio Lower Upper
168 100
99 53.4 44.2 66.4

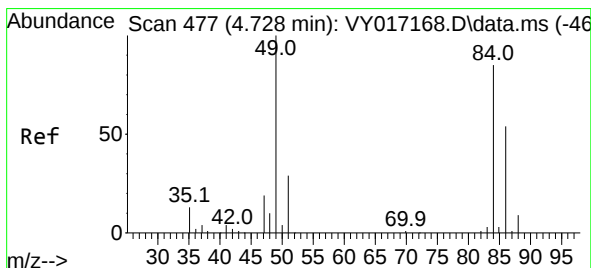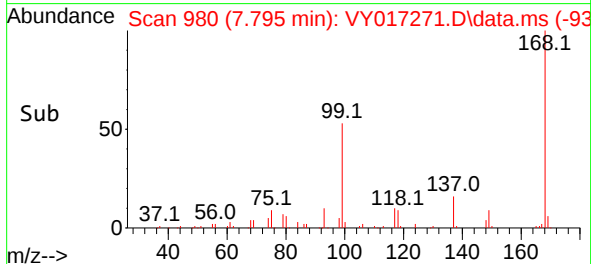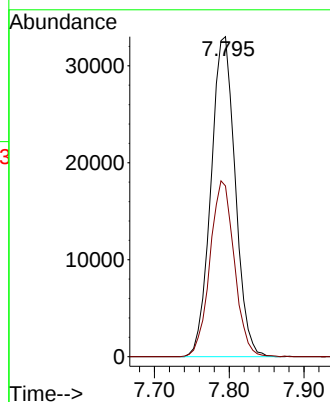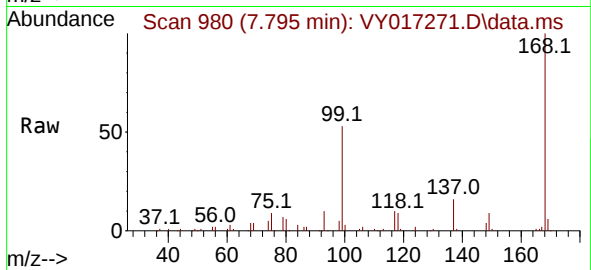

#20
Methylene Chloride
Concen: 6.988 ug/l
RT: 4.722 min Scan# 476
Delta R.T. -0.006 min
Lab File: VY017271.D
Acq: 06 Feb 2024 17:47

Tgt Ion: 84 Resp: 8005
Ion Ratio Lower Upper
84 100
49 102.0 95.2 142.8
51 31.0 29.9 44.9
86 57.5 52.2 78.4

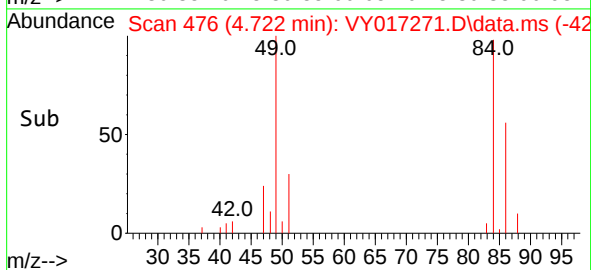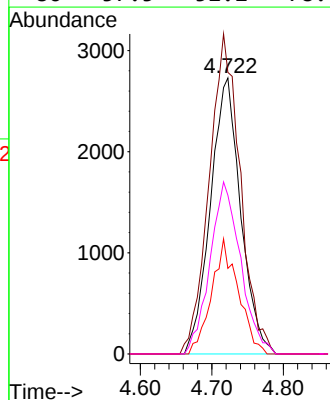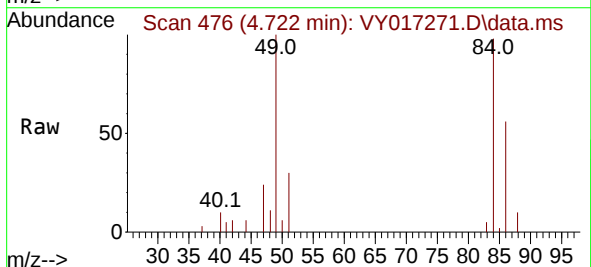

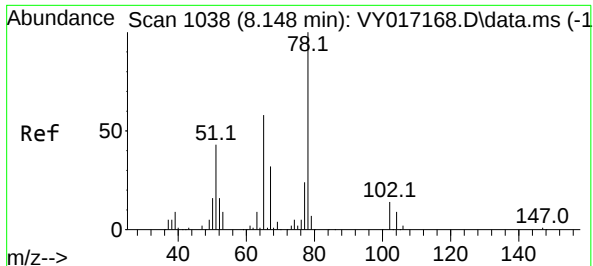

#33

1,2-Dichloroethane-d4

Concen: 65.385 ug/l

RT: 8.142 min Scan# 1037

Delta R.T. -0.006 min

Lab File: VY017271.D

Acq: 06 Feb 2024 17:47

Instrument :

MSVOA_Y

ClientSampleId :





RT5149

Tgt Ion: 65 Resp: 43475

Ion Ratio Lower Upper

65 100

67 53.1 0.0 109.0

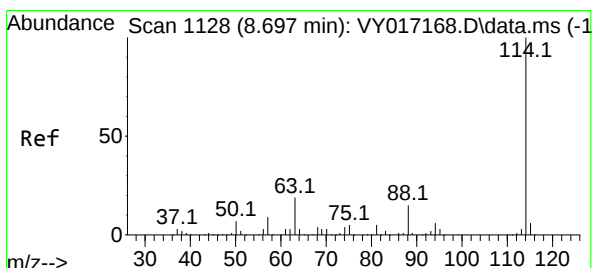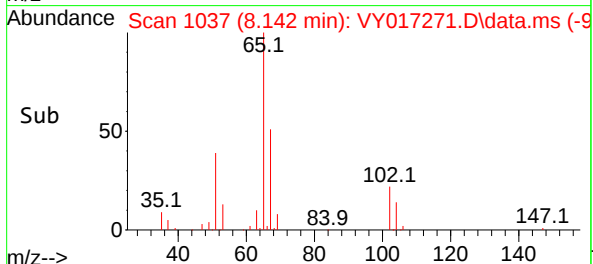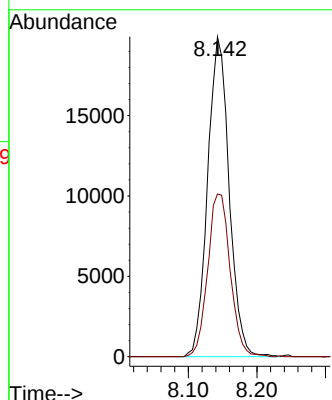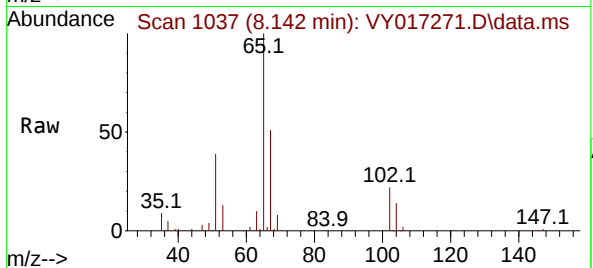

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.006 min

Lab File: VY017271.D

Acq: 06 Feb 2024 17:47




Tgt Ion: 114 Resp: 139836


Ion Ratio Lower Upper

114 100

63 19.6 0.0 37.4

88 14.5 0.0 29.0


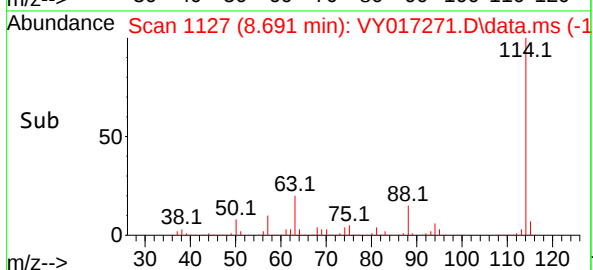
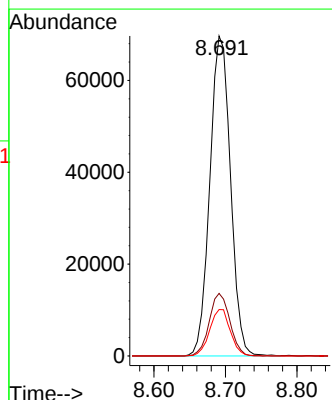
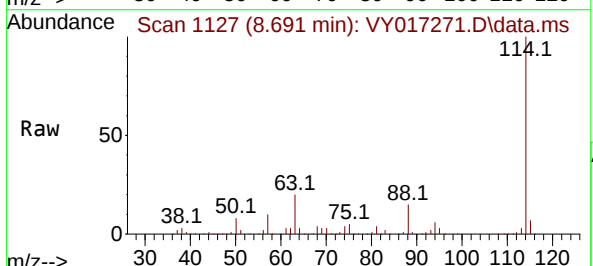


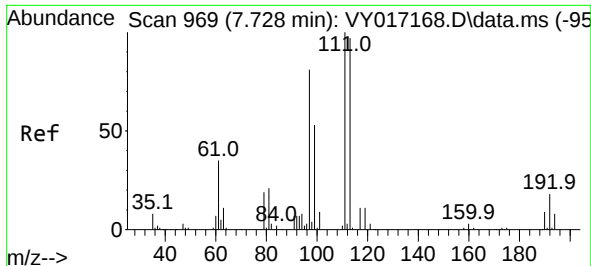

#35
Dibromofluoromethane
Concen: 57.613 ug/l
RT: 7.722 min Scan# 90
Delta R.T. -0.006 min
Lab File: VY017271.D
Acq: 06 Feb 2024 17:47




Instrument :
MSVOA_Y
ClientSampleId :
RT5149


Tgt Ion:113 Resp: 43499
Ion Ratio Lower Upper
113 100
111 102.9 83.8 125.6
192 18.0 14.5 21.7

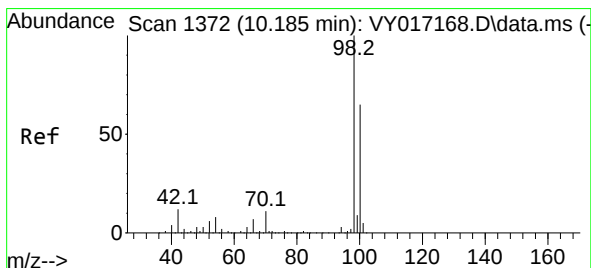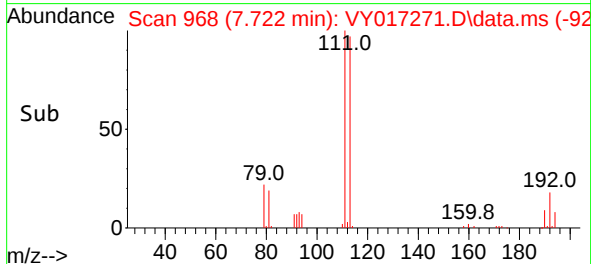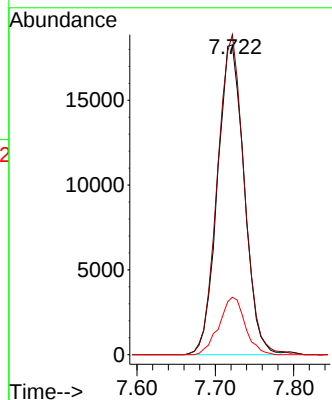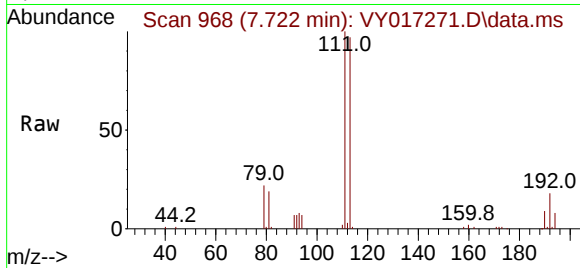

#50
Toluene-d8
Concen: 61.404 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY017271.D
Acq: 06 Feb 2024 17:47

Tgt Ion: 98 Resp: 168799
Ion Ratio Lower Upper
98 100
100 64.9 52.3 78.5


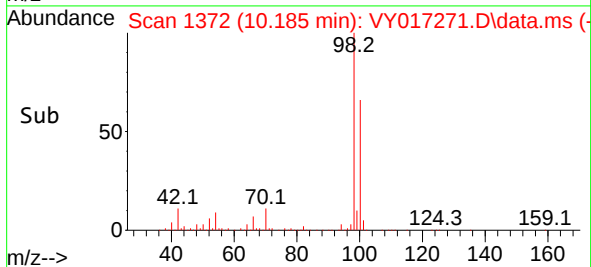
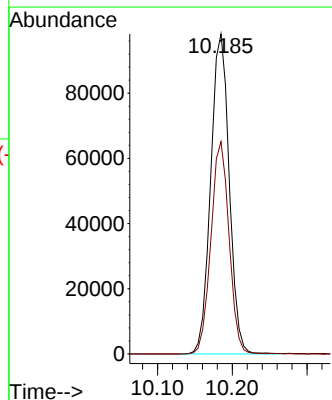
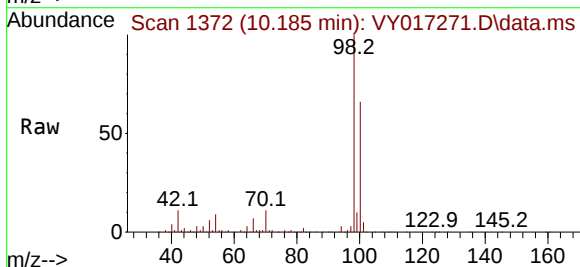


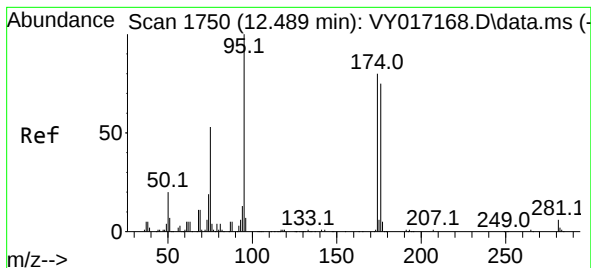

#62
4-Bromofluorobenzene
Concen: 59.299 ug/l
RT: 12.489 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VY017271.D
Acq: 06 Feb 2024 17:47




Instrument :
MSVOA_Y
ClientSampleId :
RT5149


Tgt Ion:	95	Resp:	53400
Ion	Ratio	Lower	Upper
95	100		
174	74.3	0.0	160.0
176	71.0	0.0	151.8

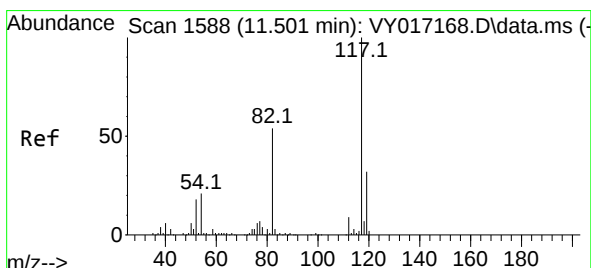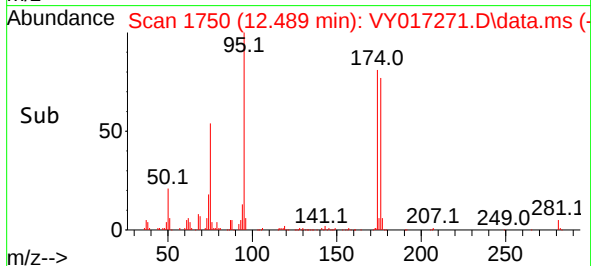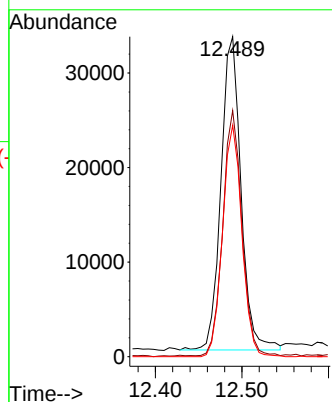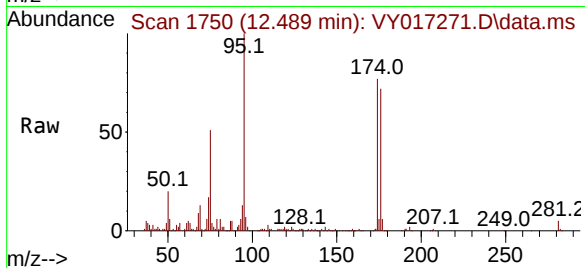

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.006 min
Lab File: VY017271.D
Acq: 06 Feb 2024 17:47

Tgt Ion:	117	Resp:	126074
Ion	Ratio	Lower	Upper
117	100		
82	55.7	43.8	65.8
119	31.2	26.5	39.7

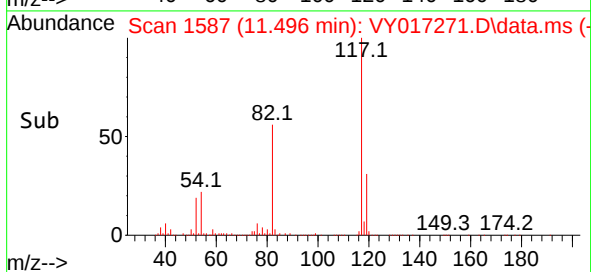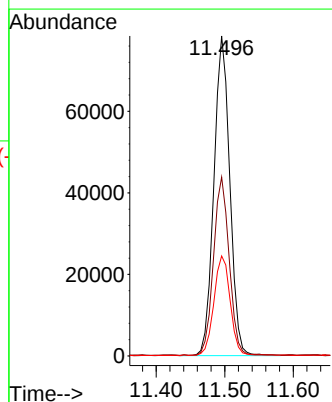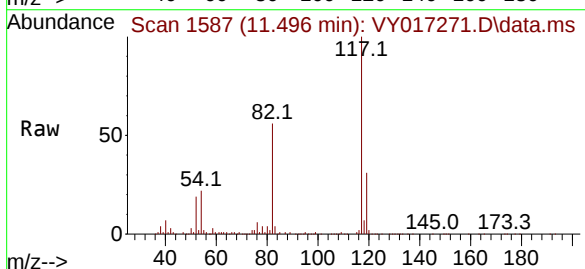

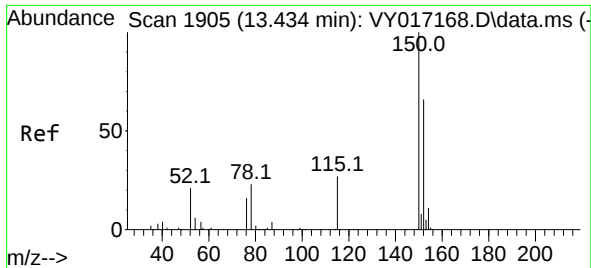

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.434 min Scan# 1905

Delta R.T. 0.000 min

Lab File: VY017271.D


Acq: 06 Feb 2024 17:47

Instrument :

MSVOA_Y

ClientSampleId :

RT5149

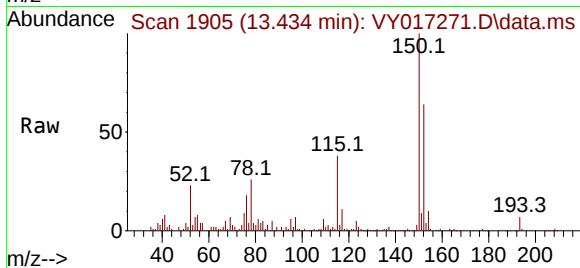

Tgt Ion:152 Resp: 48319

Ion Ratio Lower Upper

152 100

115 60.0 30.0 90.0

150 156.3 0.0 344.6

