
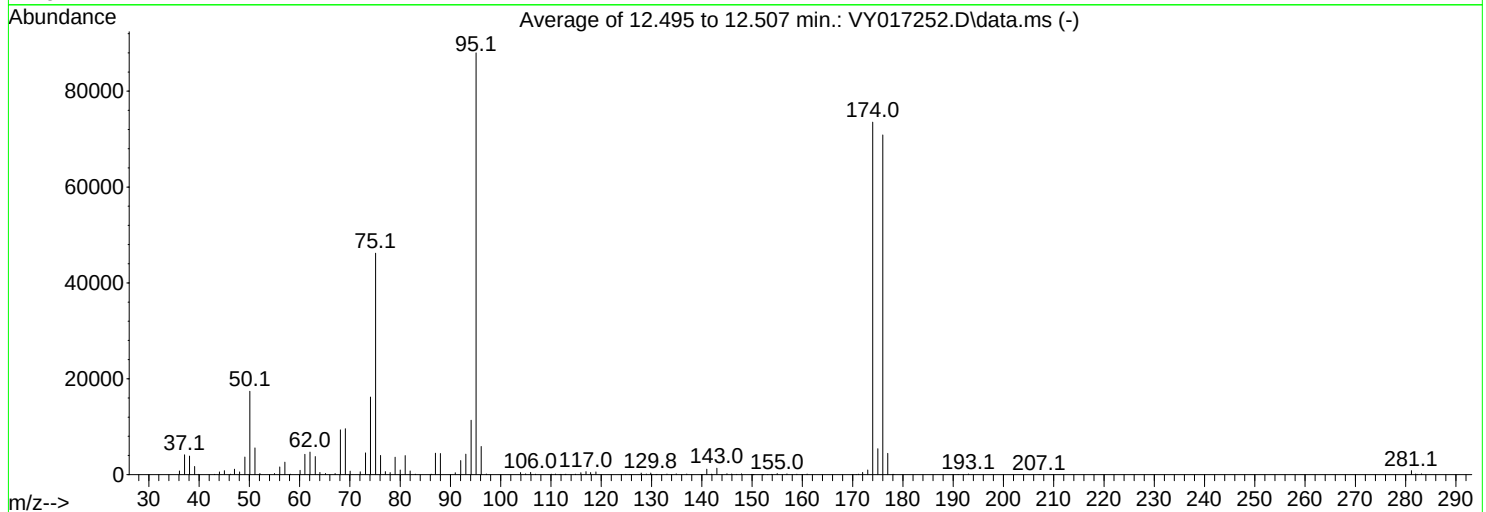


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020624\
Data File : VY017252.D
Acq On : 06 Feb 2024 08:41
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020124S.M
Title : SW846 8260
Last Update : Fri Feb 02 00:56:04 2024

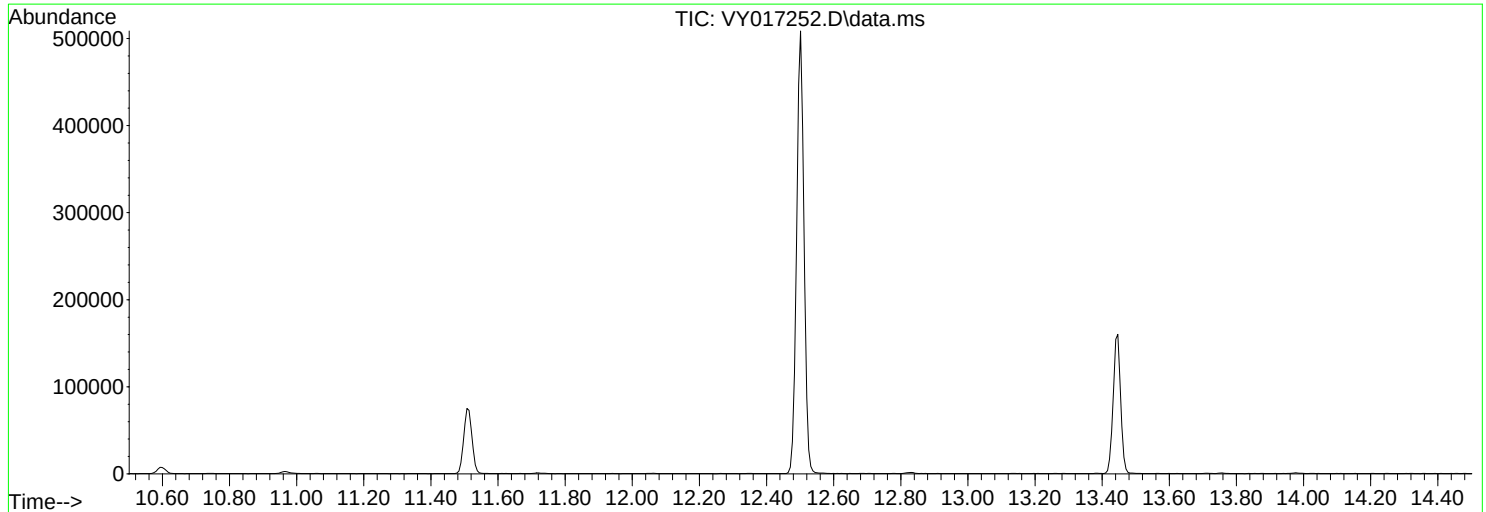

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	17401	PASS
75	95	30	60	52.5	46189	PASS
95	95	100	100	100.0	88000	PASS
96	95	5	9	6.7	5895	PASS
173	174	0.00	2	1.3	969	PASS
174	95	50	100	83.6	73539	PASS
175	174	5	9	7.4	5409	PASS
176	174	95	101	96.4	70856	PASS
177	176	5	9	6.3	4439	PASS