

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY020720\
 Data File : VY001561.D
 Acq On : 07 Feb 2020 17:53
 Operator : SY/MD
 Sample : L1403-03RE
 Misc : 9.46G/5ML/MSVOA Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Feb 08 01:27:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 04 15:10:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.82	168	178316	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	314339	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	281651	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.44	152	125696	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.17	65	102168	56.91	ug/l	0.00
Spiked Amount			Recovery	=	113.82%	
35) Dibromofluoromethane	7.75	113	91733	50.61	ug/l	0.00
Spiked Amount			Recovery	=	101.22%	
50) Toluene-d8	10.19	98	371647	54.19	ug/l	0.00
Spiked Amount			Recovery	=	108.38%	
62) 4-Bromofluorobenzene	12.49	95	130257	48.21	ug/l	0.00
Spiked Amount			Recovery	=	96.42%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	5.00	59	40	Below Cal	#	76
16) Acetone	3.97	43	1487	2.863	ug/l #	80
29) Tetrahydrofuran	7.39	42	426	1.055	ug/l #	52
31) Cyclohexane	7.81	56	3787	1.083	ug/l #	1
36) 1,1-Dichloropropene	7.82	75	14333	4.984	ug/l #	48
38) Carbon Tetrachloride	7.82	117	17702	6.363	ug/l #	16
76) 1,2,3-Trichloropropane	12.49	75	64911	48.020	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.49	75	64911	92.917	ug/l #	16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY020720\
Data File : VY001561.D
Acq On : 07 Feb 2020 17:53
Operator : SY/MD
Sample : L1403-03RE
Misc : 9.46G/5ML/MSVOA Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Feb 08 01:27:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 04 15:10:08 2020
Response via : Initial Calibration

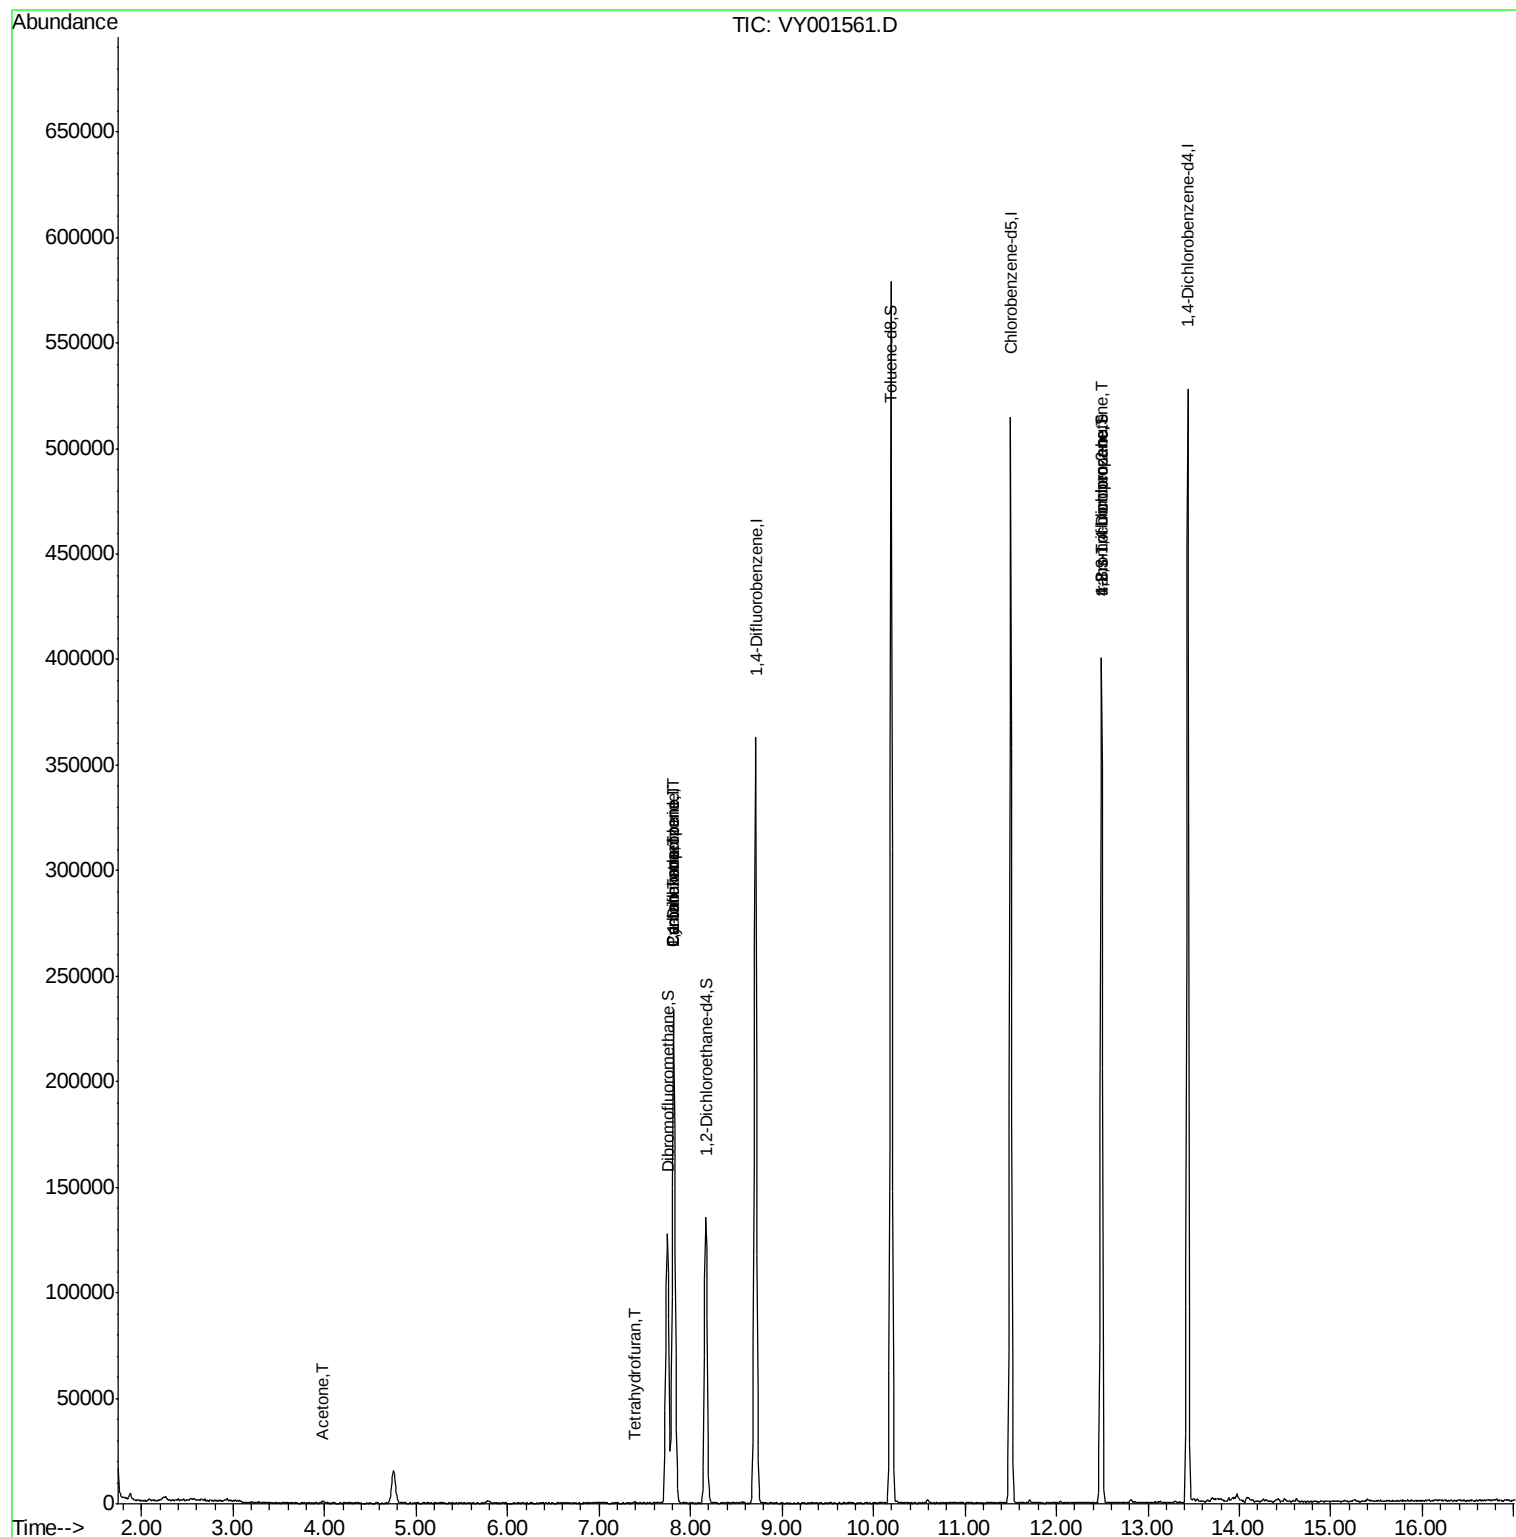

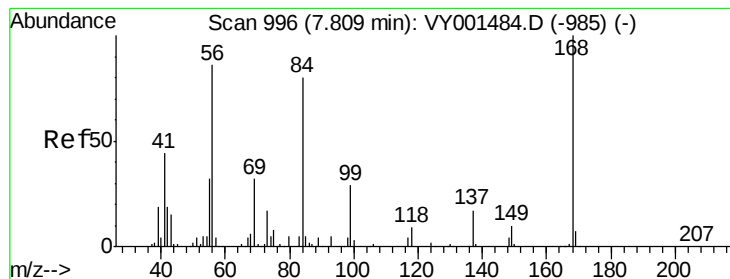

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.82 min Scan# 997

Delta R.T. 0.01 min

Lab File: VY001561.D

Acq: 07 Feb 2020 17:53

Instrument :

MSVOA_Y


ClientSampleId :

Tot Ion:168 Resp: 178316

Ion Ratio Lower Upper

168 100

99 57.9 48.2 72.4

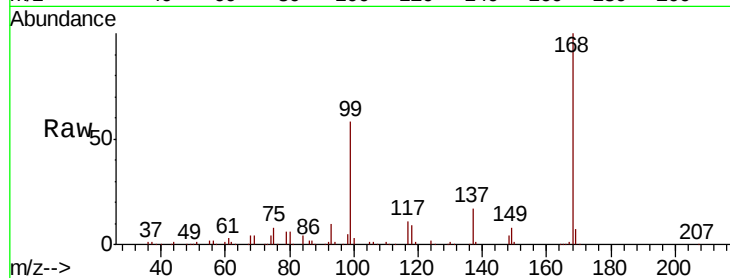

Abundance Ion 167.90 (167.60 to 168.60): VY001484.D (-985) (-)

Ion 98.90 (98.60 to 99.60): VY001484.D (-985) (-)

7.82

80000



60000

40000

20000

0

Time-->

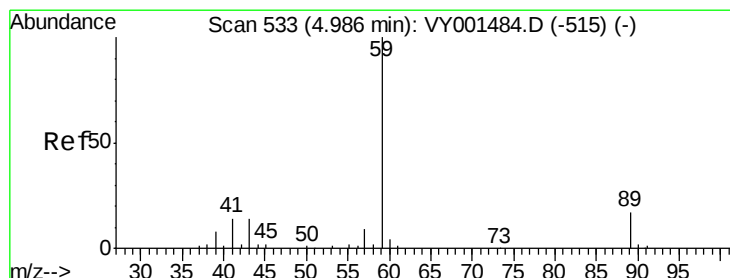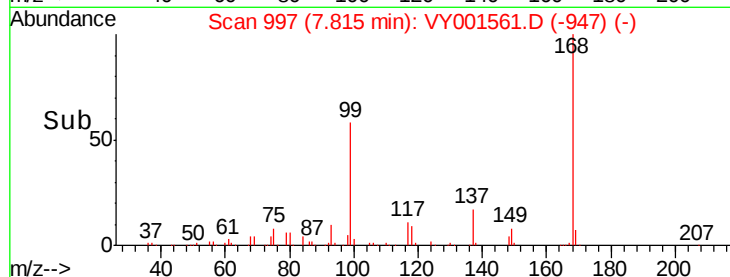

#11

Tert butyl alcohol

Concen: Below Cal

RT: 5.00 min Scan# 536

Delta R.T. 0.02 min

Lab File: VY001561.D


Acq: 07 Feb 2020 17:53

Tgt Ion: 59 Resp: 40

Ion Ratio Lower Upper

59 100

57 0.0 7.0 10.6#

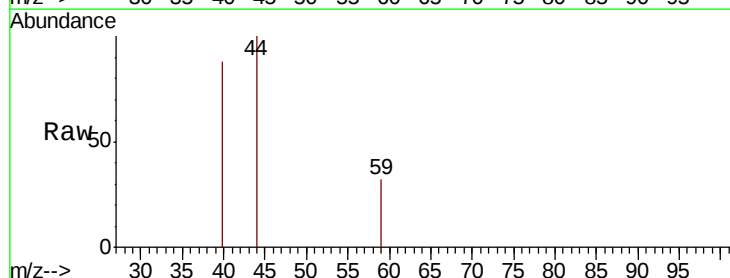

Abundance Ion 59.00 (58.70 to 59.70): VY001484.D (-515) (-)

Ion 57.00 (56.70 to 57.70): VY001484.D (-515) (-)

100

80


60


40

20

0

Time-->




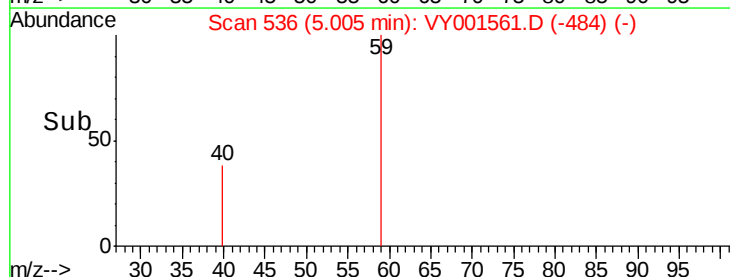


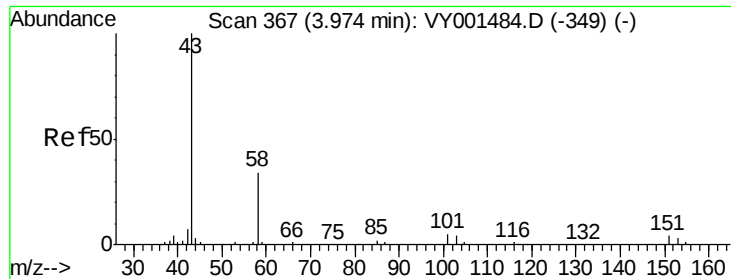

#16
Acetone
Concen: 2.863 ug/l
RT: 3.97 min Scan# 367
Delta R.T. -0.00 min
Lab File: VY001561.D
Acq: 07 Feb 2020 17:53




Instrument :
MSVOA_Y
ClientSampleId :


Tot Ion: 43 Resp: 1487
Ion Ratio Lower Upper
43 100
58 23.2 27.5 41.3#

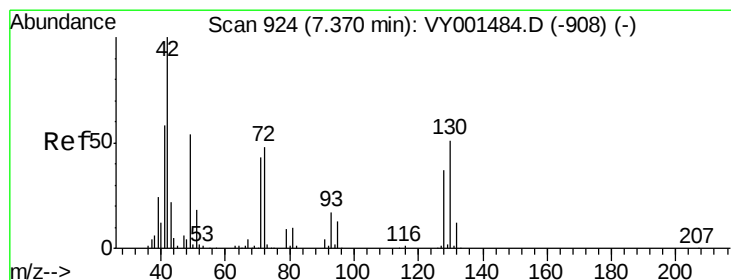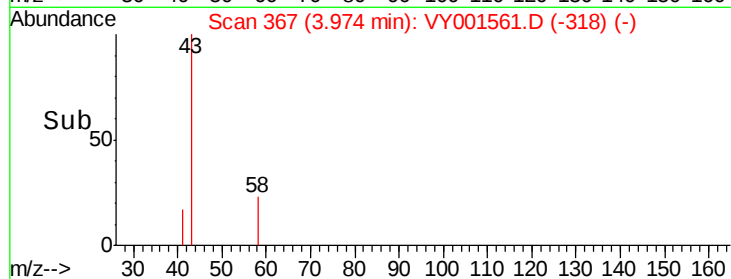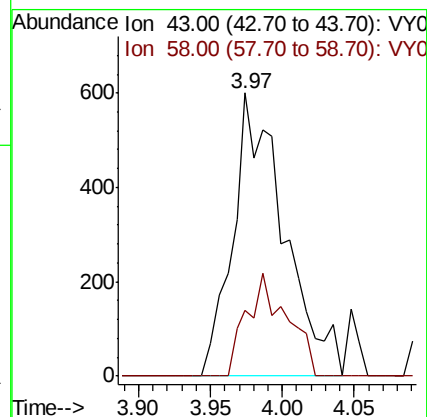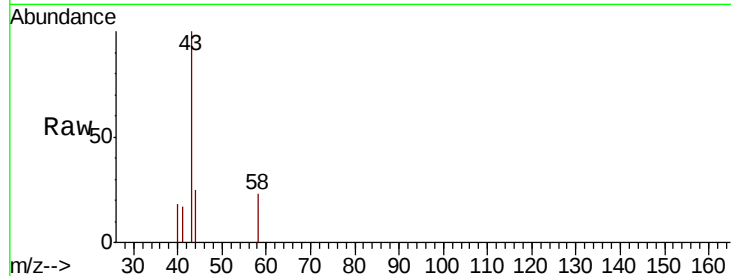

#29
Tetrahydrofuran
Concen: 1.055 ug/l
RT: 7.39 min Scan# 927
Delta R.T. 0.02 min
Lab File: VY001561.D
Acq: 07 Feb 2020 17:53

Tgt Ion: 42 Resp: 426
Ion Ratio Lower Upper
42 100
72 0.0 37.8 56.6#
71 27.9 34.8 52.2#

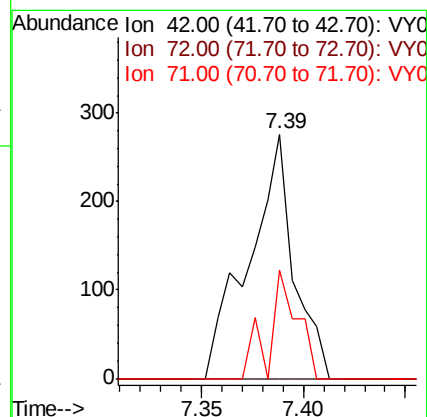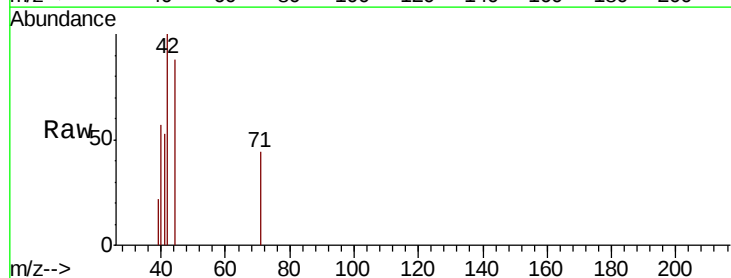


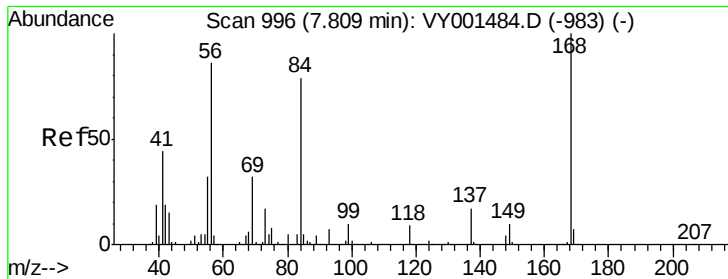




#31
Cyclohexane
Concen: 1.083 ug/l
RT: 7.81 min Scan# 996
Delta R.T. -0.00 min
Lab File: VY001561.D
Acq: 07 Feb 2020 17:53

Instrument :
MSVOA_Y
ClientSampled :

Tot Ion: 56 Resp: 3787
Ion Ratio Lower Upper
56 100
69 155.4 29.6 44.4#
84 150.8 73.6 110.4#

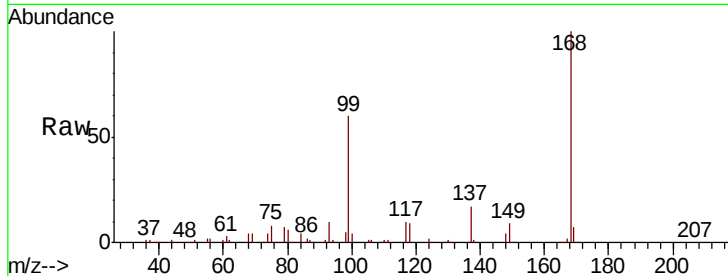


Abundance Ion 56.00 (55.70 to 56.70): VY0
Ion 69.00 (68.70 to 69.70): VY0
Ion 84.00 (83.70 to 84.70): VY0

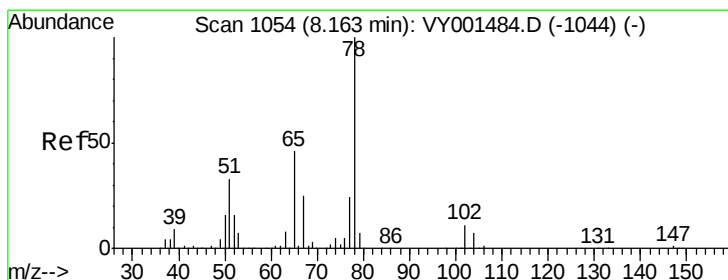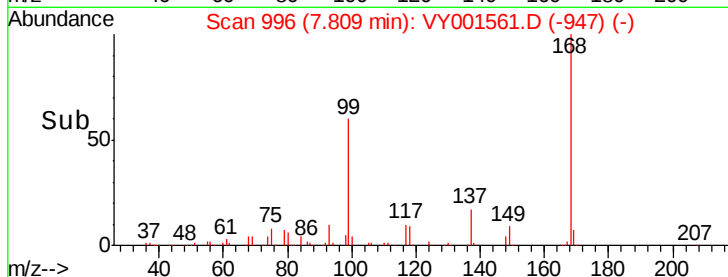
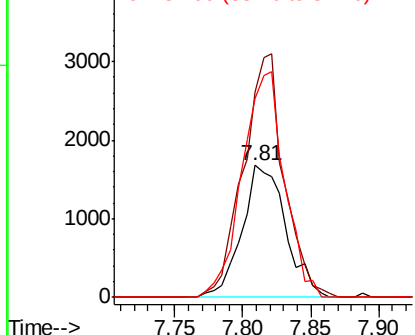



#33
1,2-Dichloroethane-d4
Concen: 56.906 ug/l
RT: 8.17 min Scan# 1055
Delta R.T. 0.01 min
Lab File: VY001561.D
Acq: 07 Feb 2020 17:53

Tgt Ion: 65 Resp: 102168
Ion Ratio Lower Upper
65 100
67 54.3 0.0 108.6

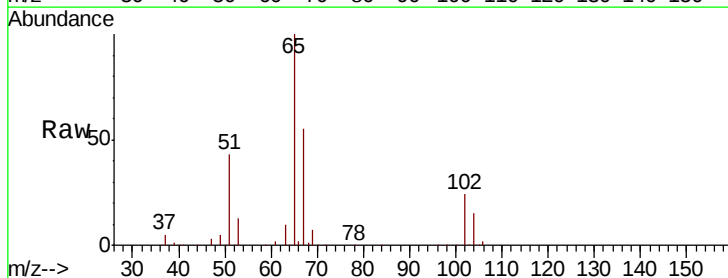

Abundance Ion 64.90 (64.60 to 65.60): VY0
Ion 66.90 (66.60 to 67.60): VY0

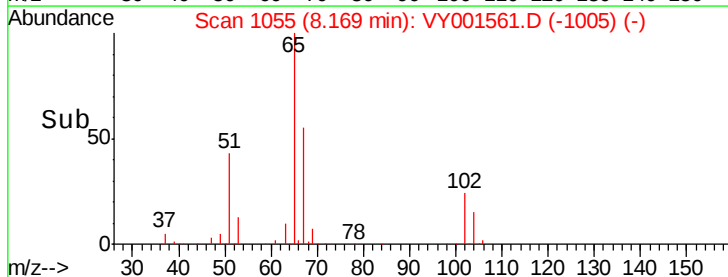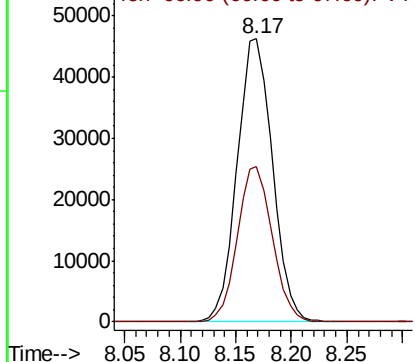

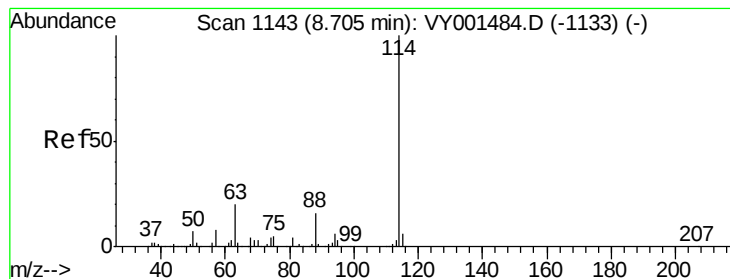

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.71 min Scan# 1144

Delta R.T. 0.01 min

Lab File: VY001561.D

Acq: 07 Feb 2020 17:53

Instrument :

MSVOA_Y

ClientSampleId :


Tot Ion:114 Resp: 314339

Ion Ratio Lower Upper

114 100

63 19.4 0.0 39.8




88 16.0 0.0 32.6

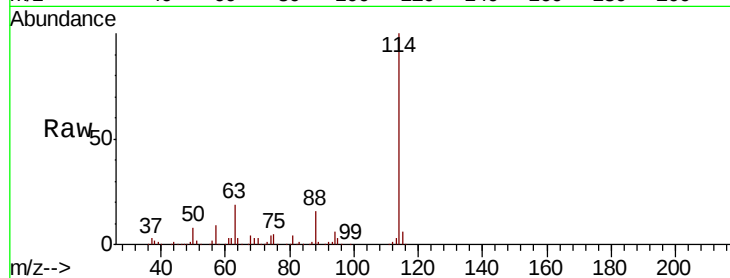

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

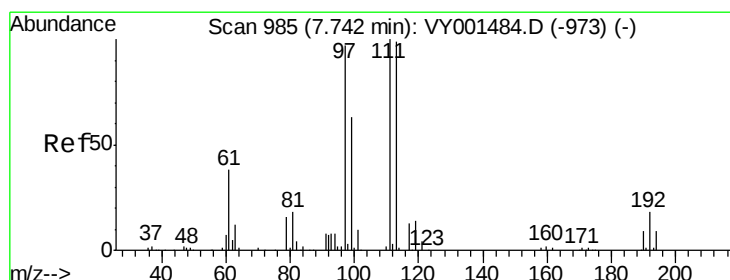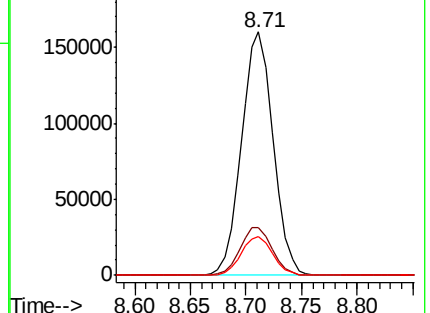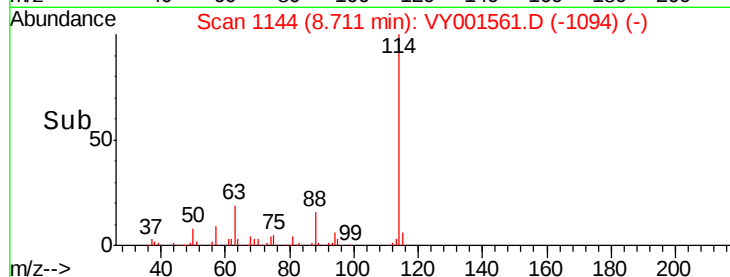

#35

Dibromofluoromethane

Concen: 50.608 ug/l

RT: 7.75 min Scan# 986

Delta R.T. 0.01 min

Lab File: VY001561.D

Acq: 07 Feb 2020 17:53


Tgt Ion:113 Resp: 91733

Ion Ratio Lower Upper

113 100

111 101.8 82.9 124.3



192 19.7 14.6 22.0

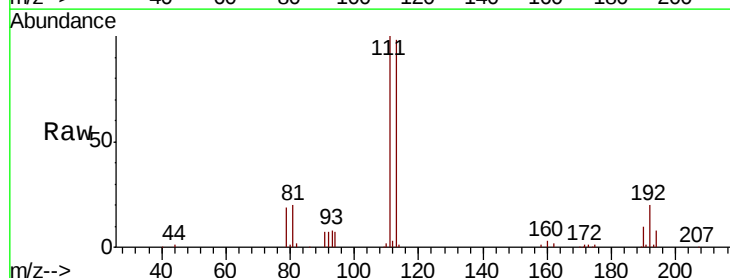


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



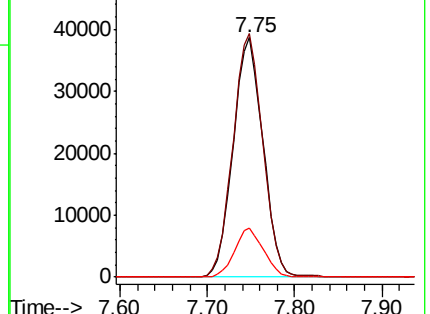
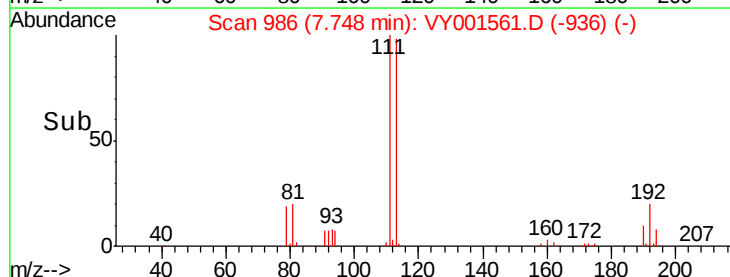


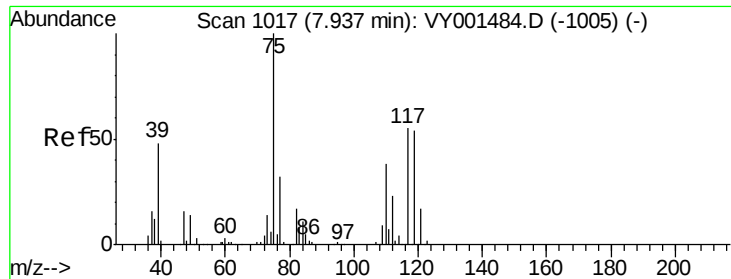

#36
 1,1-Dichloropropene
 Concen: 4.984 ug/l
 RT: 7.82 min Scan# 997
 Delta R.T. -0.12 min
 Lab File: VY001561.D
 Acq: 07 Feb 2020 17:53




Instrument :
 MSVOA_Y
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
75	100		
110	7.7	18.2	54.6#
77	0.0	25.0	37.4#

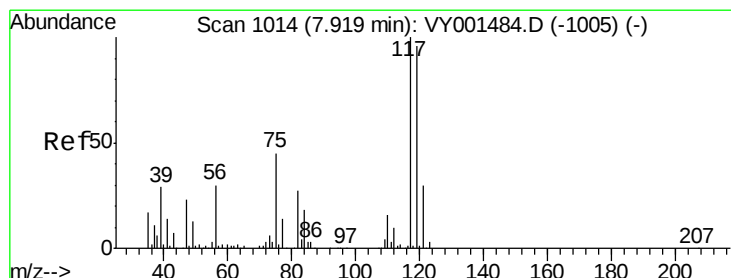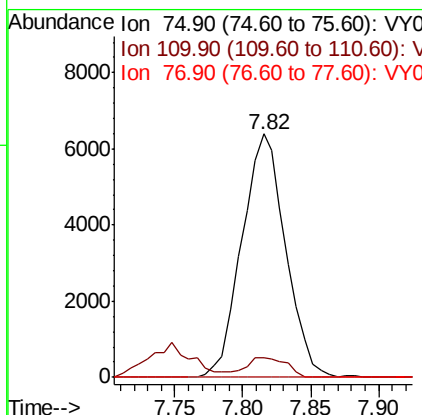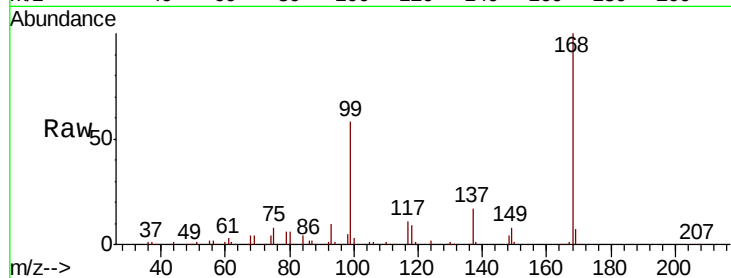

#38
 Carbon Tetrachloride
 Concen: 6.363 ug/l
 RT: 7.82 min Scan# 997
 Delta R.T. -0.10 min
 Lab File: VY001561.D
 Acq: 07 Feb 2020 17:53

Tgt Ion	Ratio	Lower	Upper
117	100		
119	5.0	76.4	114.6#
121	0.0	24.2	36.4#

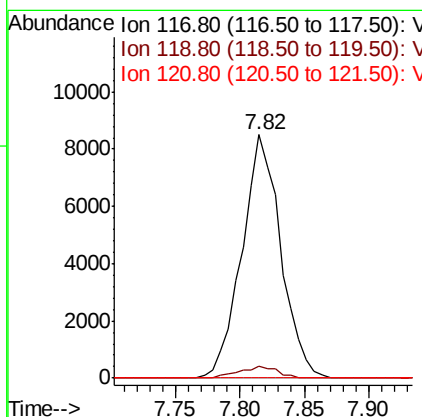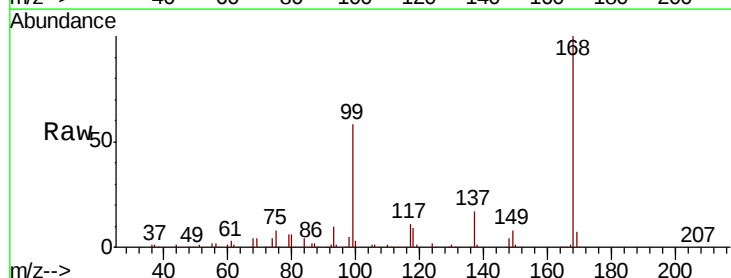

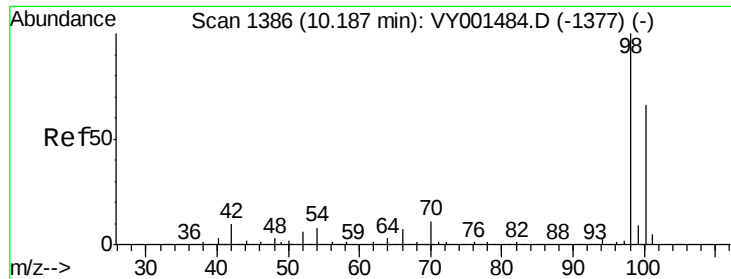

#50

Toluene-d8

Concen: 54.192 ug/l

RT: 10.19 min Scan# 1387

Delta R.T. 0.01 min

Lab File: VY001561.D

Acq: 07 Feb 2020 17:53

Instrument :

MSVOA_Y


ClientSampleId :

Tot Ion: 98 Resp: 371647




Ion Ratio Lower Upper

98 100

100 66.5 53.0 79.6

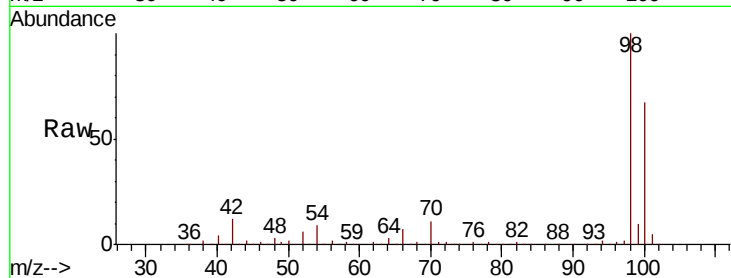

Abundance Ion 98.00 (97.70 to 98.70): VY001484.D (-1377) (-)

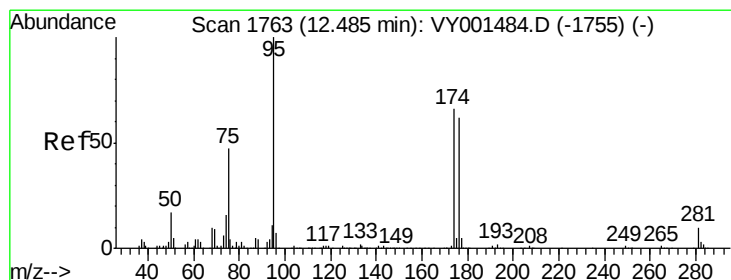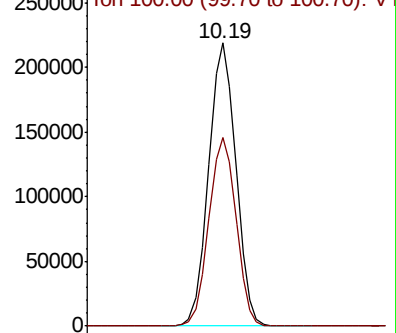

#62

4-Bromofluorobenzene

Concen: 48.214 ug/l

RT: 12.49 min Scan# 1764

Delta R.T. 0.01 min

Lab File: VY001561.D

Acq: 07 Feb 2020 17:53


Tgt Ion: 95 Resp: 130257

Ion Ratio Lower Upper



95 100


174 75.9 0.0 141.4

176 72.1 0.0 135.4

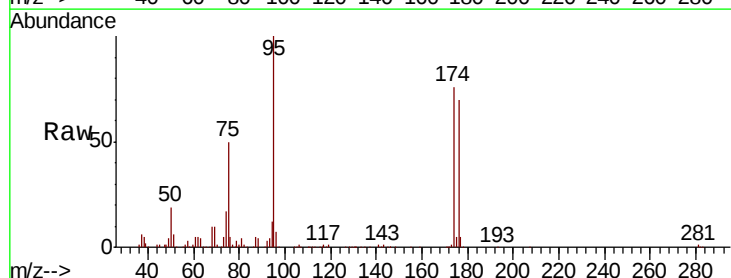

Abundance Ion 94.90 (94.60 to 95.60): VY001484.D (-1755) (-)

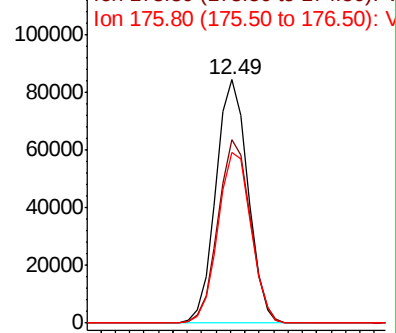







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1602
Delta R.T. 0.01 min
Lab File: VY001561.D
Acq: 07 Feb 2020 17:53

Instrument :
MSVOA_Y
ClientSampled :

Tot Ion:117 Resp: 281651
Ion Ratio Lower Upper
117 100
82 54.3 46.1 69.1
119 31.2 26.1 39.1

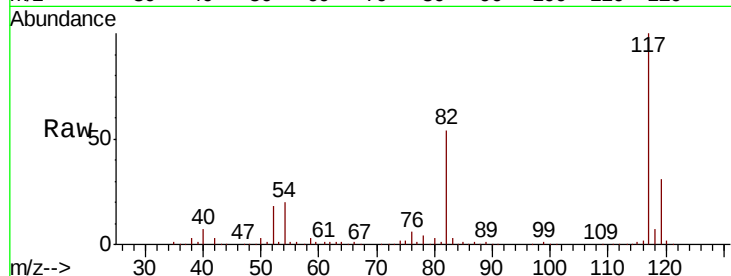


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

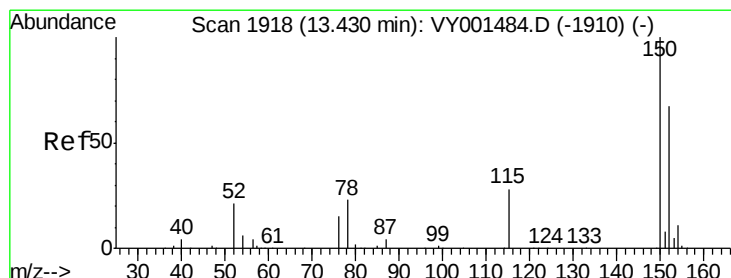
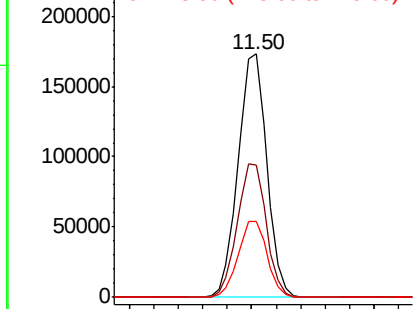



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.44 min Scan# 1919
Delta R.T. 0.01 min
Lab File: VY001561.D
Acq: 07 Feb 2020 17:53

Tgt Ion:152 Resp: 125696
Ion Ratio Lower Upper
152 100
115 61.2 31.4 94.3
150 159.7 0.0 346.8

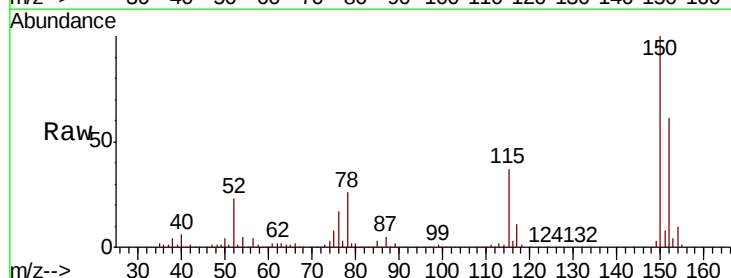

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

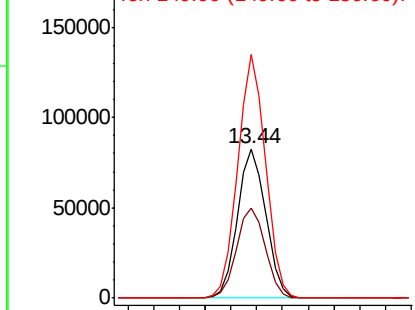



#76

1,2,3-Trichloropropane

Concen: 48.020 ug/l

RT: 12.49 min Scan# 1764

Delta R.T. -0.15 min

Lab File: VY001561.D

Acq: 07 Feb 2020 17:53

Instrument :

MSVOA_Y





ClientSampleId :

Tot Ion: 75 Resp: 64911

Ion Ratio Lower Upper

75 100

77 1.3 0.0 0.0#

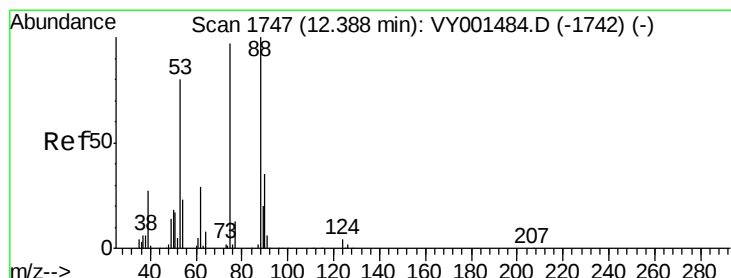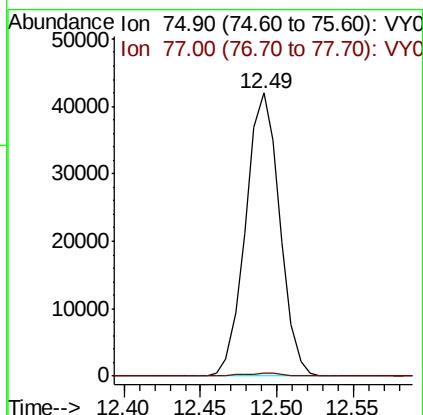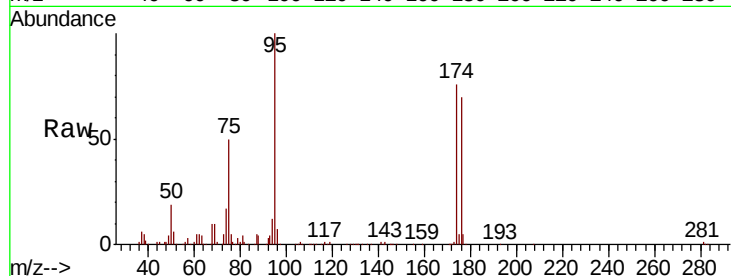

#81

trans-1,4-Dichloro-2-butene

Concen: 92.917 ug/l

RT: 12.49 min Scan# 1764

Delta R.T. 0.10 min

Lab File: VY001561.D

Acq: 07 Feb 2020 17:53

Tgt Ion: 75 Resp: 64911

Ion Ratio Lower Upper

75 100

53 0.0 67.7 101.5#

89 0.1 34.6 52.0#

