
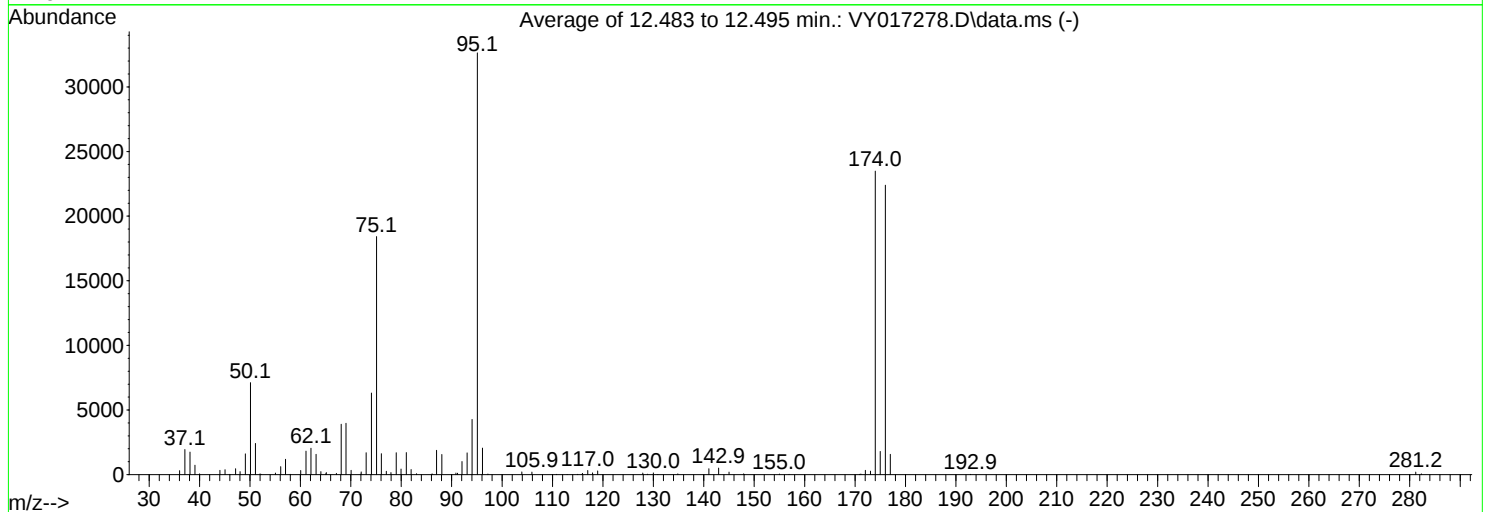


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY020724\  
Data File : VY017278.D  
Acq On : 07 Feb 2024 09:04  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y020124S.M  
Title : SW846 8260  
Last Update : Fri Feb 02 00:56:04 2024

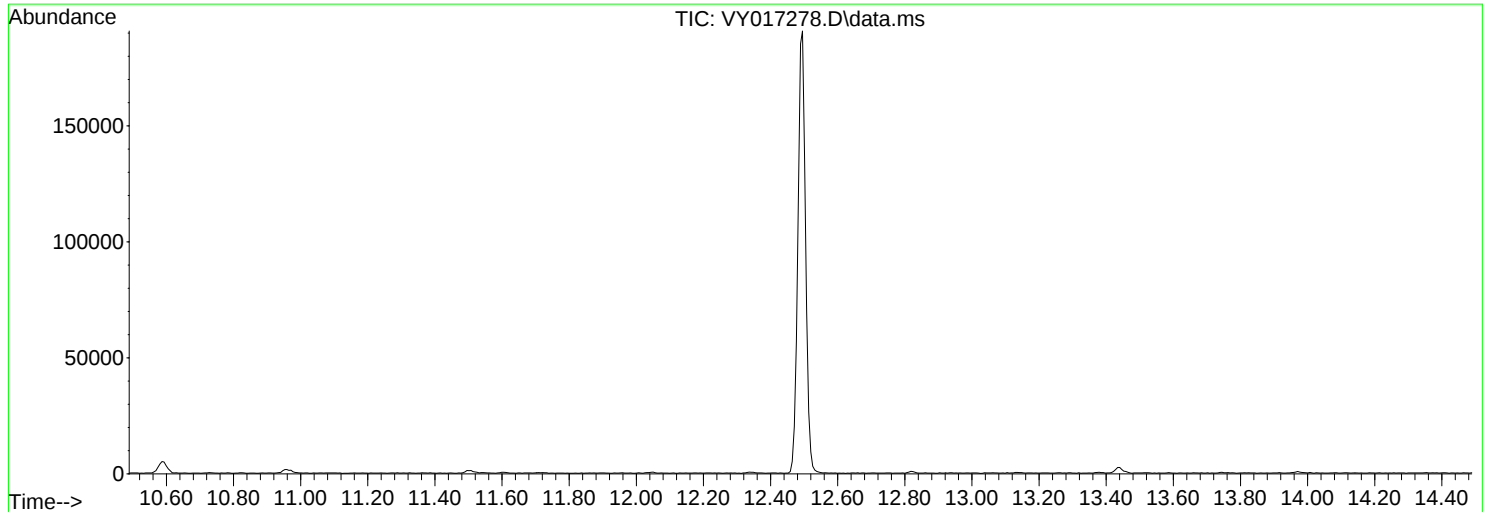

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1742

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 21.8  | 7119  | PASS      |
| 75     | 95      | 30     | 60     | 56.4  | 18418 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 32635 | PASS      |
| 96     | 95      | 5      | 9      | 6.3   | 2052  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.2   | 277   | PASS      |
| 174    | 95      | 50     | 100    | 72.0  | 23485 | PASS      |
| 175    | 174     | 5      | 9      | 7.6   | 1791  | PASS      |
| 176    | 174     | 95     | 101    | 95.4  | 22401 | PASS      |
| 177    | 176     | 5      | 9      | 7.0   | 1574  | PASS      |