

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY021020\
 Data File : VY001579.D
 Acq On : 10 Feb 2020 12:31
 Operator : SY/MD
 Sample : VY0210SBL01
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0210SBL01

Quant Time: Feb 11 06:05:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 04 15:10:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.81	168	184455	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	326420	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	290397	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.44	152	126340	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.16	65	102560	55.22	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.44%	
35) Dibromofluoromethane	7.74	113	95467	50.72	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.44%	
50) Toluene-d8	10.19	98	396713	55.71	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.42%	
62) 4-Bromofluorobenzene	12.49	95	132957	47.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.78%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY021020\
Data File : VY001579.D
Acq On : 10 Feb 2020 12:31
Operator : SY/MD
Sample : VY0210SBL01
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0210SBL01

Quant Time: Feb 11 06:05:10 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 04 15:10:08 2020
Response via : Initial Calibration

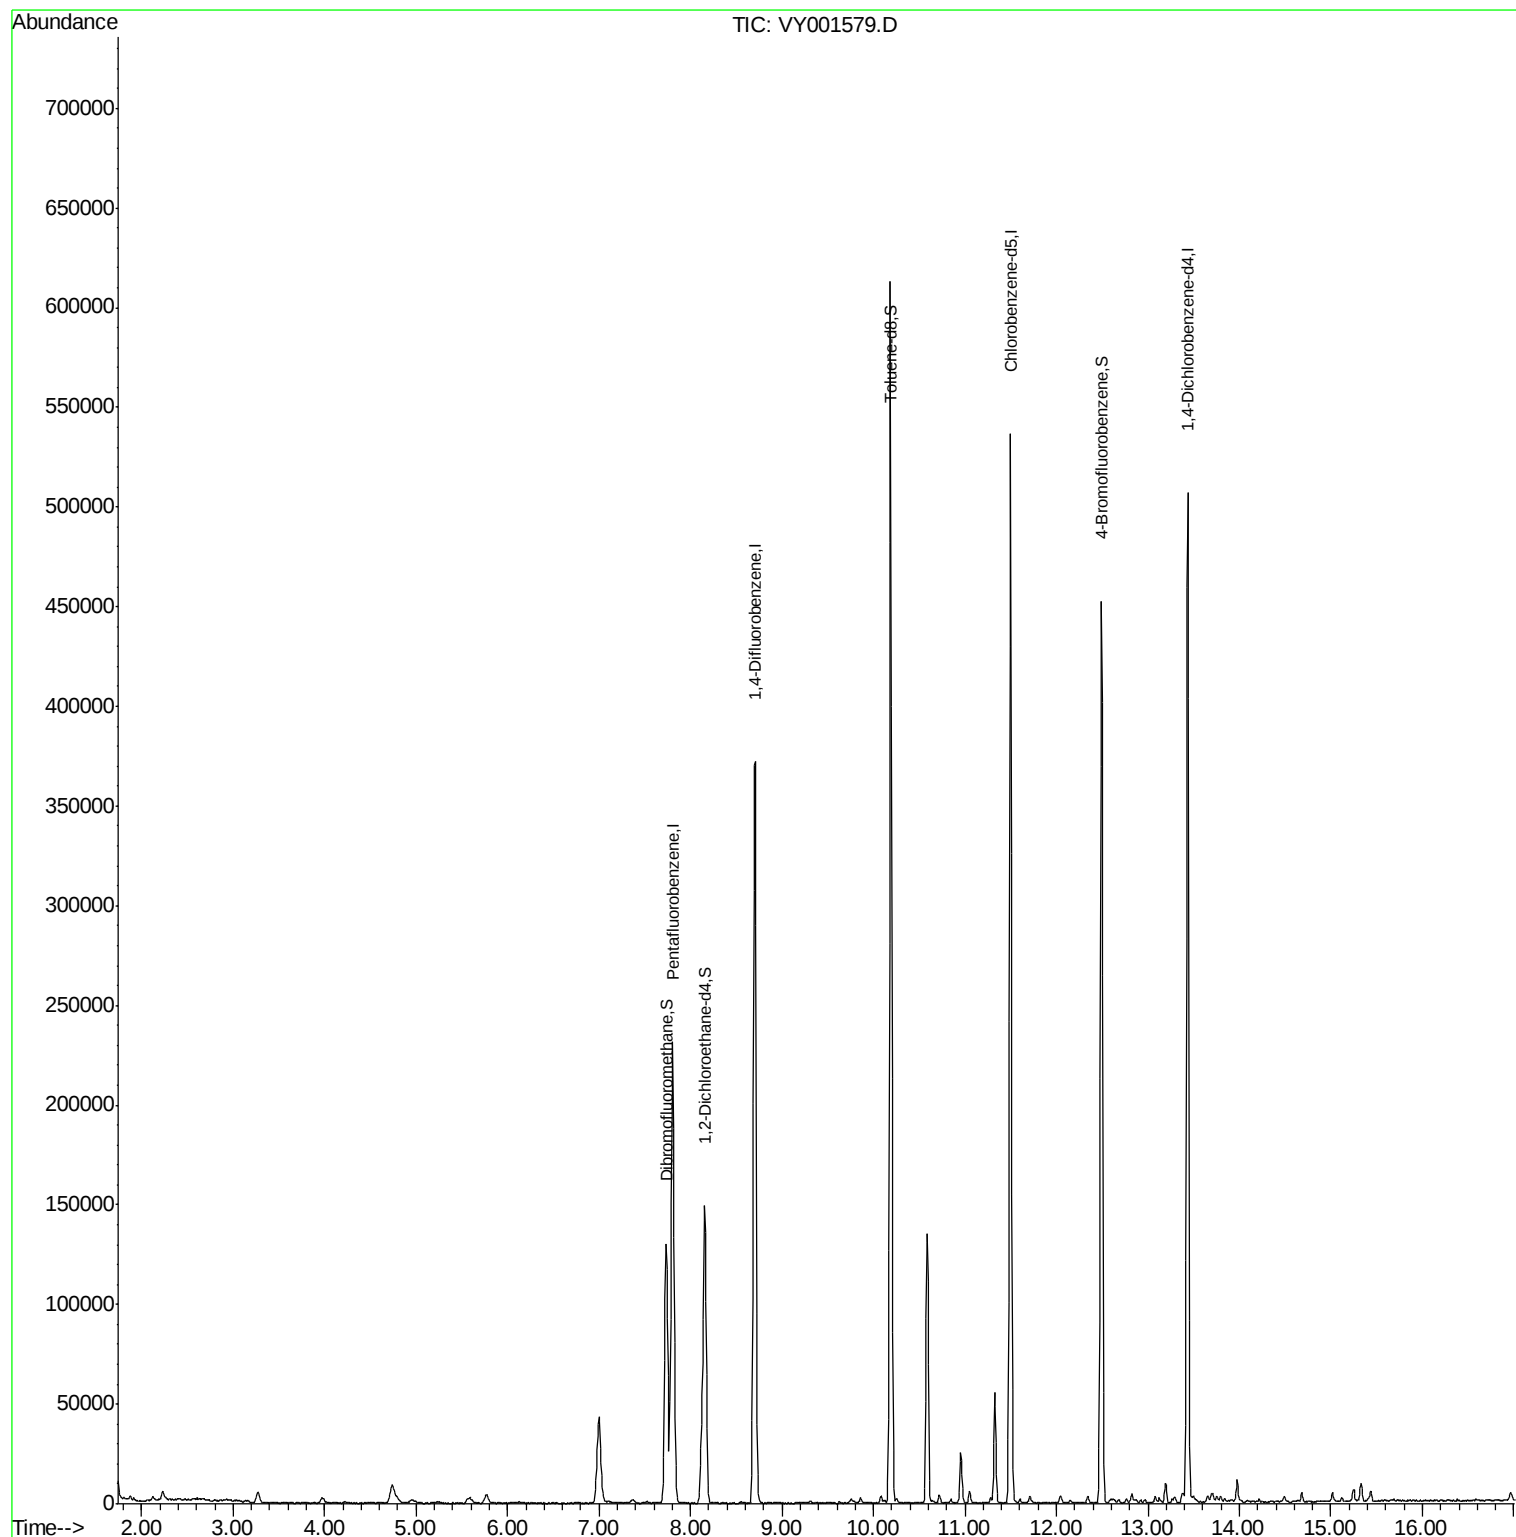

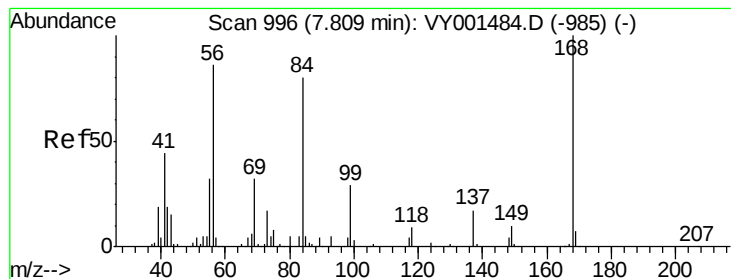

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.81 min Scan# 996

Delta R.T. 0.00 min

Lab File: VY001579.D

Acq: 10 Feb 2020 12:31

Instrument :

MSVOA_Y

ClientSampleId :


VY0210SBL01

Tot Ion:168 Resp: 184455

Ion Ratio Lower Upper




168 100

99 53.5 48.2 72.4

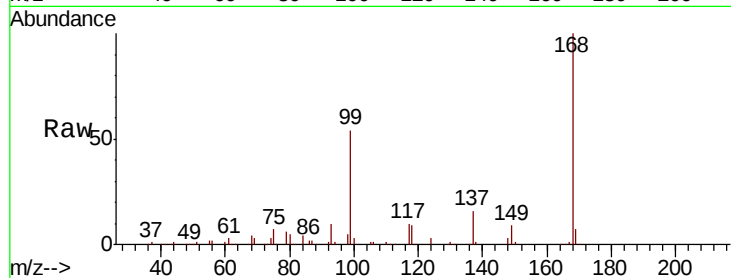

Abundance Ion 167.90 (167.60 to 168.60): VY001579.D (-947) (-)

Ion 98.90 (98.60 to 99.60): VY001579.D (-947) (-)

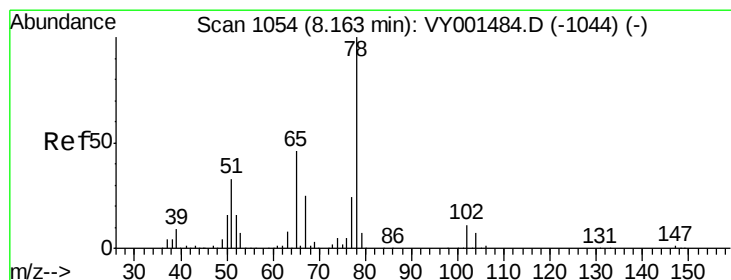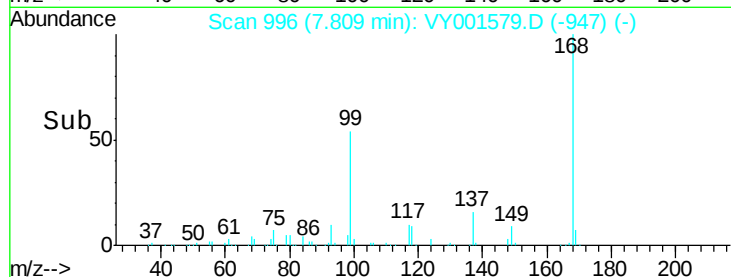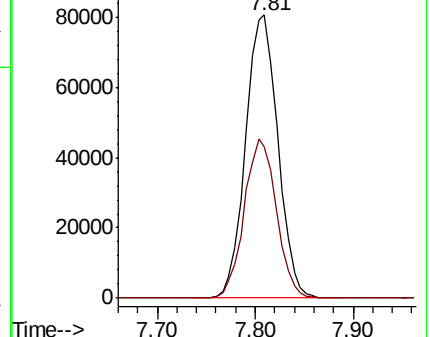

#33

1,2-Dichloroethane-d4

Concen: 55.223 ug/l

RT: 8.16 min Scan# 1053

Delta R.T. -0.01 min

Lab File: VY001579.D


Acq: 10 Feb 2020 12:31

Tgt Ion: 65 Resp: 102560

Ion Ratio Lower Upper



65 100


67 55.8 0.0 108.6

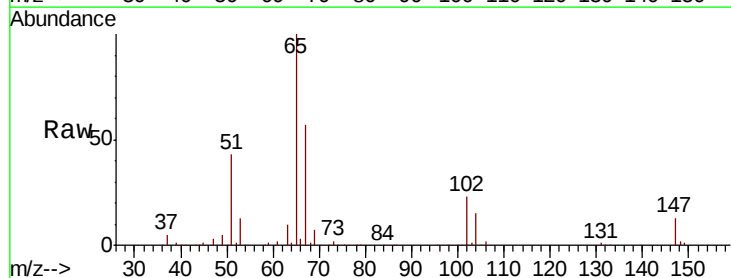

Abundance Ion 64.90 (64.60 to 65.60): VY001579.D (-1005) (-)

Ion 66.90 (66.60 to 67.60): VY001579.D (-1005) (-)



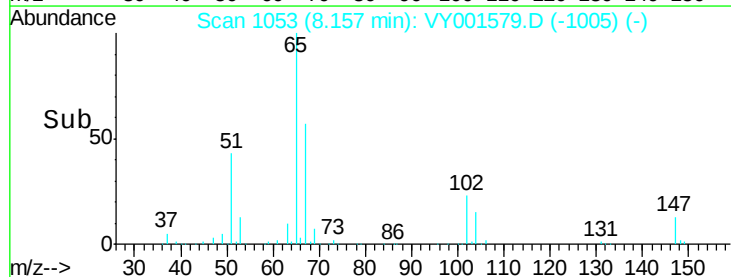
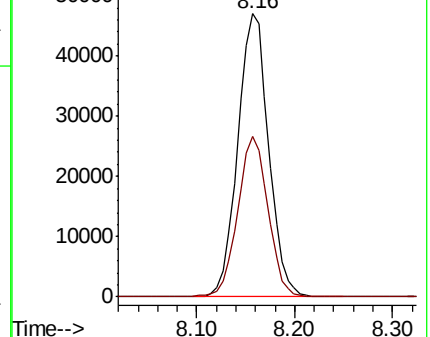


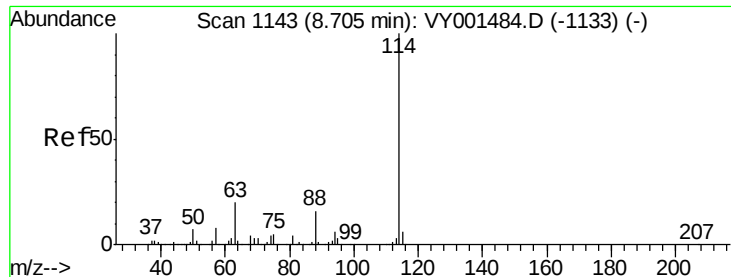

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.71 min Scan# 1143
 Delta R.T. 0.00 min
 Lab File: VY001579.D
 Acq: 10 Feb 2020 12:31




Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0210SBL01


Tot Ion	Ratio	Lower	Upper
114	100		
63	19.5	0.0	39.8
88	15.4	0.0	32.6

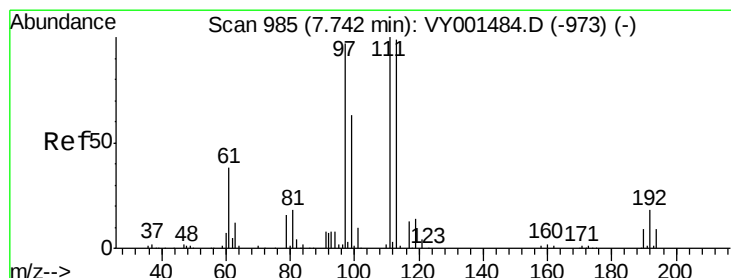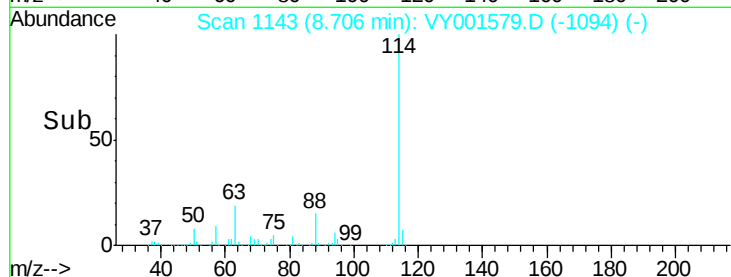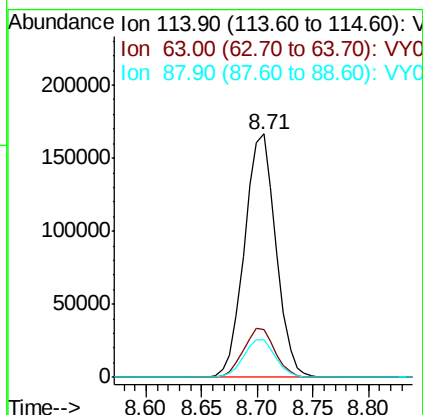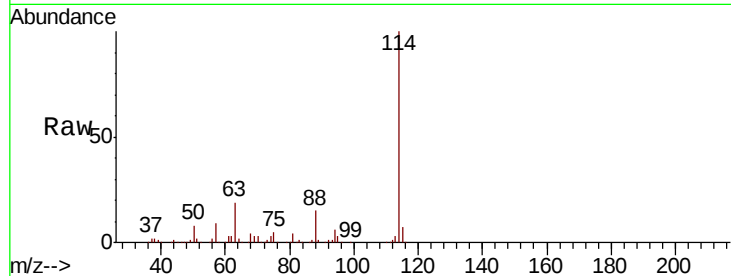

#35
 Dibromofluoromethane
 Concen: 50.718 ug/l
 RT: 7.74 min Scan# 984
 Delta R.T. -0.01 min
 Lab File: VY001579.D
 Acq: 10 Feb 2020 12:31

Tgt Ion	Ratio	Lower	Upper
113	100		
111	104.1	82.9	124.3
192	19.3	14.6	22.0

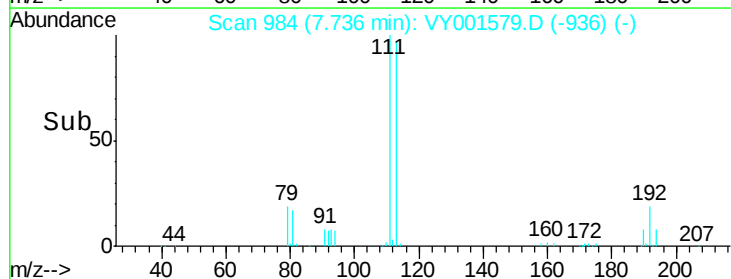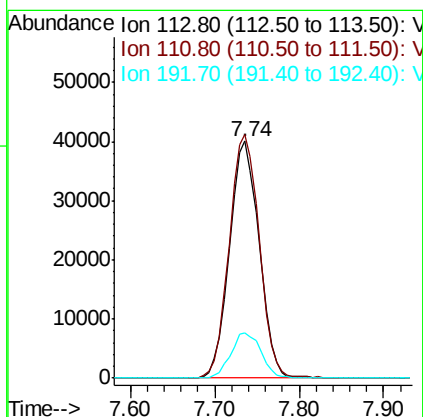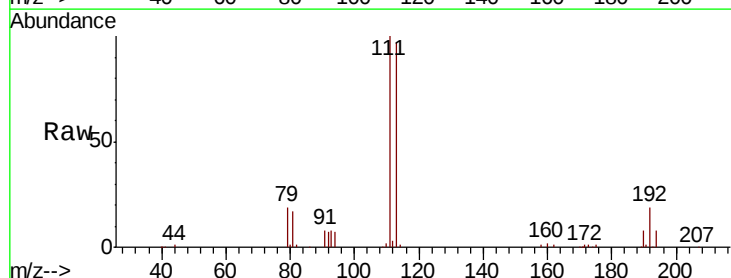

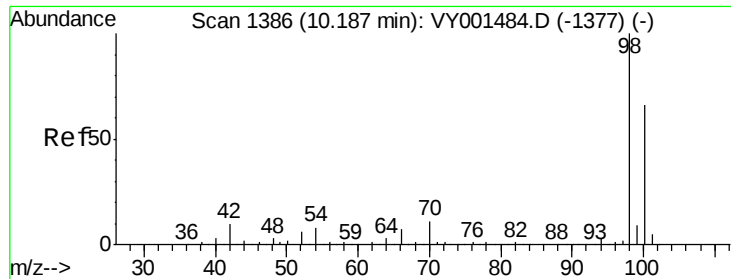

#50

Toluene-d8

Concen: 55.706 ug/l

RT: 10.19 min Scan# 1386

Delta R.T. 0.00 min

Lab File: VY001579.D

Acq: 10 Feb 2020 12:31

Instrument :

MSVOA_Y

ClientSampleId :


VY0210SBL01

Tot Ion: 98 Resp: 396713

Ion Ratio Lower Upper

98 100

100 65.5 53.0 79.6

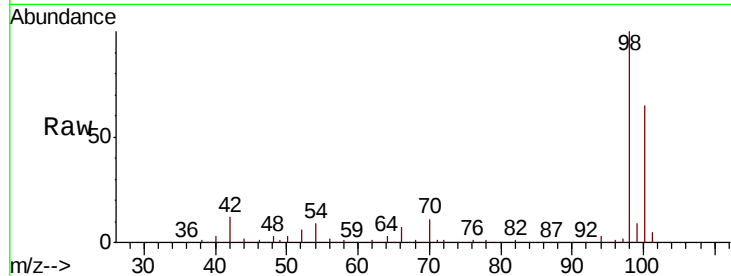

Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY

250000

200000

150000



100000

50000

0

10.10 10.20 10.30

Time-->

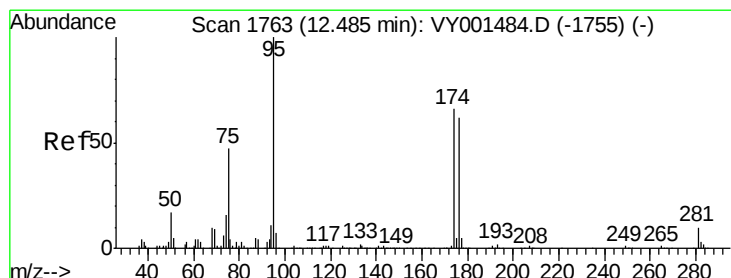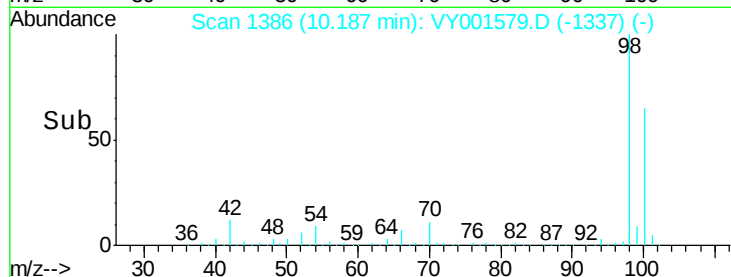

#62

4-Bromofluorobenzene

Concen: 47.392 ug/l

RT: 12.49 min Scan# 1764

Delta R.T. 0.01 min

Lab File: VY001579.D

Acq: 10 Feb 2020 12:31


Tgt Ion: 95 Resp: 132957

Ion Ratio Lower Upper

95 100

174 74.3 0.0 141.4

176 71.4 0.0 135.4

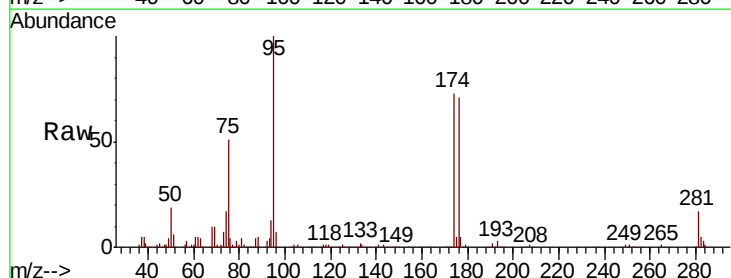

Abundance Ion 94.90 (94.60 to 95.60): VY0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

120000

100000

80000

60000


40000


20000

0

12.40 12.50

Time-->

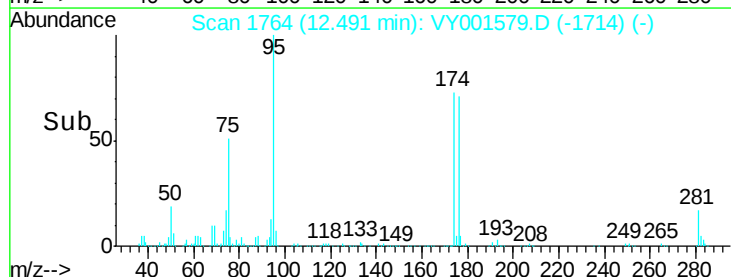


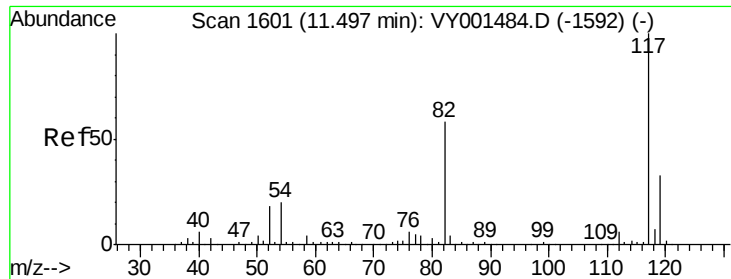




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1601
Delta R.T. 0.00 min
Lab File: VY001579.D
Acq: 10 Feb 2020 12:31

Instrument :
MSVOA_Y
ClientSampleId :
VY0210SBL01

Tot Ion:117 Resp: 290397
Ion Ratio Lower Upper
117 100
82 57.6 46.1 69.1
119 31.8 26.1 39.1

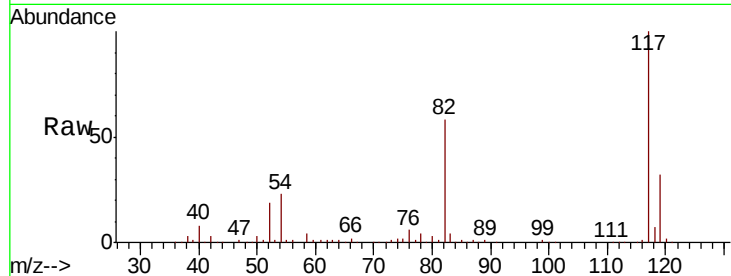


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

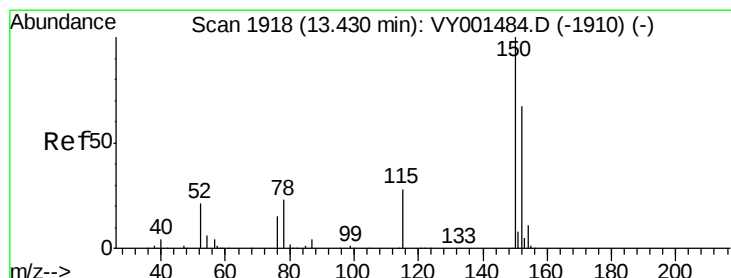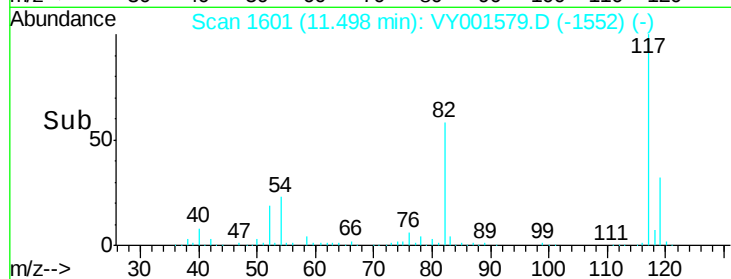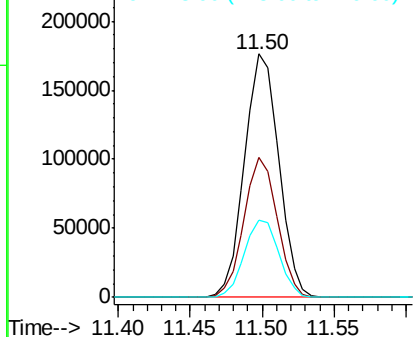

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.44 min Scan# 1919
Delta R.T. 0.01 min
Lab File: VY001579.D
Acq: 10 Feb 2020 12:31

Tgt Ion:152 Resp: 126340
Ion Ratio Lower Upper
152 100
115 59.9 31.4 94.3
150 157.7 0.0 346.8

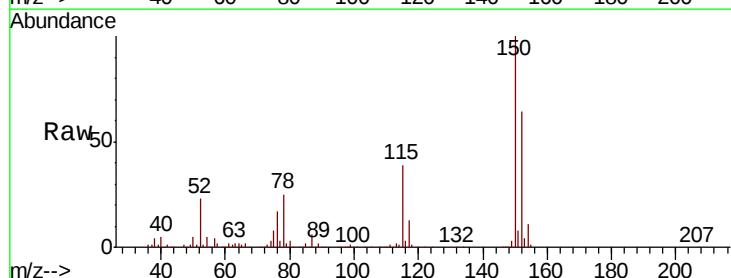

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

