

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021121\
 Data File : VY004003.D
 Acq On : 11 Feb 2021 16:00
 Operator : SY/MD
 Sample : M1393-01
 Misc : 4.70g/5mL/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 R-LA-3-1-WC

Quant Time: Feb 11 16:09:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012821S.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 01 00:38:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	167906	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	296033	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	281888	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	133241	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	115613	62.62	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	125.24%
35) Dibromofluoromethane	7.722	113	90928	52.53	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.06%
50) Toluene-d8	10.179	98	368460	54.25	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.50%
62) 4-Bromofluorobenzene	12.477	95	128643	51.96	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	103.92%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021121\
Data File : VY004003.D
Acq On : 11 Feb 2021 16:00
Operator : SY/MD
Sample : M1393-01
Misc : 4.70g/5mL/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
R-LA-3-1-WC

Quant Time: Feb 11 16:09:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012821S.M
Quant Title : SW846 8260
QLast Update : Mon Feb 01 00:38:02 2021
Response via : Initial Calibration




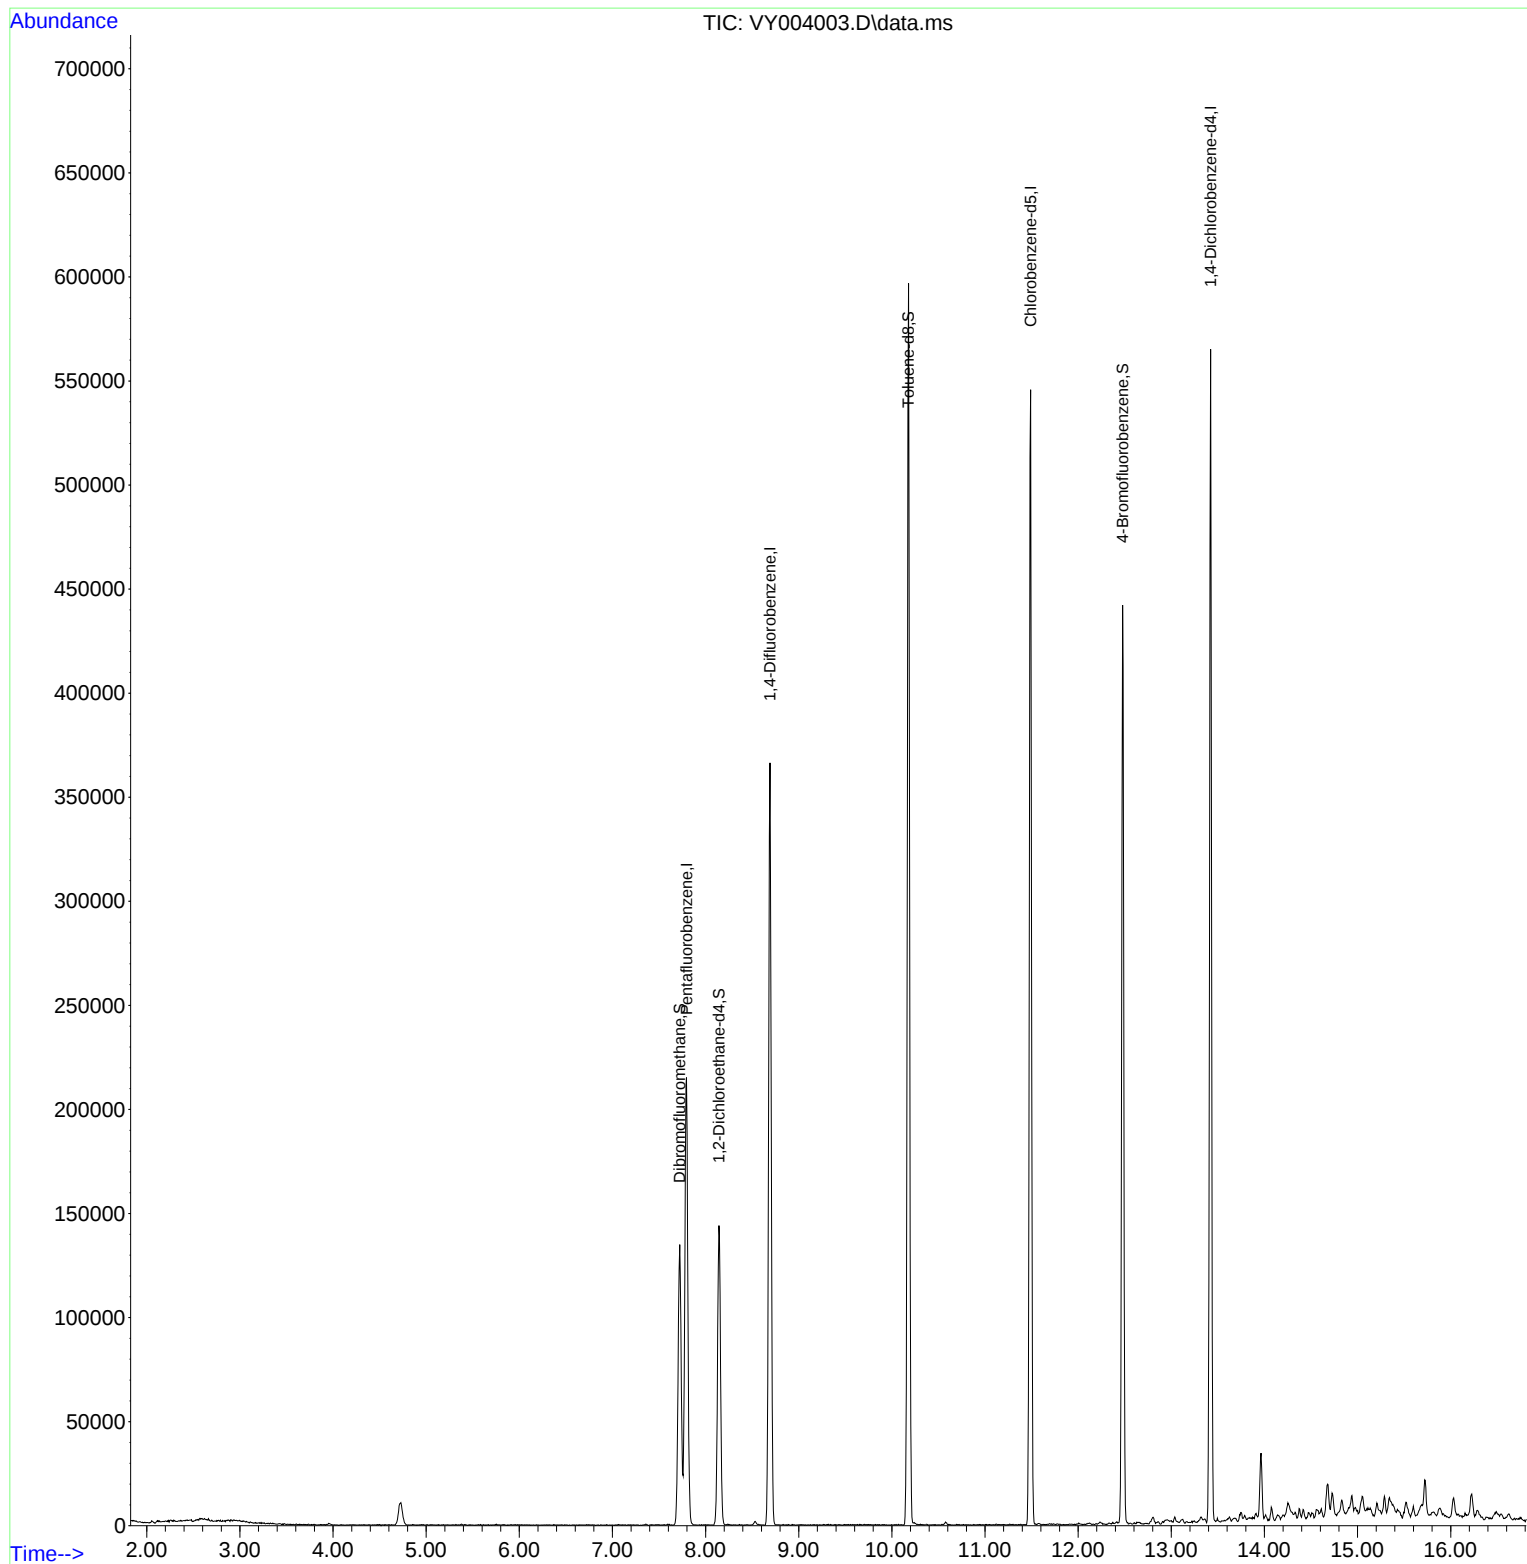


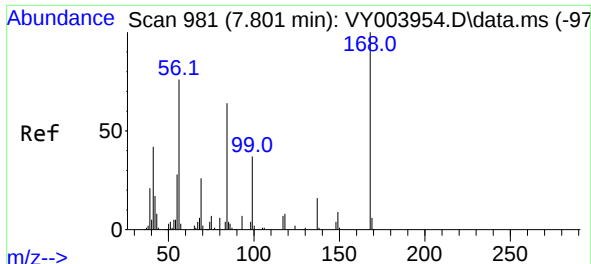

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.006 min
Lab File: VY004003.D
Acq: 11 Feb 2021 16:00




Instrument :
MSVOA_Y
ClientSampleId :
R-LA-3-1-WC


Tgt Ion:168 Resp: 167906
Ion Ratio Lower Upper
168 100
99 53.5 46.1 69.1

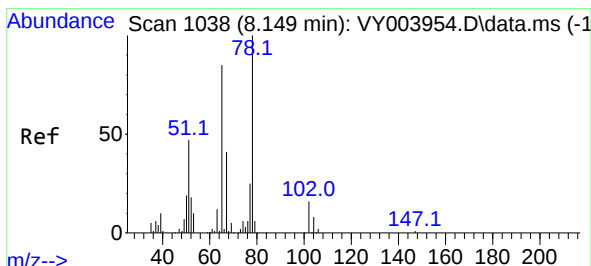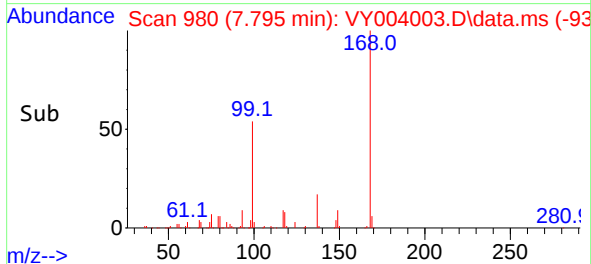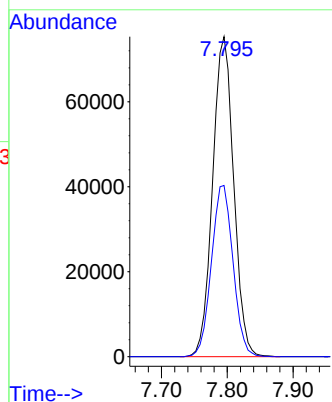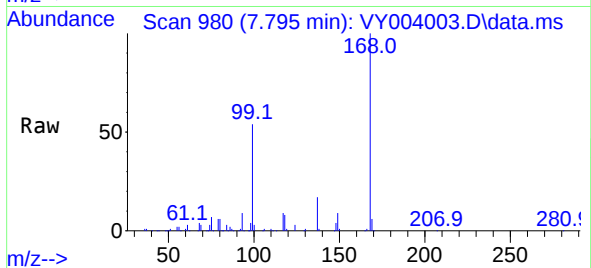

#33
1,2-Dichloroethane-d4
Concen: 62.62 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.006 min
Lab File: VY004003.D
Acq: 11 Feb 2021 16:00

Tgt Ion: 65 Resp: 115613
Ion Ratio Lower Upper
65 100
67 51.4 0.0 101.8


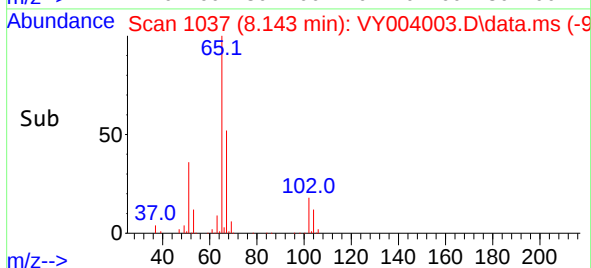
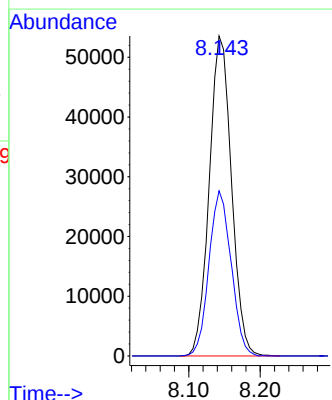
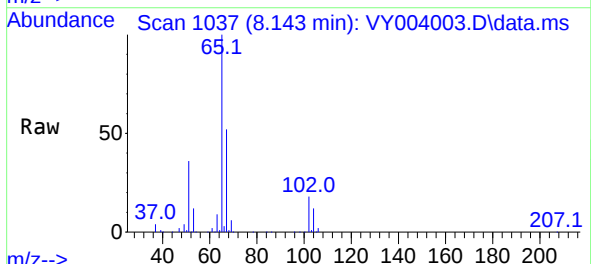


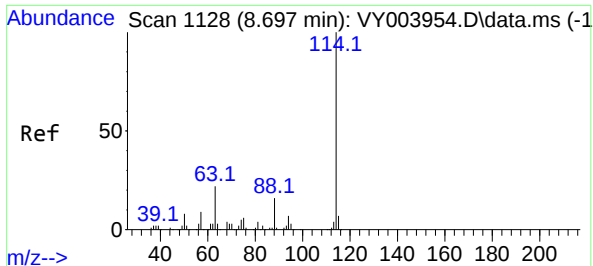

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. -0.006 min
Lab File: VY004003.D
Acq: 11 Feb 2021 16:00




Instrument :
MSVOA_Y
ClientSampleId :
R-LA-3-1-WC


Tgt Ion:	114	Resp:	296033
Ion	Ratio	Lower	Upper
114	100		
63	22.0	0.0	47.2
88	16.3	0.0	30.2

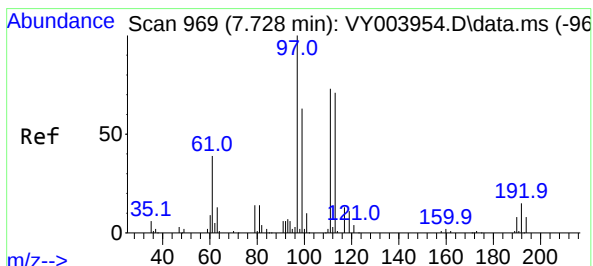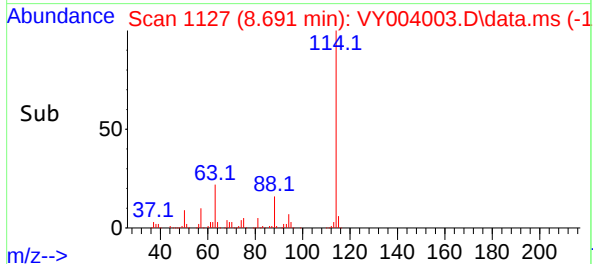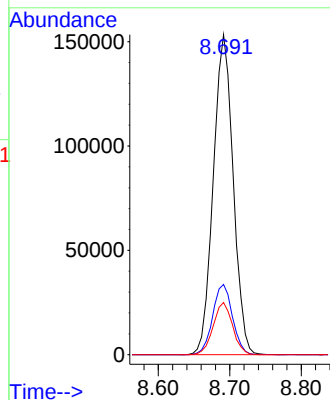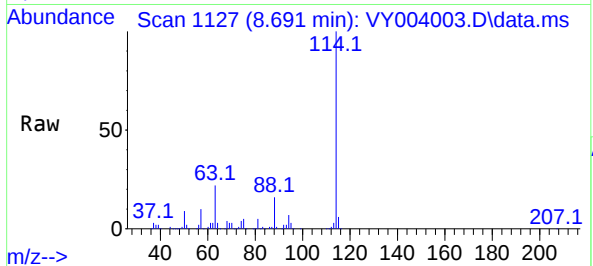

#35
Dibromofluoromethane
Concen: 52.53 ug/l
RT: 7.722 min Scan# 968
Delta R.T. -0.006 min
Lab File: VY004003.D
Acq: 11 Feb 2021 16:00

Tgt Ion:	113	Resp:	90928
Ion	Ratio	Lower	Upper
113	100		
111	103.9	82.2	123.4
192	22.0	18.3	27.5


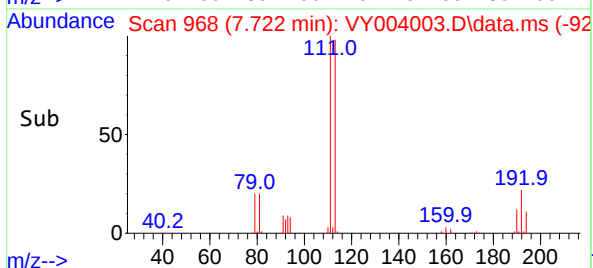
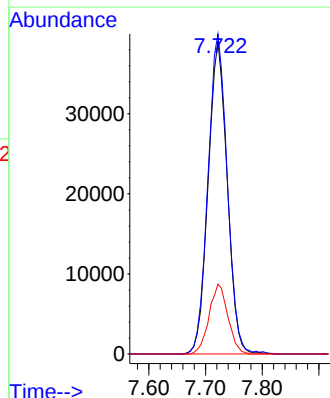
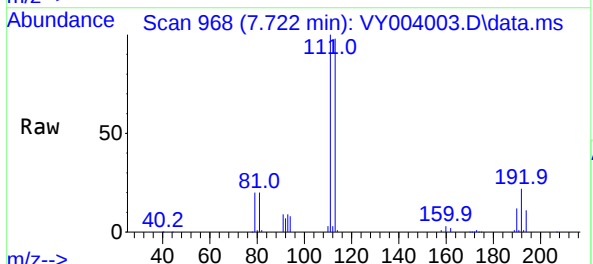


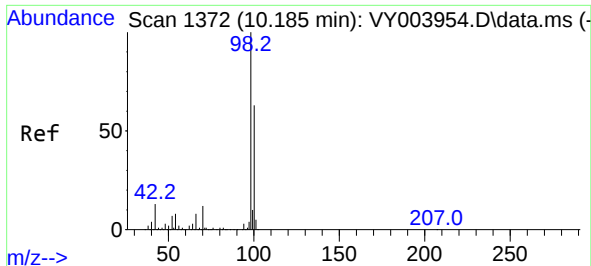

#50
Toluene-d8
Concen: 54.25 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.006 min
Lab File: VY004003.D
Acq: 11 Feb 2021 16:00




Instrument :
MSVOA_Y
ClientSampleId :
R-LA-3-1-WC


Tgt Ion: 98 Resp: 368460
Ion Ratio Lower Upper
98 100
100 64.0 50.5 75.7

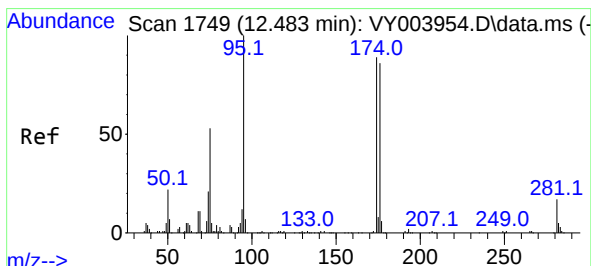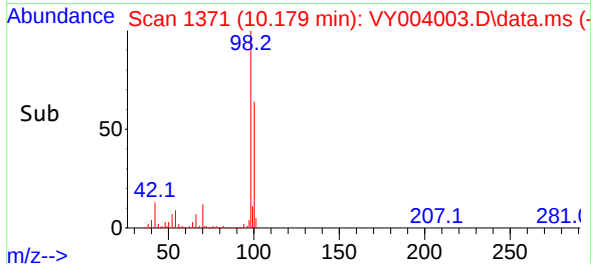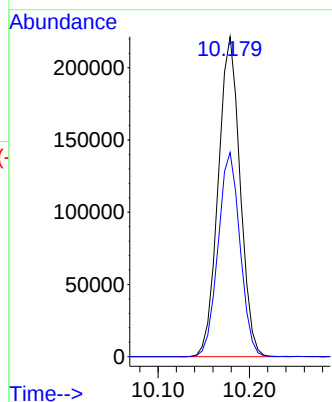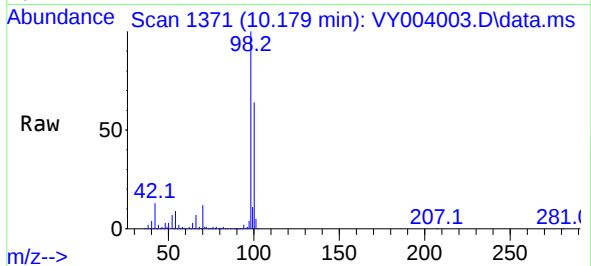

#62
4-Bromofluorobenzene
Concen: 51.96 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY004003.D
Acq: 11 Feb 2021 16:00

Tgt Ion: 95 Resp: 128643
Ion Ratio Lower Upper
95 100
174 88.2 0.0 184.4
176 86.0 0.0 177.2


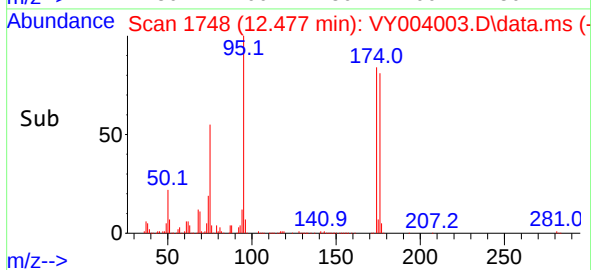
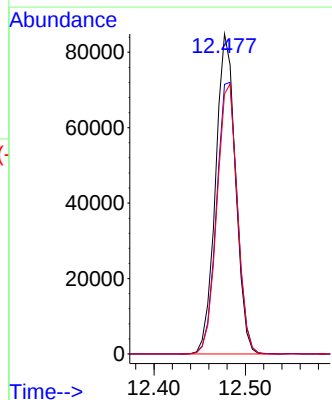
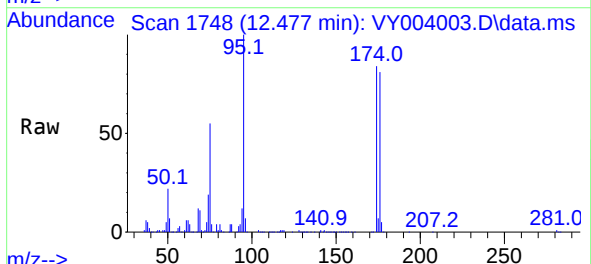


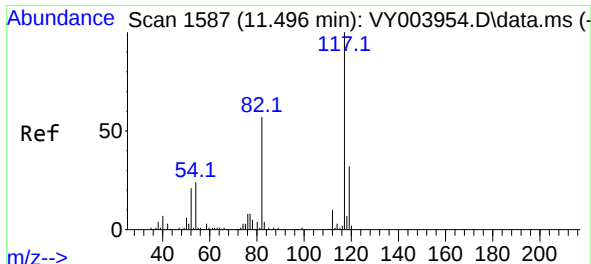

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.007 min
Lab File: VY004003.D
Acq: 11 Feb 2021 16:00

Instrument :
MSVOA_Y
ClientSampleId :
R-LA-3-1-WC

Tgt Ion:	117	Resp:	281888
Ion	Ratio	Lower	Upper
117	100		
82	56.5	44.3	66.5
119	30.8	25.0	37.6

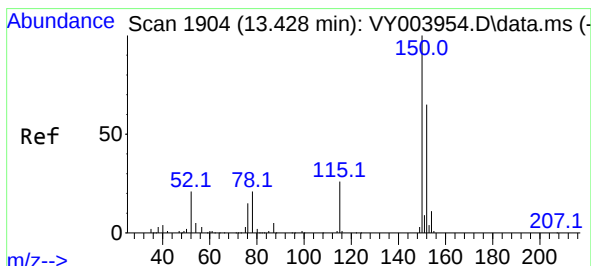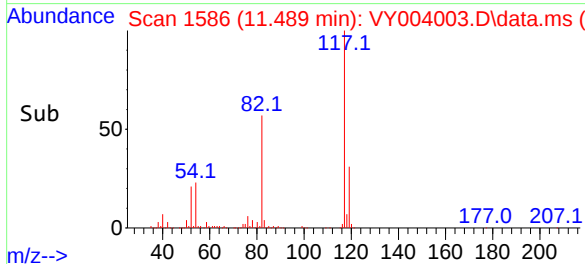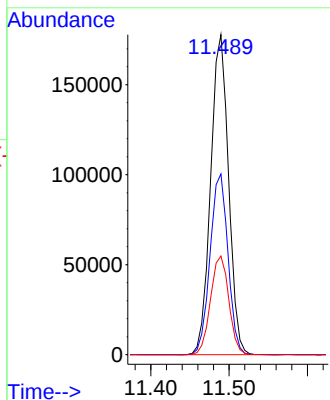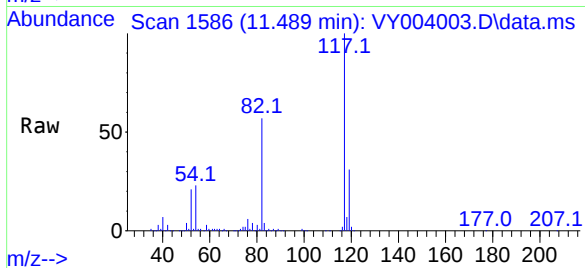

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY004003.D
Acq: 11 Feb 2021 16:00

Tgt Ion:	152	Resp:	133241
Ion	Ratio	Lower	Upper
152	100		
115	57.9	28.2	84.6
150	158.9	0.0	356.2

