

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY021220\
 Data File : VY001615.D
 Acq On : 12 Feb 2020 17:13
 Operator : SY/MD
 Sample : L1385-01
 Misc : 7.33G/5ML/MSVOA Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 HD-02-021220

Quant Time: Feb 13 08:18:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 04 15:10:08 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.81	168	53372	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	90512	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	74627	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.44	152	31907	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.16	65	27665	51.48	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.96%	
35) Dibromofluoromethane	7.74	113	25517	48.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.78%	
50) Toluene-d8	10.19	98	105198	53.27	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.54%	
62) 4-Bromofluorobenzene	12.49	95	33356	42.88	ug/l	0.00
Spiked Amount 50.000			Recovery	=	85.76%	
Target Compounds						
16) Acetone	3.97	43	2344	15.080	ug/l #	79
95) Naphthalene	15.25	128	2804	1.936	ug/l #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY021220\
Data File : VY001615.D
Acq On : 12 Feb 2020 17:13
Operator : SY/MD
Sample : L1385-01
Misc : 7.33G/5ML/MSVOA Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
HD-02-021220

Quant Time: Feb 13 08:18:08 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 04 15:10:08 2020
Response via : Initial Calibration

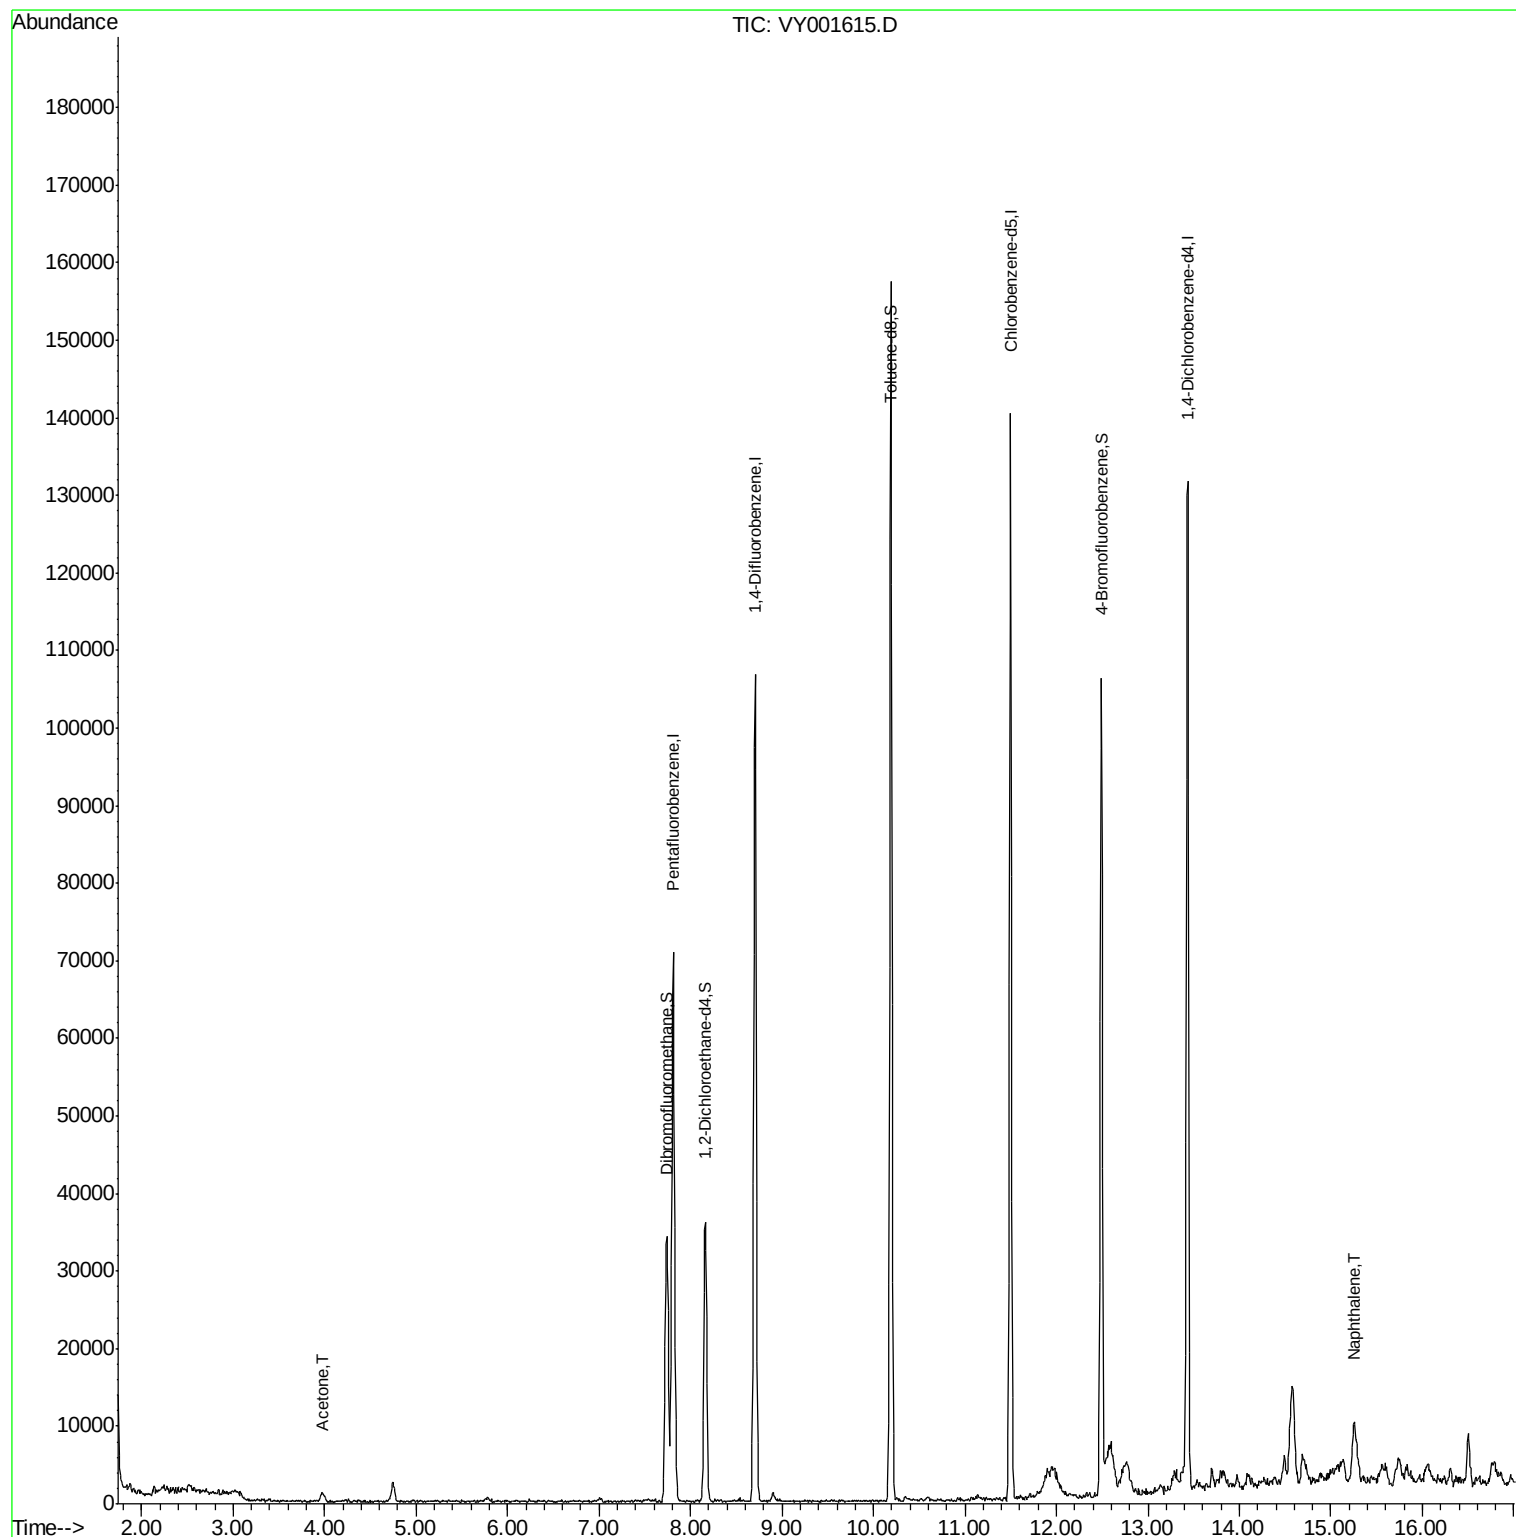

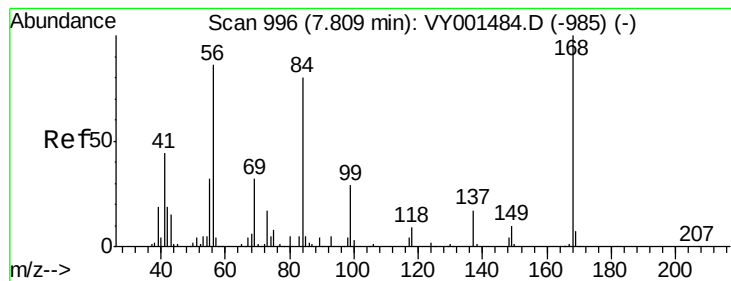

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.81 min Scan# 996

Delta R.T. 0.00 min

Lab File: VY001615.D

Acq: 12 Feb 2020 17:13

Instrument :

MSVOA_Y

ClientSampleId :


HD-02-021220

Tot Ion:168 Resp: 53372




Ion Ratio Lower Upper

168 100

99 56.7 48.2 72.4

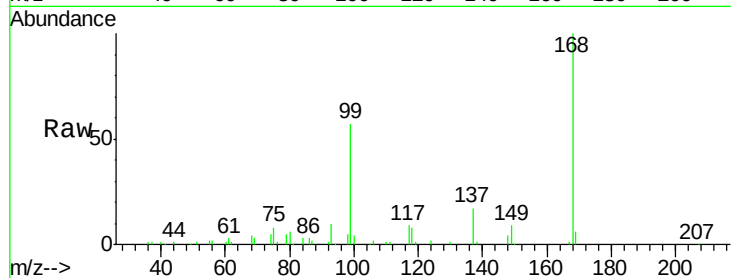

Abundance Ion 167.90 (167.60 to 168.60): VY001615.D (-947) (-)

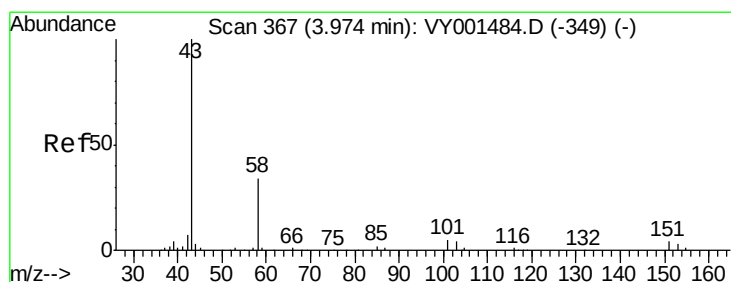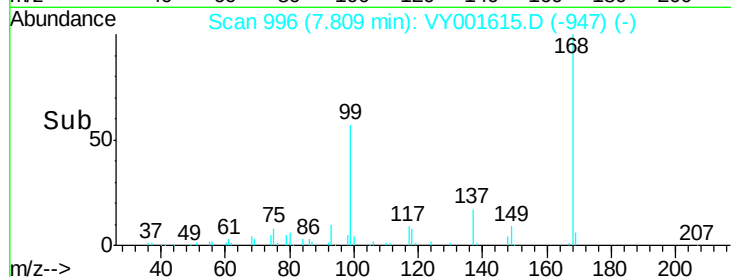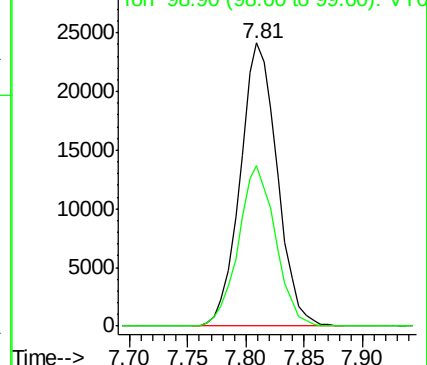

#16

Acetone

Concen: 15.080 ug/l

RT: 3.97 min Scan# 366

Delta R.T. -0.01 min

Lab File: VY001615.D


Acq: 12 Feb 2020 17:13

Tgt Ion: 43 Resp: 2344



Ion Ratio Lower Upper


43 100

58 22.5 27.5 41.3#

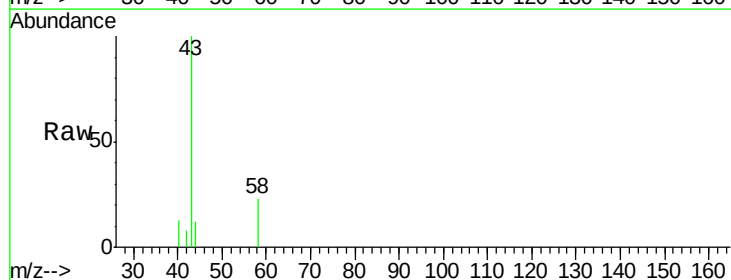

Abundance Ion 43.00 (42.70 to 43.70): VY001615.D (-318) (-)



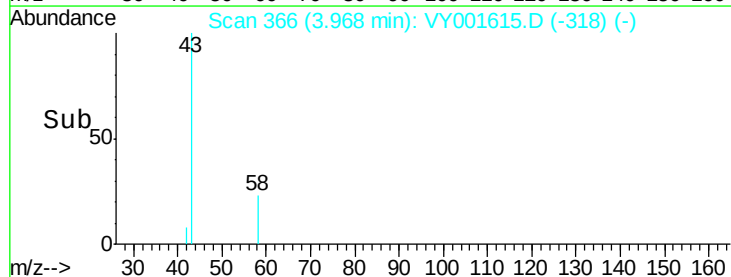
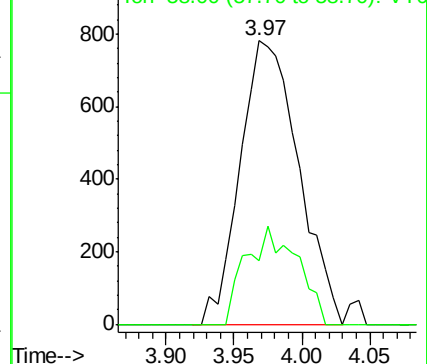


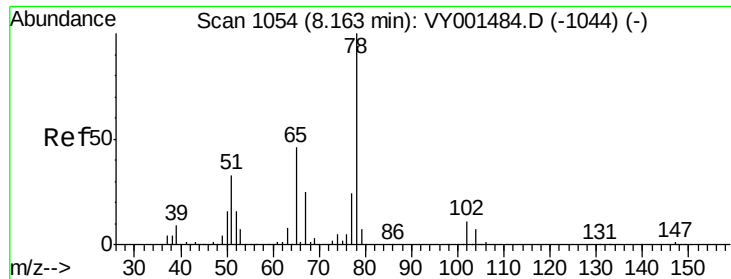

#33
 1,2-Dichloroethane-d4
 Concen: 51.481 ug/l
 RT: 8.16 min Scan# 1054
 Delta R.T. 0.00 min
 Lab File: VY001615.D
 Acq: 12 Feb 2020 17:13




Instrument :
 MSVOA_Y
 ClientSampleId :
 HD-02-021220


Tot Ion: 65 Resp: 27665
 Ion Ratio Lower Upper
 65 100
 67 53.9 0.0 108.6

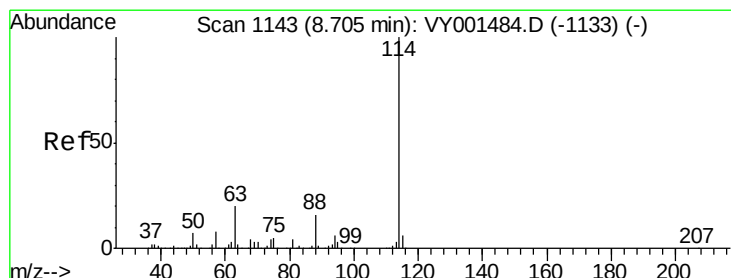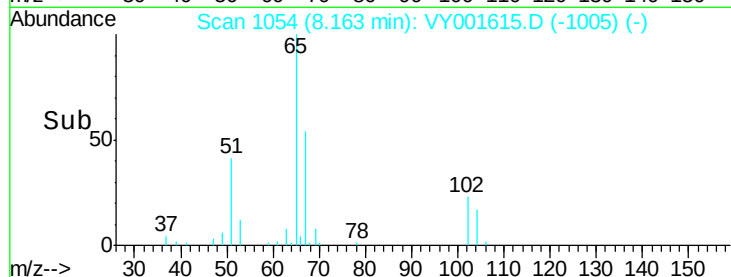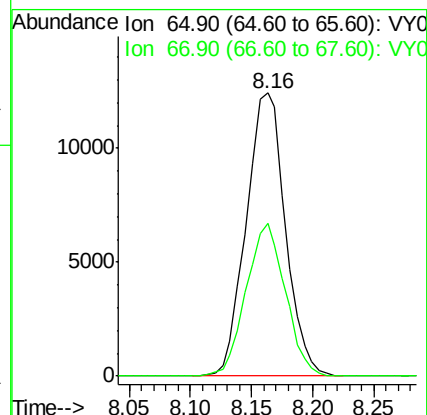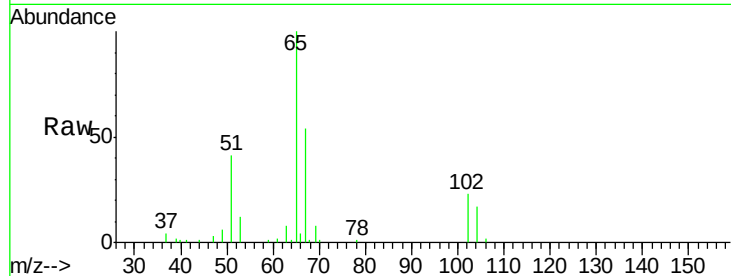

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.71 min Scan# 1143
 Delta R.T. 0.00 min
 Lab File: VY001615.D
 Acq: 12 Feb 2020 17:13

Tgt Ion: 114 Resp: 90512
 Ion Ratio Lower Upper
 114 100
 63 21.3 0.0 39.8
 88 15.9 0.0 32.6

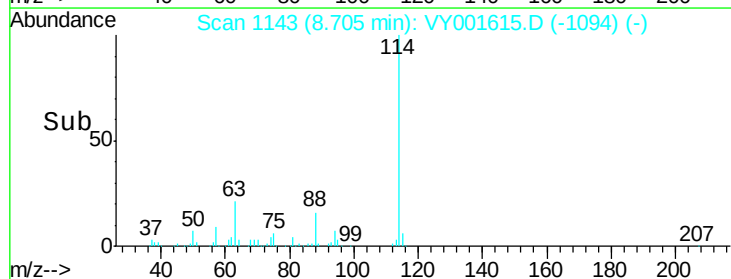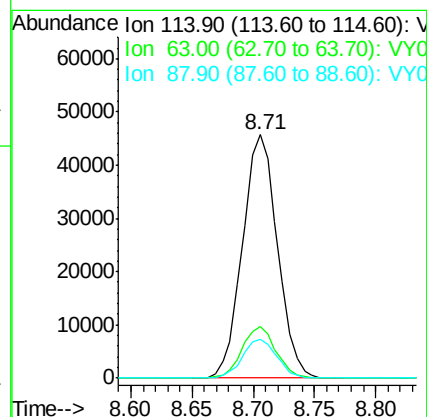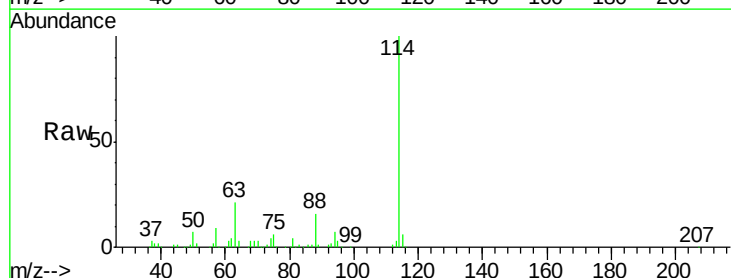


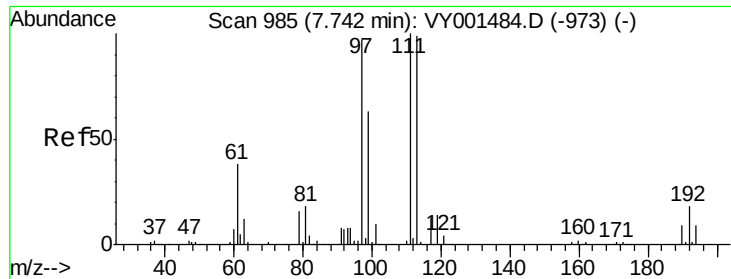




#35
 Dibromofluoromethane
 Concen: 48.889 ug/l
 RT: 7.74 min Scan# 985
 Delta R.T. 0.00 min
 Lab File: VY001615.D
 Acq: 12 Feb 2020 17:13

Instrument :
 MSVOA_Y
 ClientSampled :
 HD-02-021220

Tot Ion	Ratio	Lower	Upper
113	100		
111	99.7	82.9	124.3
192	17.6	14.6	22.0

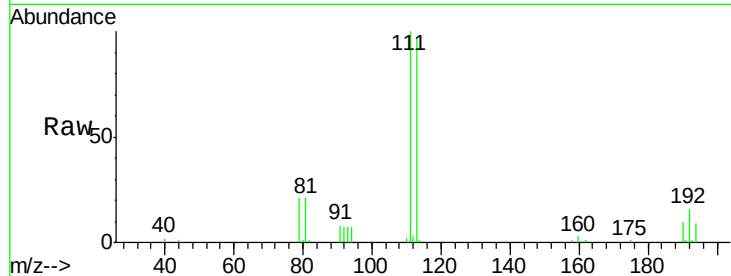


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

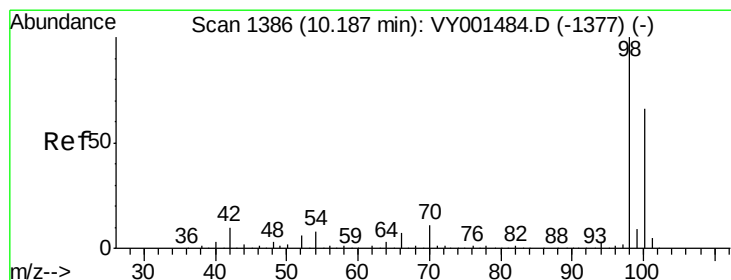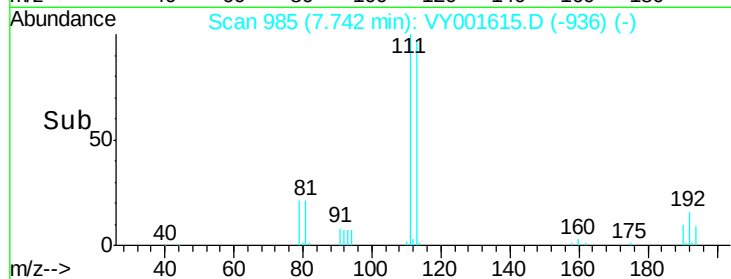
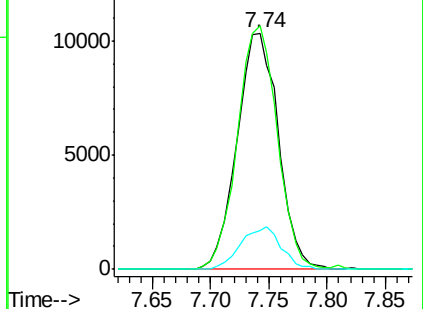



#50
 Toluene-d8
 Concen: 53.273 ug/l
 RT: 10.19 min Scan# 1387
 Delta R.T. 0.01 min
 Lab File: VY001615.D
 Acq: 12 Feb 2020 17:13

Tgt Ion	Ratio	Lower	Upper
98	100		
100	66.4	53.0	79.6

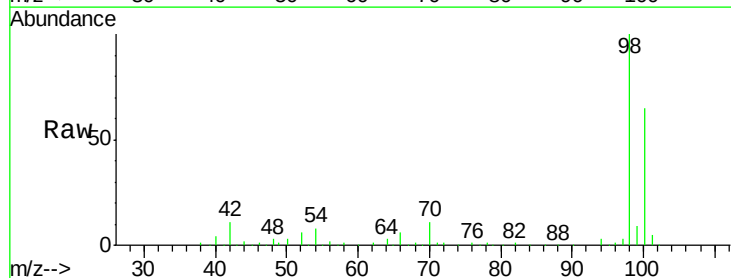

Abundance Ion 98.00 (97.70 to 98.70): VY0
 Ion 100.00 (99.70 to 100.70): VY



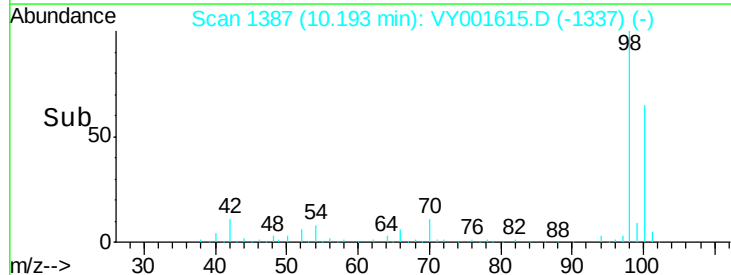
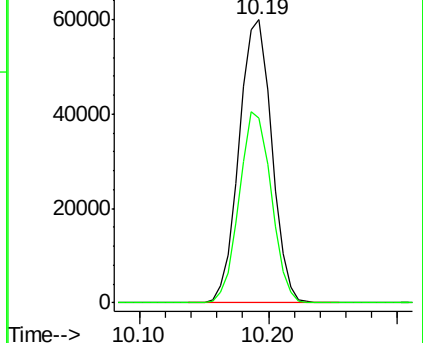


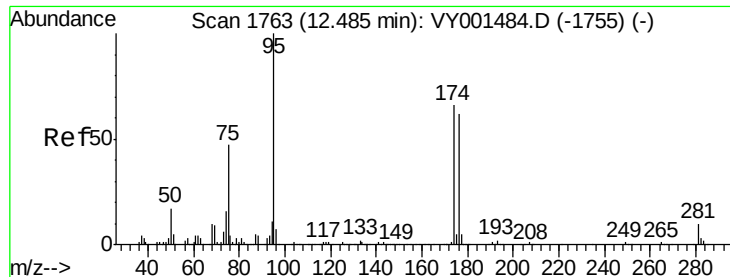

#62
4-Bromofluorobenzene
Concen: 42.878 ug/l
RT: 12.49 min Scan# 1764
Delta R.T. 0.01 min
Lab File: VY001615.D
Acq: 12 Feb 2020 17:13




Instrument :
MSVOA_Y
ClientSampleId :
HD-02-021220


Tot Ion: 95 Resp: 33356
Ion Ratio Lower Upper
95 100
174 73.8 0.0 141.4
176 72.8 0.0 135.4

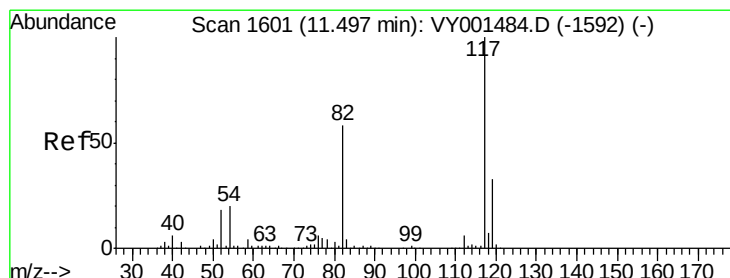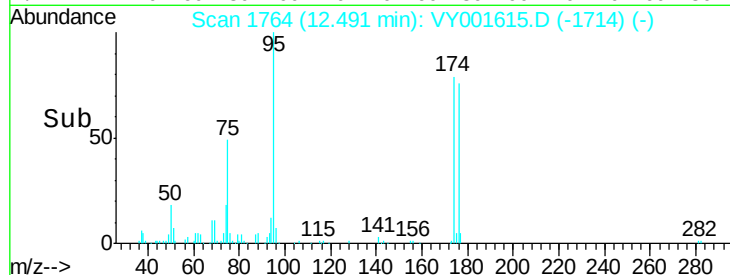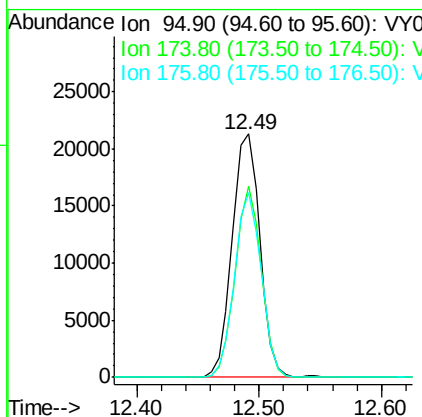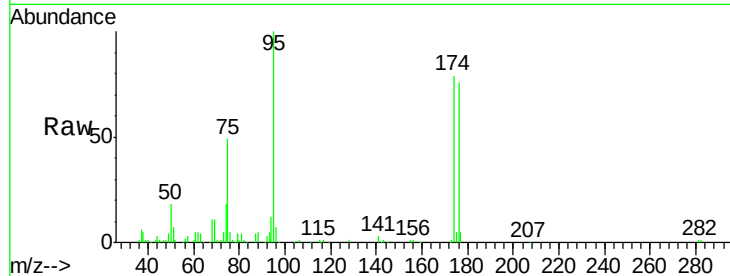

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1601
Delta R.T. 0.00 min
Lab File: VY001615.D
Acq: 12 Feb 2020 17:13

Tgt Ion: 117 Resp: 74627
Ion Ratio Lower Upper
117 100
82 57.7 46.1 69.1
119 30.6 26.1 39.1

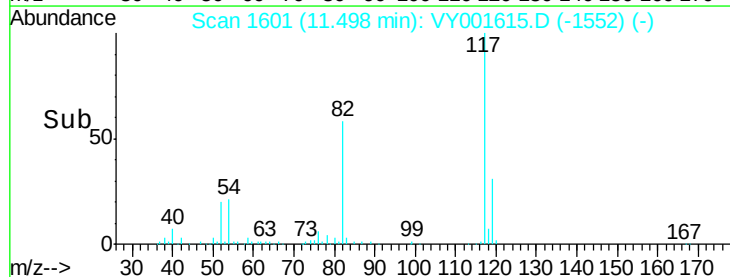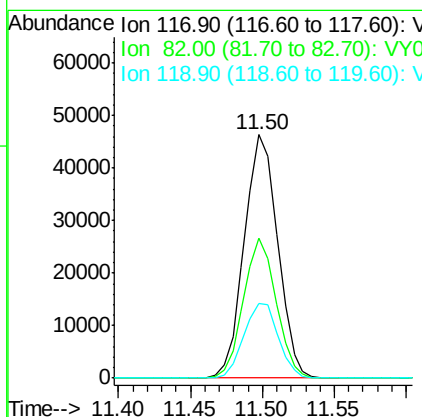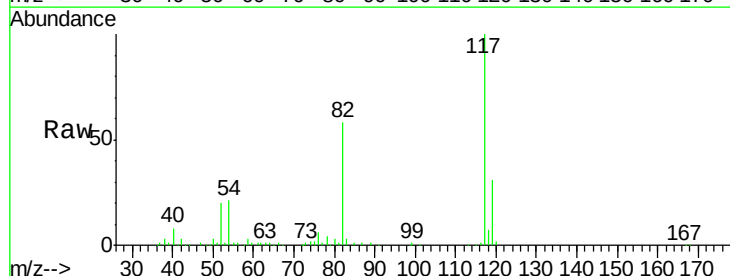

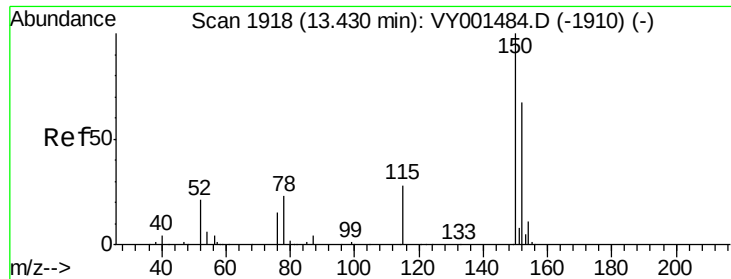

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.44 min Scan# 1919

Delta R.T. 0.01 min

Lab File: VY001615.D

Acq: 12 Feb 2020 17:13

Instrument :

MSVOA_Y

ClientSampleId :

HD-02-021220


Tot Ion:152 Resp: 31907

Ion Ratio Lower Upper

152 100

115 64.2 31.4 94.3




150 157.9 0.0 346.8

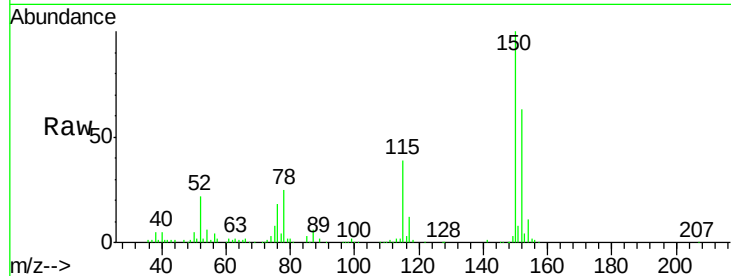

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

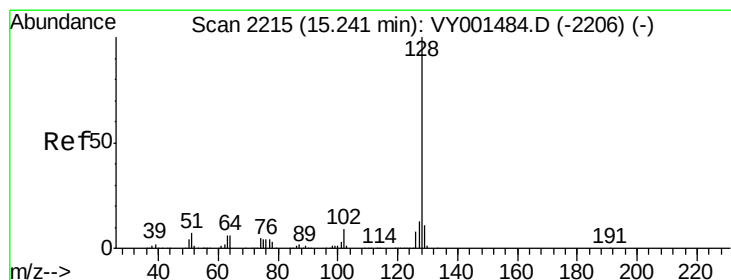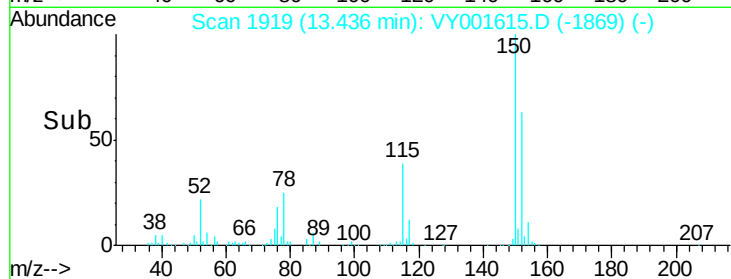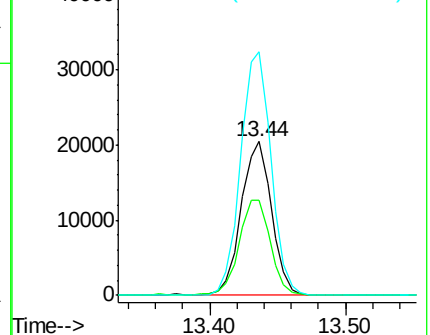

#95

Naphthalene

Concen: 1.936 ug/l

RT: 15.25 min Scan# 2216

Delta R.T. 0.01 min

Lab File: VY001615.D

Acq: 12 Feb 2020 17:13


Tgt Ion:128 Resp: 2804

Ion Ratio Lower Upper

128 100

127 10.9 10.1 15.1

129 21.3 8.9 13.3#

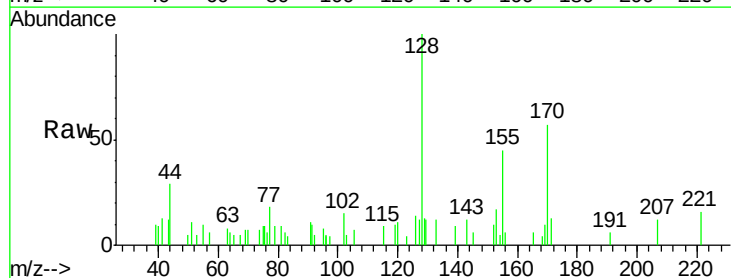

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

