
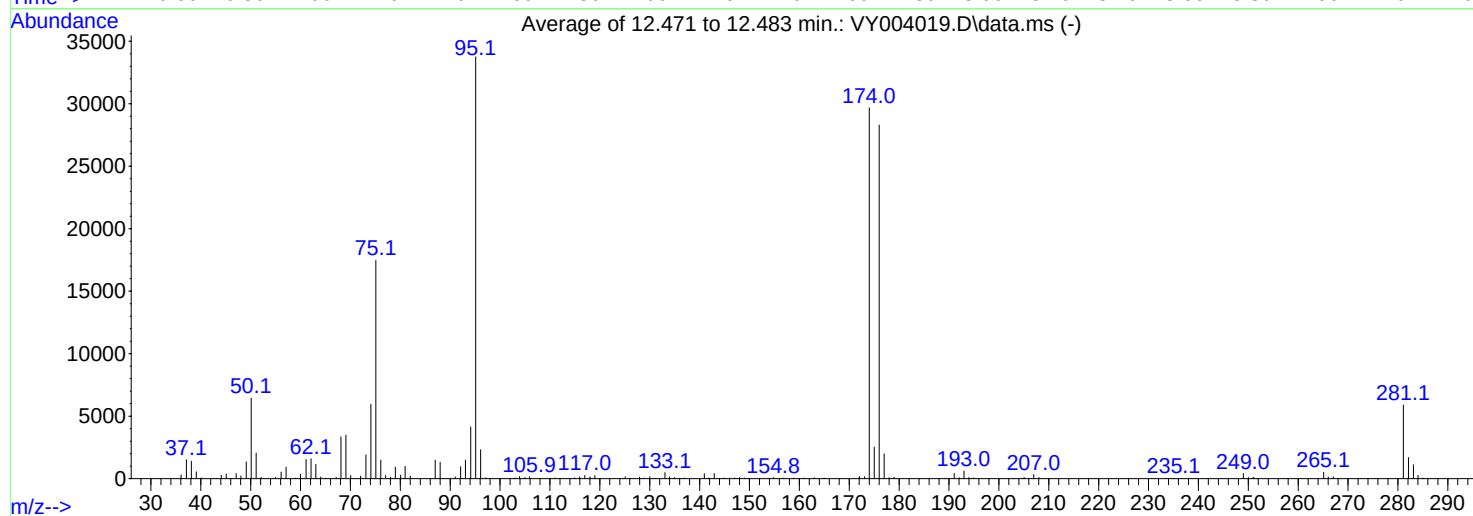


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021221\
Data File : VY004019.D
Acq On : 12 Feb 2021 12:16
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012821S.M
Title : SW846 8260
Last Update : Mon Feb 01 00:38:02 2021

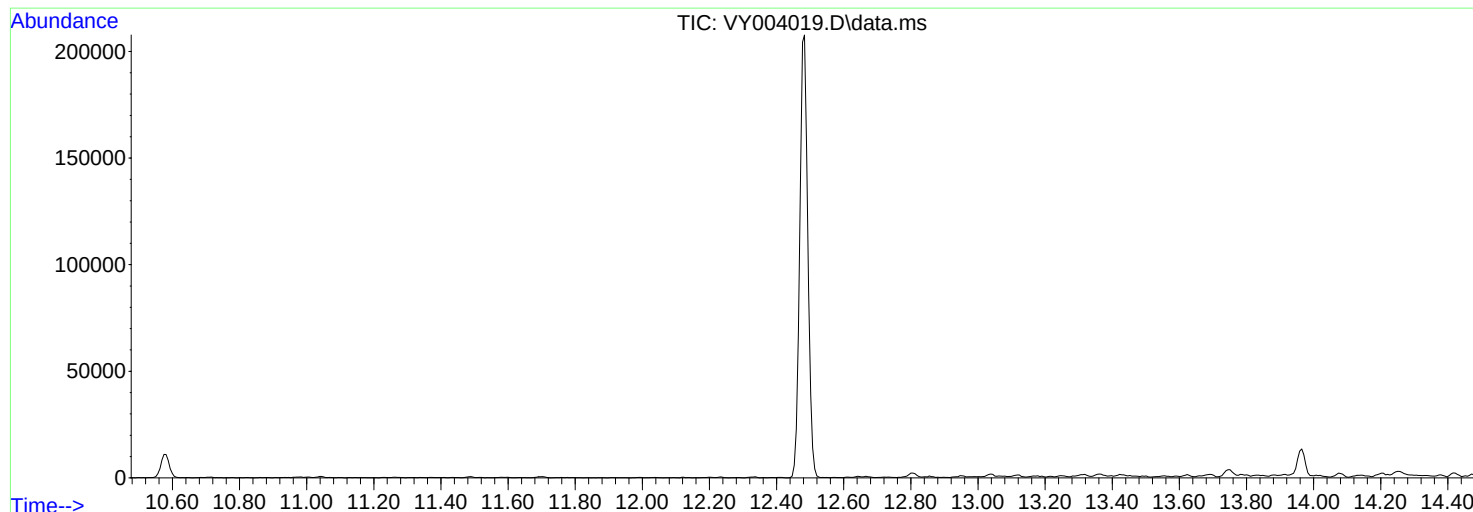

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	6444	PASS
75	95	30	60	51.7	17465	PASS
95	95	100	100	100.0	33752	PASS
96	95	5	9	6.9	2325	PASS
173	174	0.00	2	0.6	169	PASS
174	95	50	100	87.9	29683	PASS
175	174	5	9	8.5	2526	PASS
176	174	95	101	95.3	28301	PASS
177	176	5	9	7.0	1985	PASS