
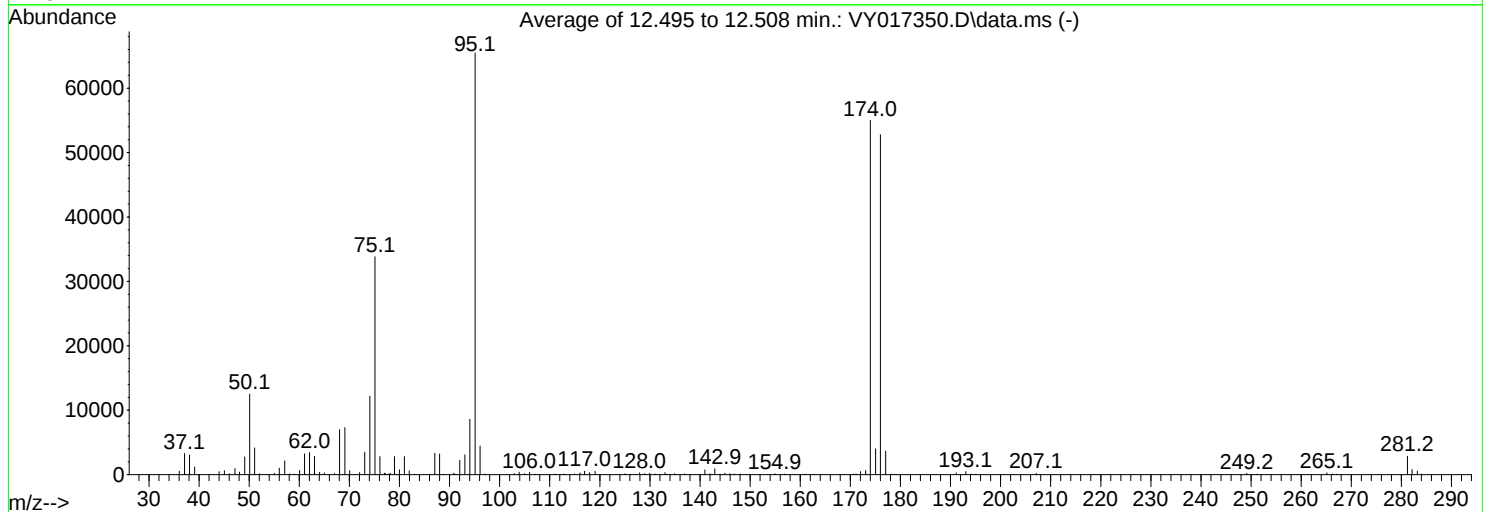


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021224\
Data File : VY017350.D
Acq On : 12 Feb 2024 08:28
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020124S.M
Title : SW846 8260
Last Update : Fri Feb 02 00:56:04 2024

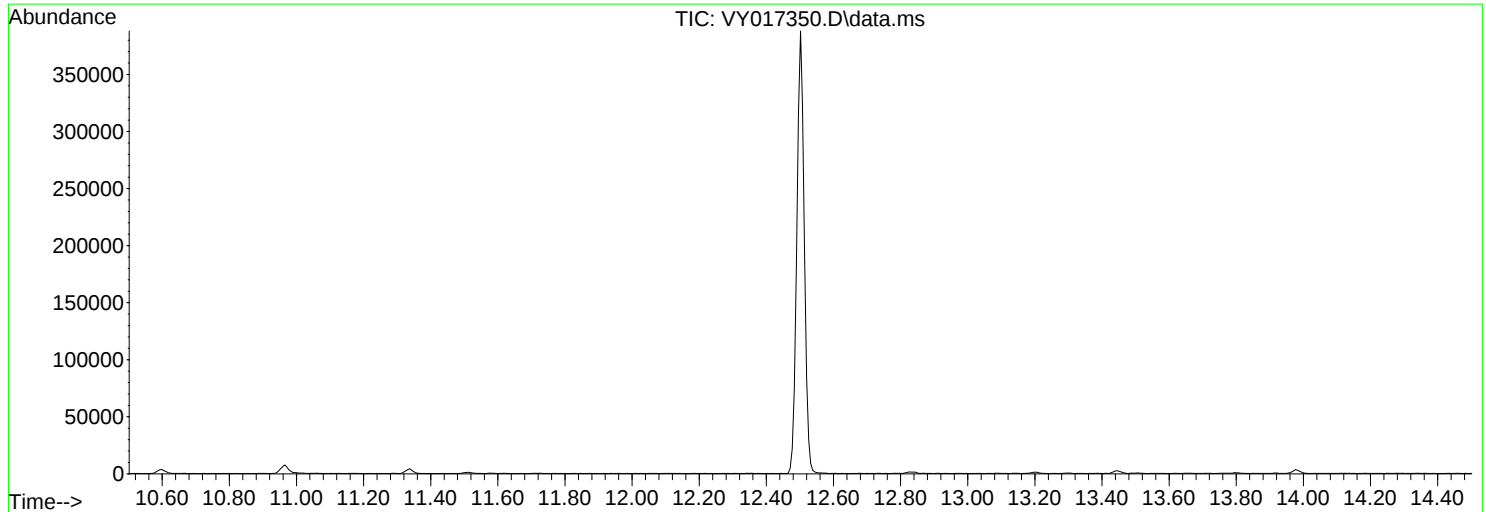

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	12495	PASS
75	95	30	60	51.7	33845	PASS
95	95	100	100	100.0	65485	PASS
96	95	5	9	6.8	4444	PASS
173	174	0.00	2	1.2	639	PASS
174	95	50	100	84.0	54989	PASS
175	174	5	9	7.3	4001	PASS
176	174	95	101	96.0	52789	PASS
177	176	5	9	6.9	3648	PASS