

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY021320\
 Data File : VY001628.D
 Acq On : 13 Feb 2020 16:07
 Operator : SY/MD
 Sample : L1528-04
 Misc : 5.27G/5ML/MSVOA Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 FK-GF-02-048-B

Quant Time: Feb 14 06:55:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 04 15:10:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.81	168	107550	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	181129	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	152111	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.44	152	62854	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.16	65	56721	52.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.76%	
35) Dibromofluoromethane	7.74	113	50922	48.75	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.50%	
50) Toluene-d8	10.19	98	214182	54.20	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.40%	
62) 4-Bromofluorobenzene	12.49	95	66071	42.44	ug/l	0.00
Spiked Amount	50.000		Recovery	=	84.88%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY021320\
Data File : VY001628.D
Acq On : 13 Feb 2020 16:07
Operator : SY/MD
Sample : L1528-04
Misc : 5.27G/5ML/MSVOA Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
FK-GF-02-048-B

Quant Time: Feb 14 06:55:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 04 15:10:08 2020
Response via : Initial Calibration

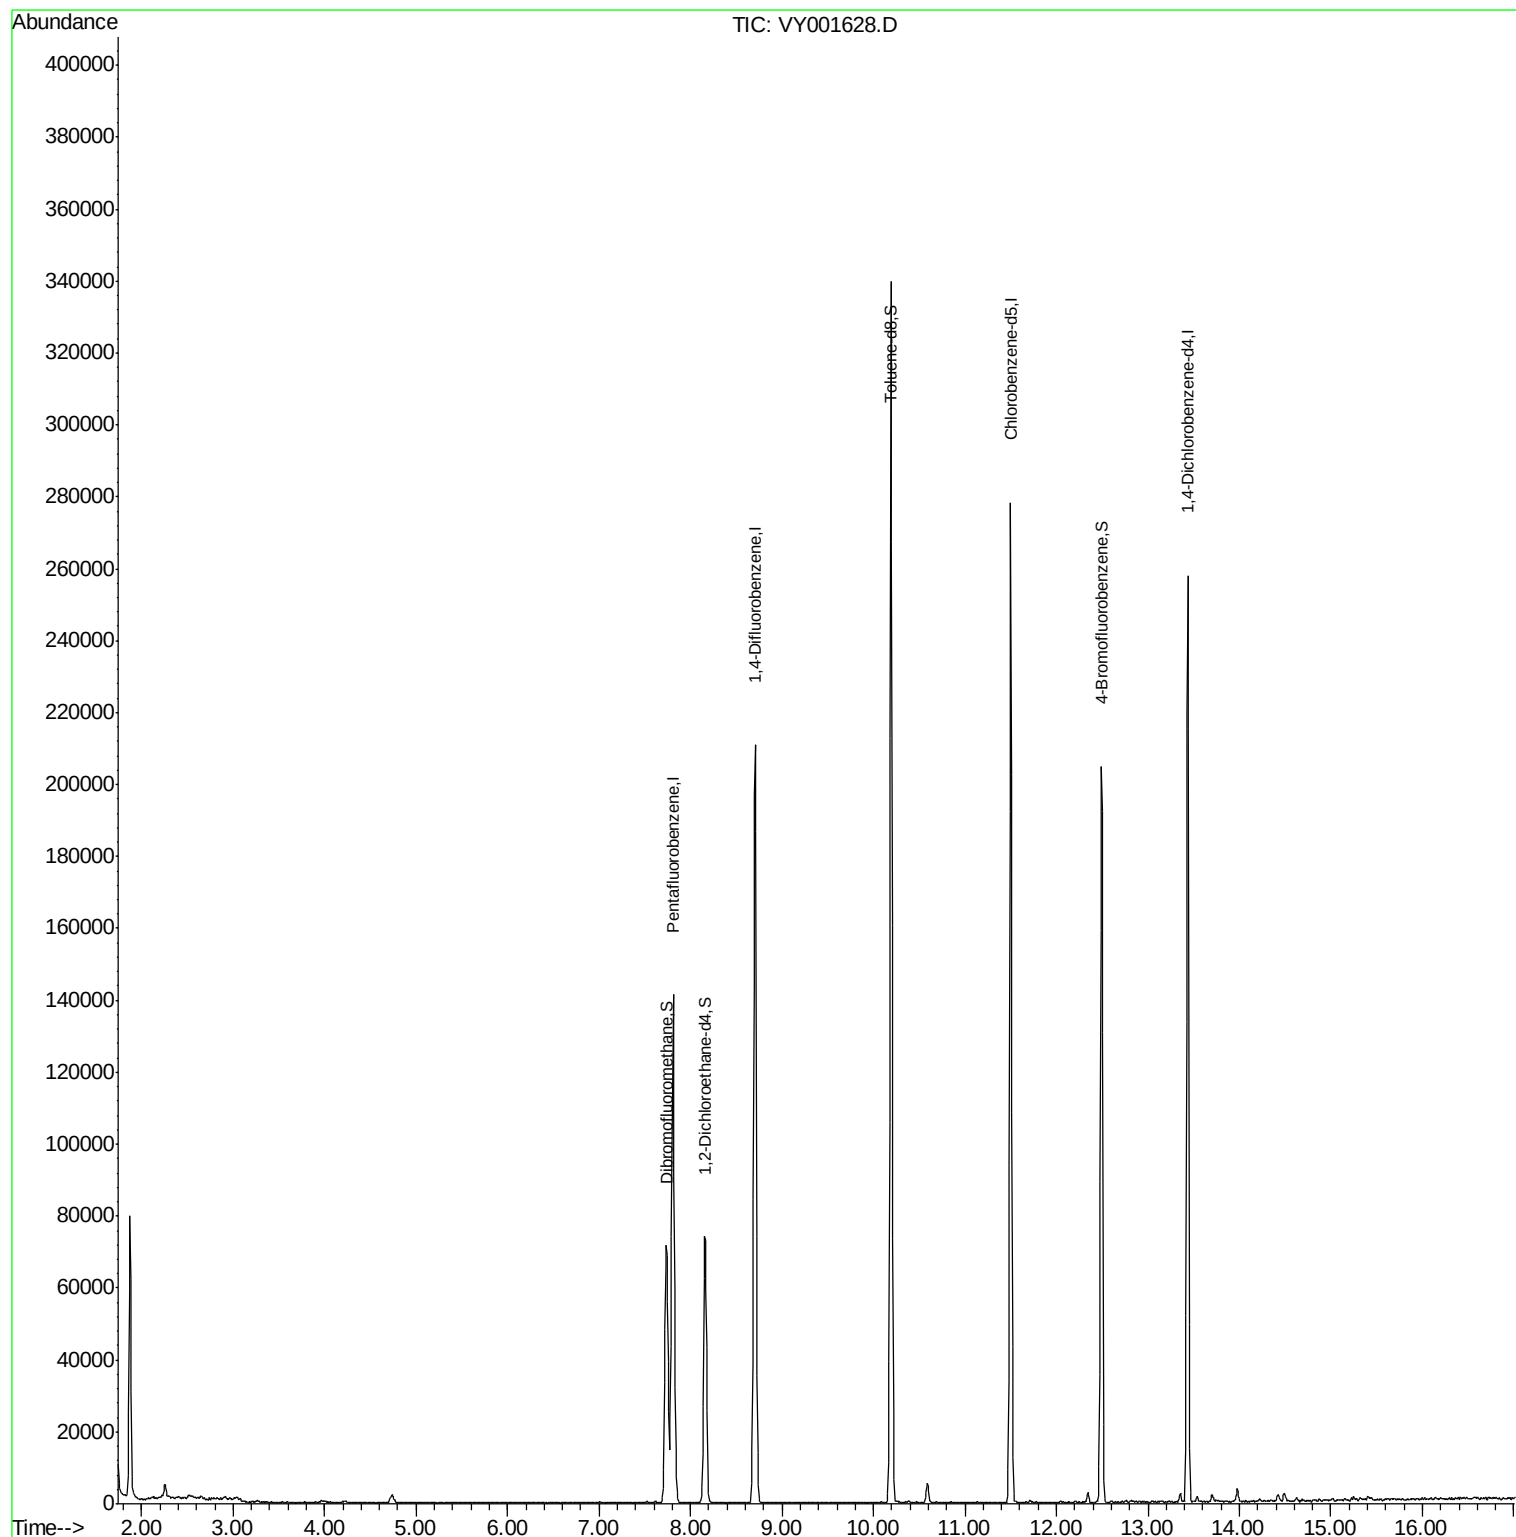

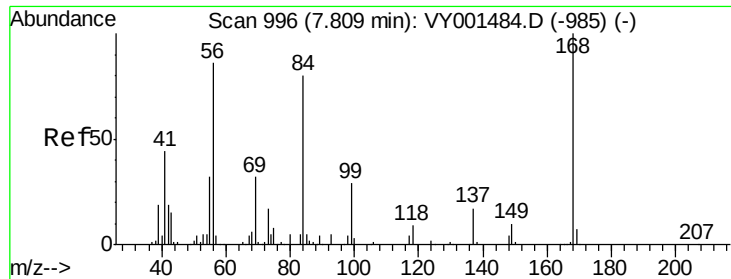

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.81 min Scan# 996

Delta R.T. 0.00 min

Lab File: VY001628.D

Acq: 13 Feb 2020 16:07

Instrument :

MSVOA_Y

ClientSampleId :


FK-GF-02-048-B

Tot Ion:168 Resp: 107550




Ion Ratio Lower Upper

168 100

99 56.8 48.2 72.4

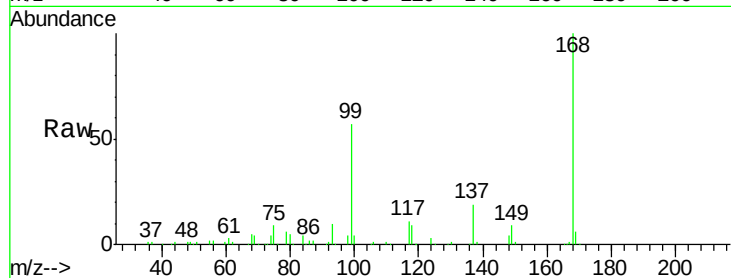

Abundance Ion 167.90 (167.60 to 168.60): VY001628.D (-947) (-)

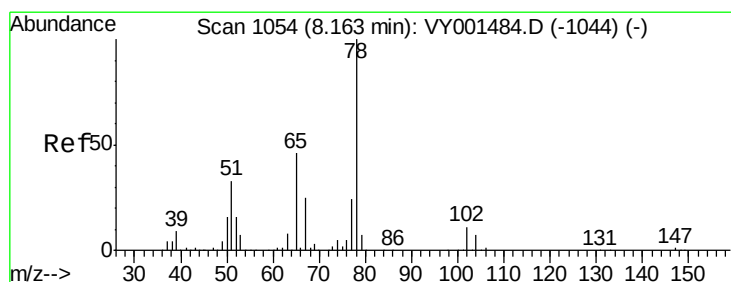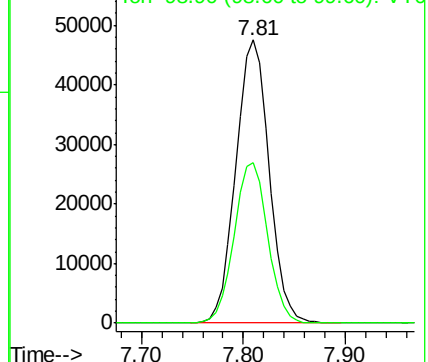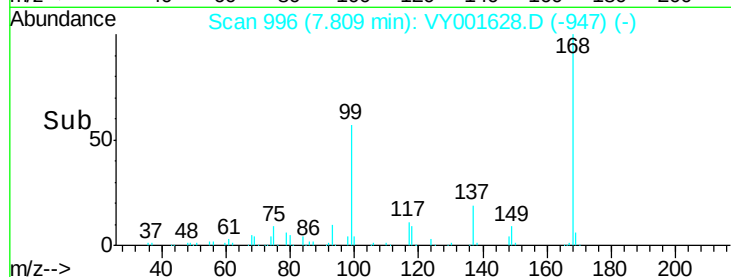

#33

1,2-Dichloroethane-d4

Concen: 52.380 ug/l

RT: 8.16 min Scan# 1053

Delta R.T. -0.01 min

Lab File: VY001628.D


Acq: 13 Feb 2020 16:07

Tgt Ion: 65 Resp: 56721



Ion Ratio Lower Upper


65 100

67 54.8 0.0 108.6

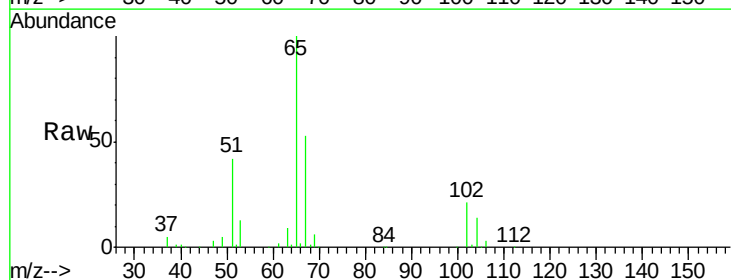

Abundance Ion 64.90 (64.60 to 65.60): VY001628.D (-1005) (-)

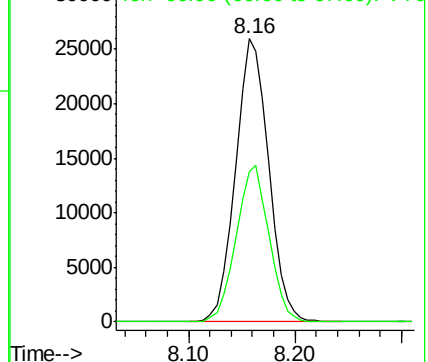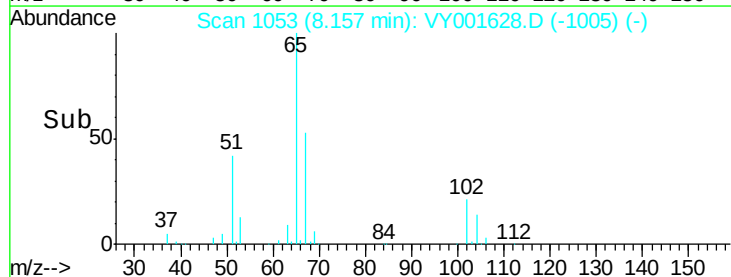

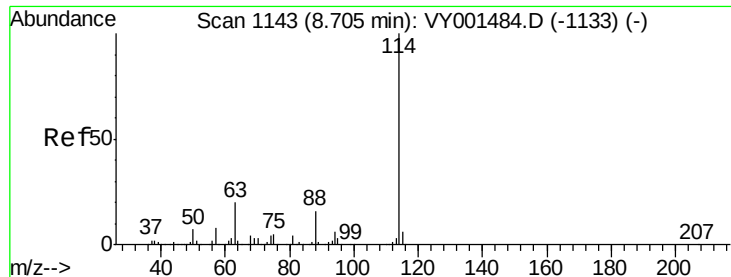

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.71 min Scan# 1143

Delta R.T. 0.00 min

Lab File: VY001628.D

Acq: 13 Feb 2020 16:07

Instrument :

MSVOA_Y

ClientSampleId :

FK-GF-02-048-B


Tot Ion:114 Resp: 181129

Ion Ratio Lower Upper

114 100

63 21.4 0.0 39.8




88 15.9 0.0 32.6

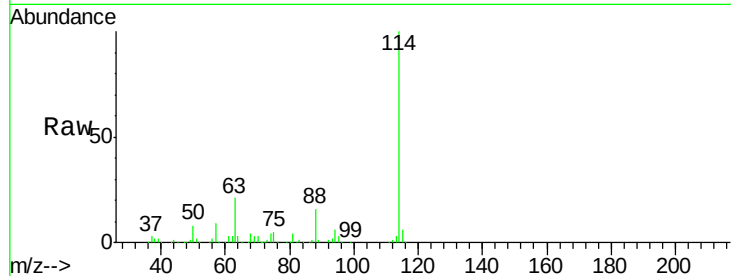

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

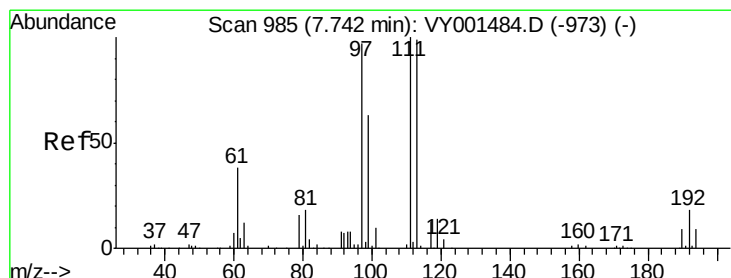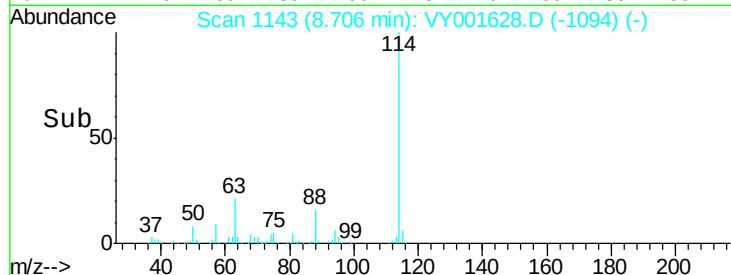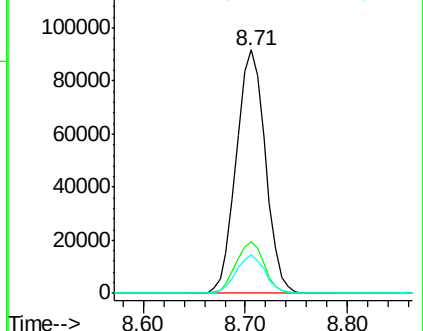

#35

Dibromofluoromethane

Concen: 48.754 ug/l

RT: 7.74 min Scan# 984

Delta R.T. -0.01 min

Lab File: VY001628.D

Acq: 13 Feb 2020 16:07


Tgt Ion:113 Resp: 50922

Ion Ratio Lower Upper

113 100

111 105.0 82.9 124.3



192 19.0 14.6 22.0

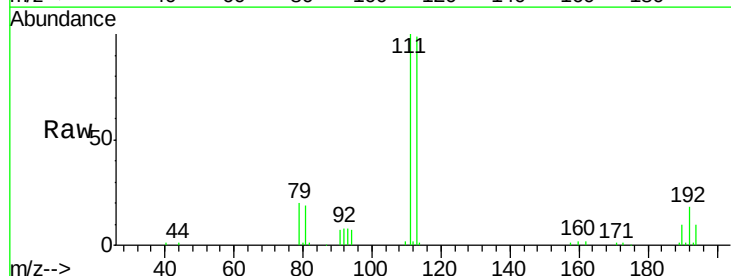


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

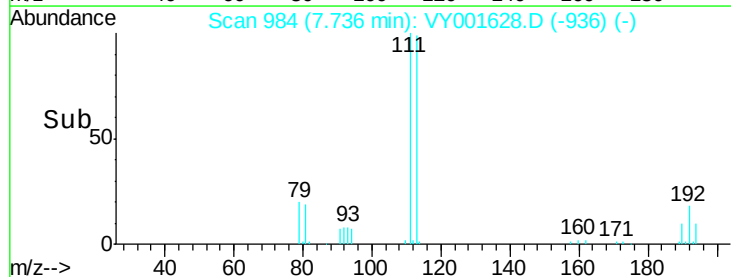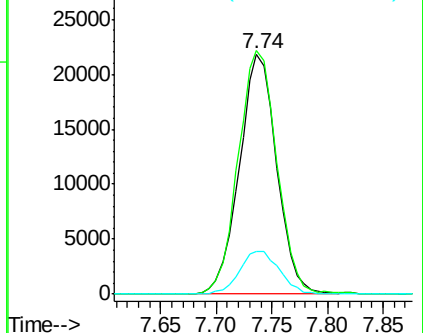

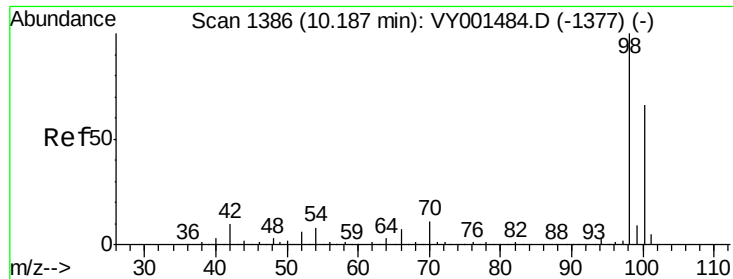

#50

Toluene-d8

Concen: 54.200 ug/l

RT: 10.19 min Scan# 1387

Delta R.T. 0.01 min

Lab File: VY001628.D

Acq: 13 Feb 2020 16:07

Instrument :

MSVOA_Y

ClientSampleId :





FK-GF-02-048-B

Tot Ion: 98 Resp: 214182

Ion Ratio Lower Upper

98 100

100 65.6 53.0 79.6

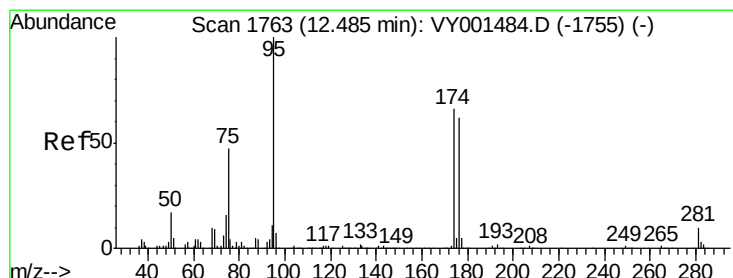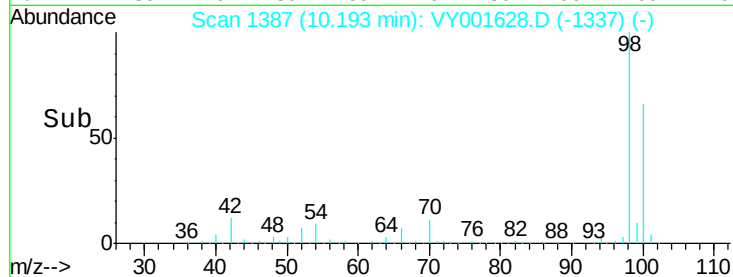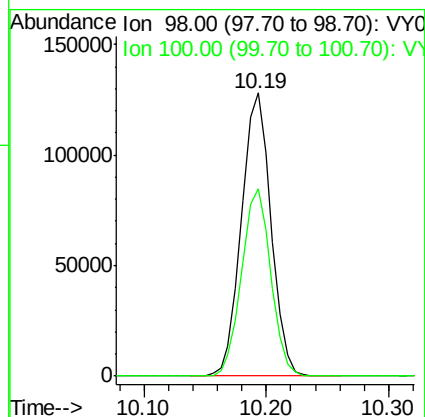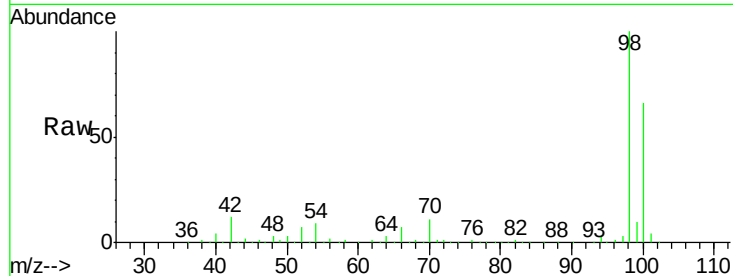

#62

4-Bromofluorobenzene

Concen: 42.441 ug/l

RT: 12.49 min Scan# 1764

Delta R.T. 0.01 min

Lab File: VY001628.D

Acq: 13 Feb 2020 16:07




Tgt Ion: 95 Resp: 66071


Ion Ratio Lower Upper

95 100

174 76.3 0.0 141.4

176 74.3 0.0 135.4

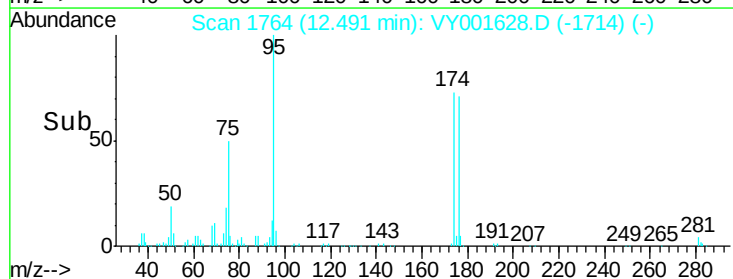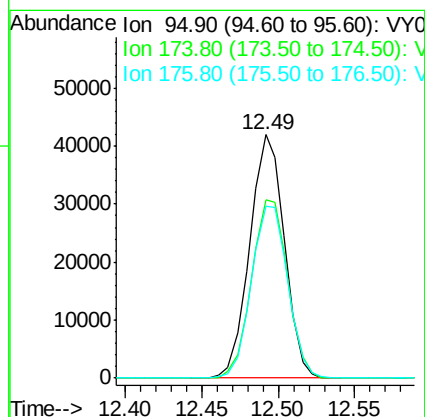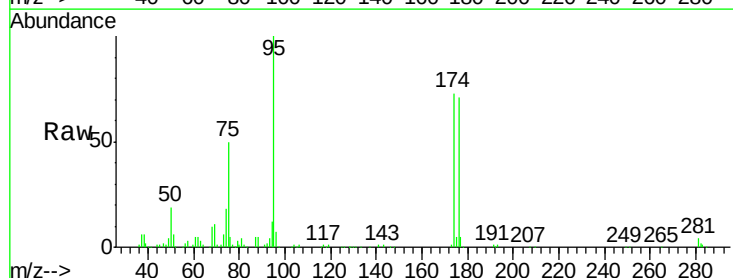


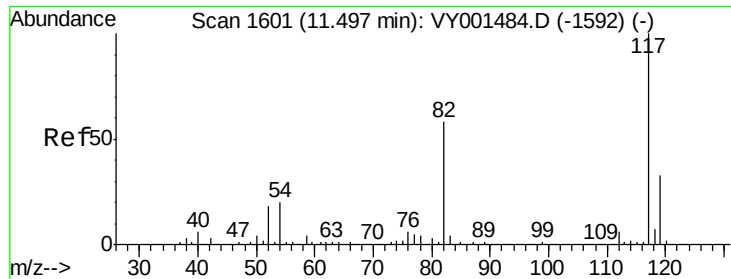




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1602
Delta R.T. 0.01 min
Lab File: VY001628.D
Acq: 13 Feb 2020 16:07

Instrument :
MSVOA_Y
ClientSampleId :
FK-GF-02-048-B

Tot Ion:117 Resp: 152111
Ion Ratio Lower Upper
117 100
82 54.2 46.1 69.1
119 31.7 26.1 39.1

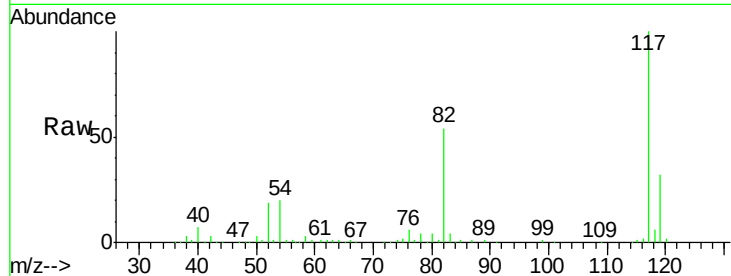


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

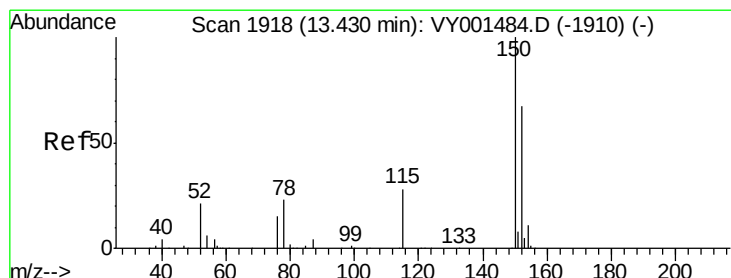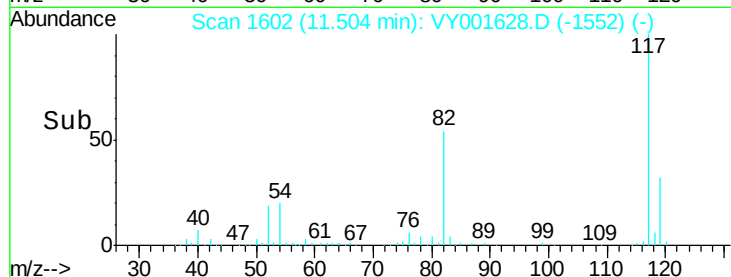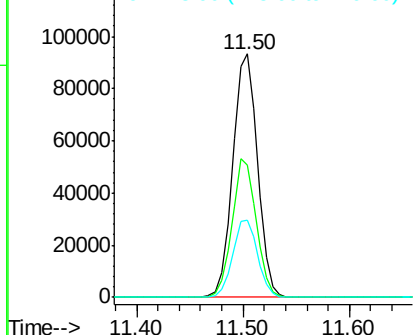

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.44 min Scan# 1919
Delta R.T. 0.01 min
Lab File: VY001628.D
Acq: 13 Feb 2020 16:07

Tgt Ion:152 Resp: 62854
Ion Ratio Lower Upper
152 100
115 59.6 31.4 94.3
150 158.3 0.0 346.8

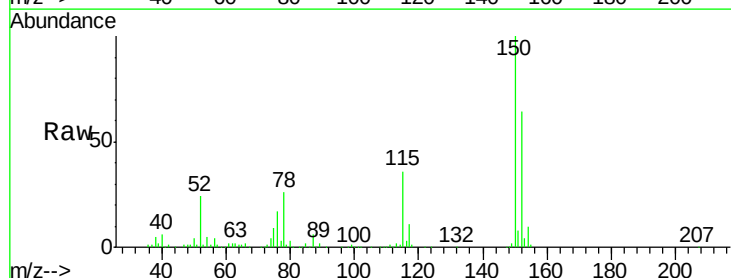

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

