


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021325\
Data File : VY021184.D
Acq On : 13 Feb 2025 08:41
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
Title : SW846 8260
Last Update : Mon Feb 03 13:08:38 2025

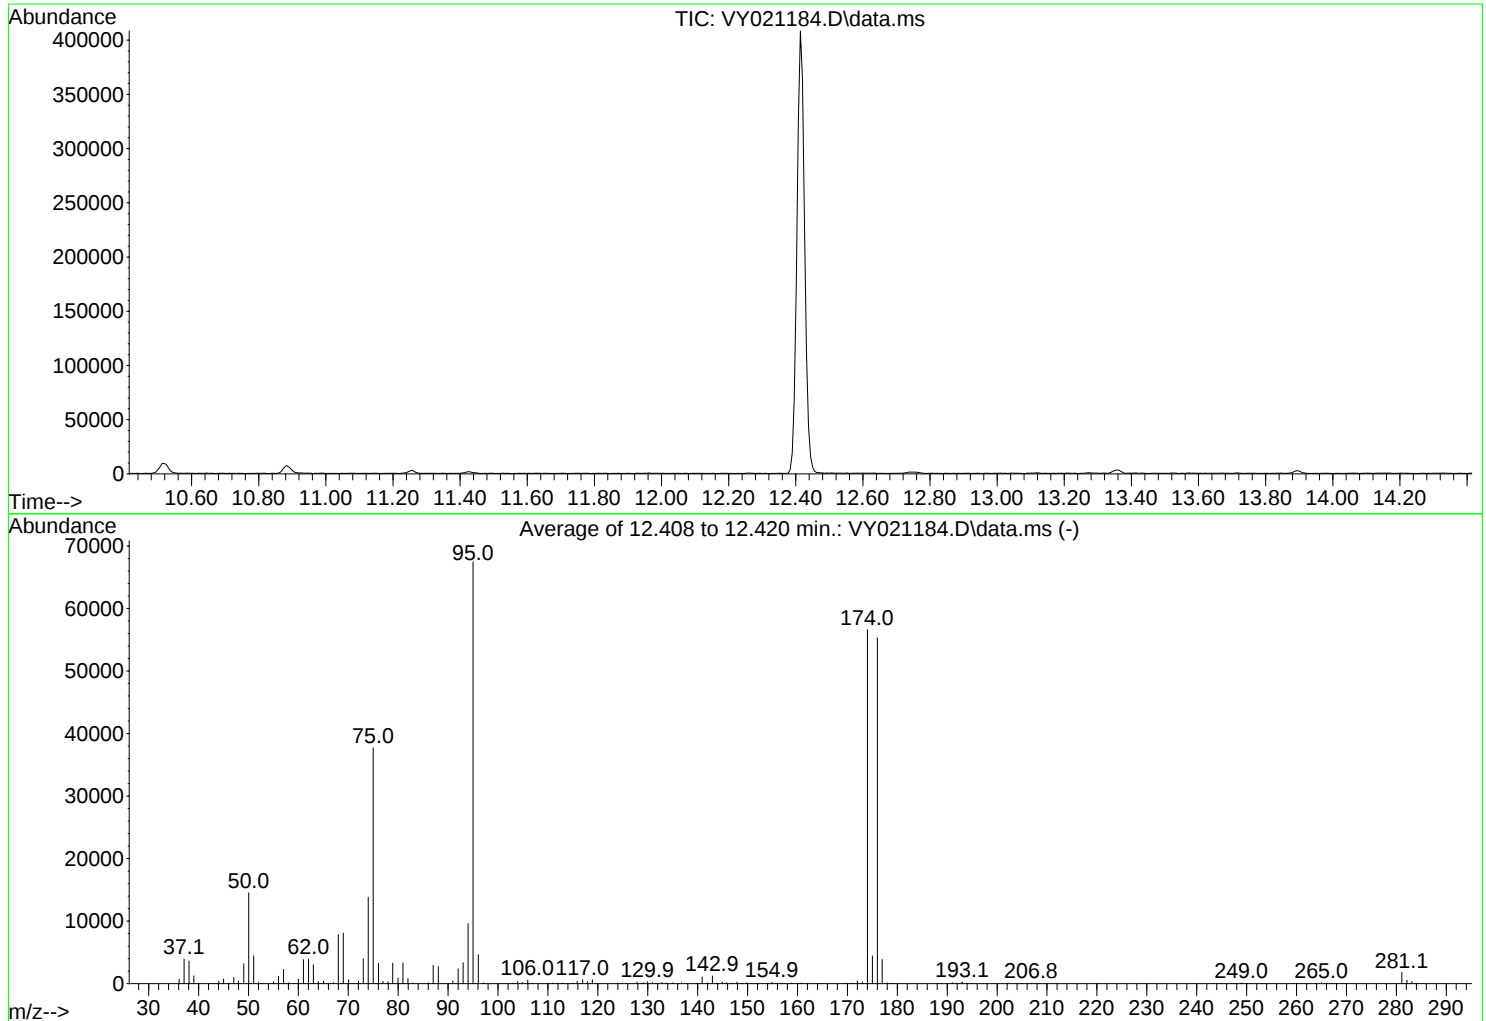

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.5	14524	PASS
75	95	30	60	55.9	37723	PASS
95	95	100	100	100.0	67461	PASS
96	95	5	9	6.8	4621	PASS
173	174	0.00	2	0.5	261	PASS
174	95	50	100	83.9	56613	PASS
175	174	5	9	7.8	4427	PASS
176	174	95	101	97.7	55293	PASS
177	176	5	9	7.0	3871	PASS