
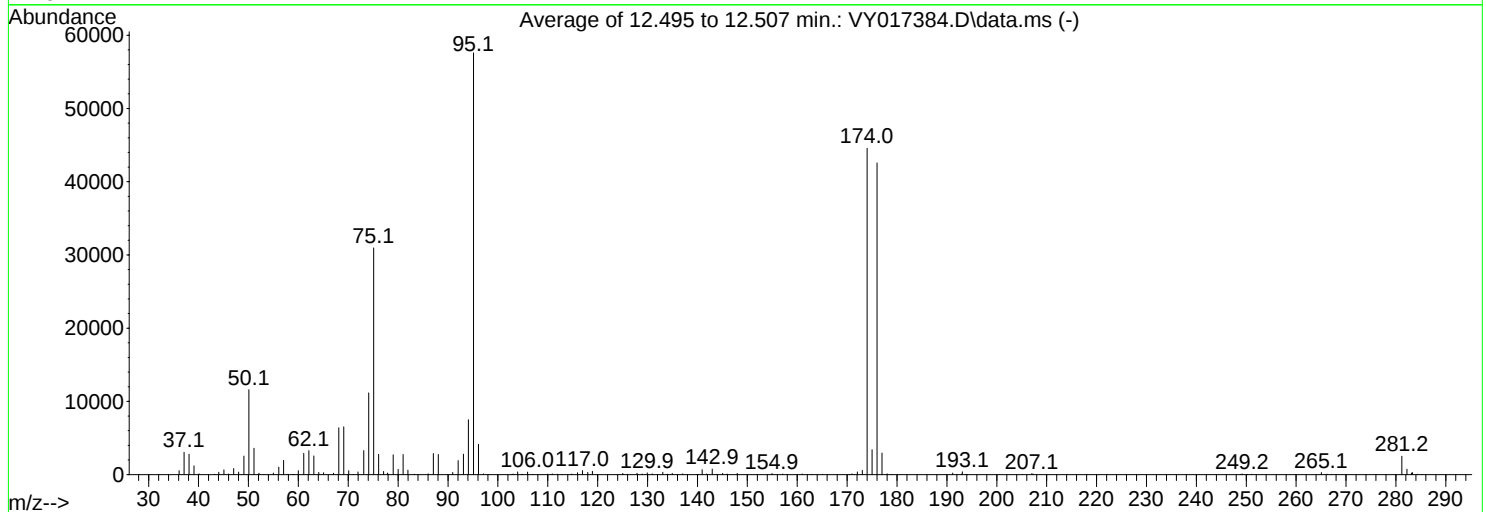


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021524\
Data File : VY017384.D
Acq On : 15 Feb 2024 08:46
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021424S.M
Title : SW846 8260
Last Update : Thu Feb 15 03:16:56 2024

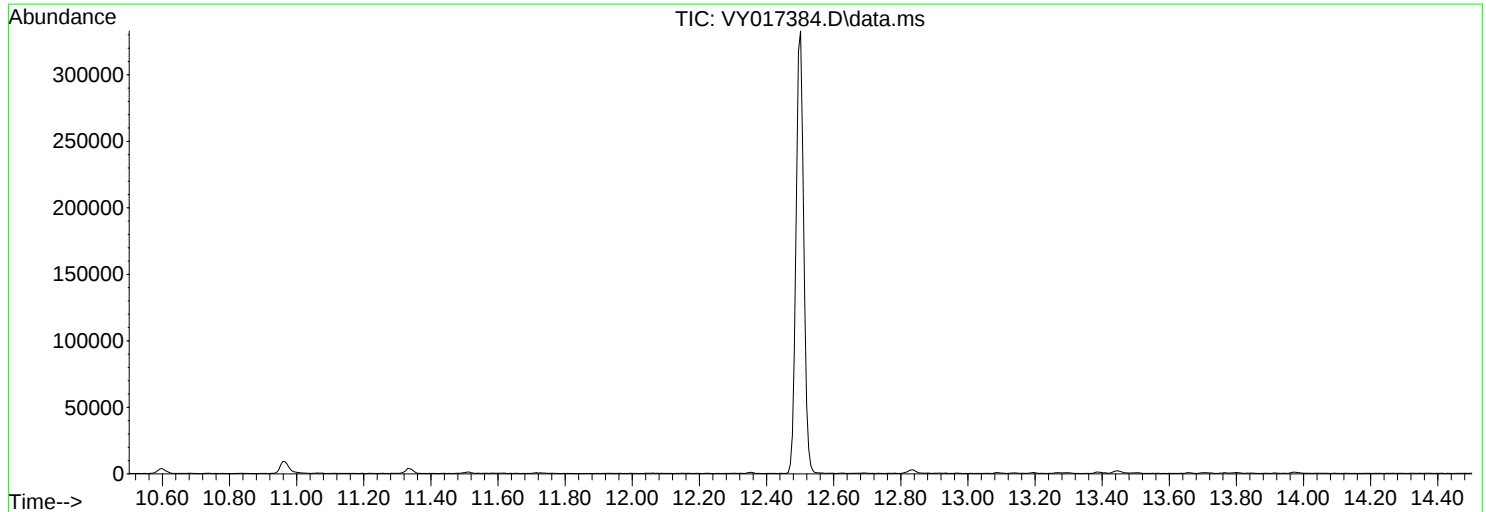

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	11612	PASS
75	95	30	60	53.8	30960	PASS
95	95	100	100	100.0	57597	PASS
96	95	5	9	7.2	4161	PASS
173	174	0.00	2	1.3	592	PASS
174	95	50	100	77.4	44576	PASS
175	174	5	9	7.6	3406	PASS
176	174	95	101	95.5	42563	PASS
177	176	5	9	6.9	2954	PASS