


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv022020\
 Data File : VY001711.D
 Acq On : 20 Feb 2020 09:46
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y021720S.M
 Title : SW846 8260
 Last Update : Mon Feb 17 12:19:53 2020

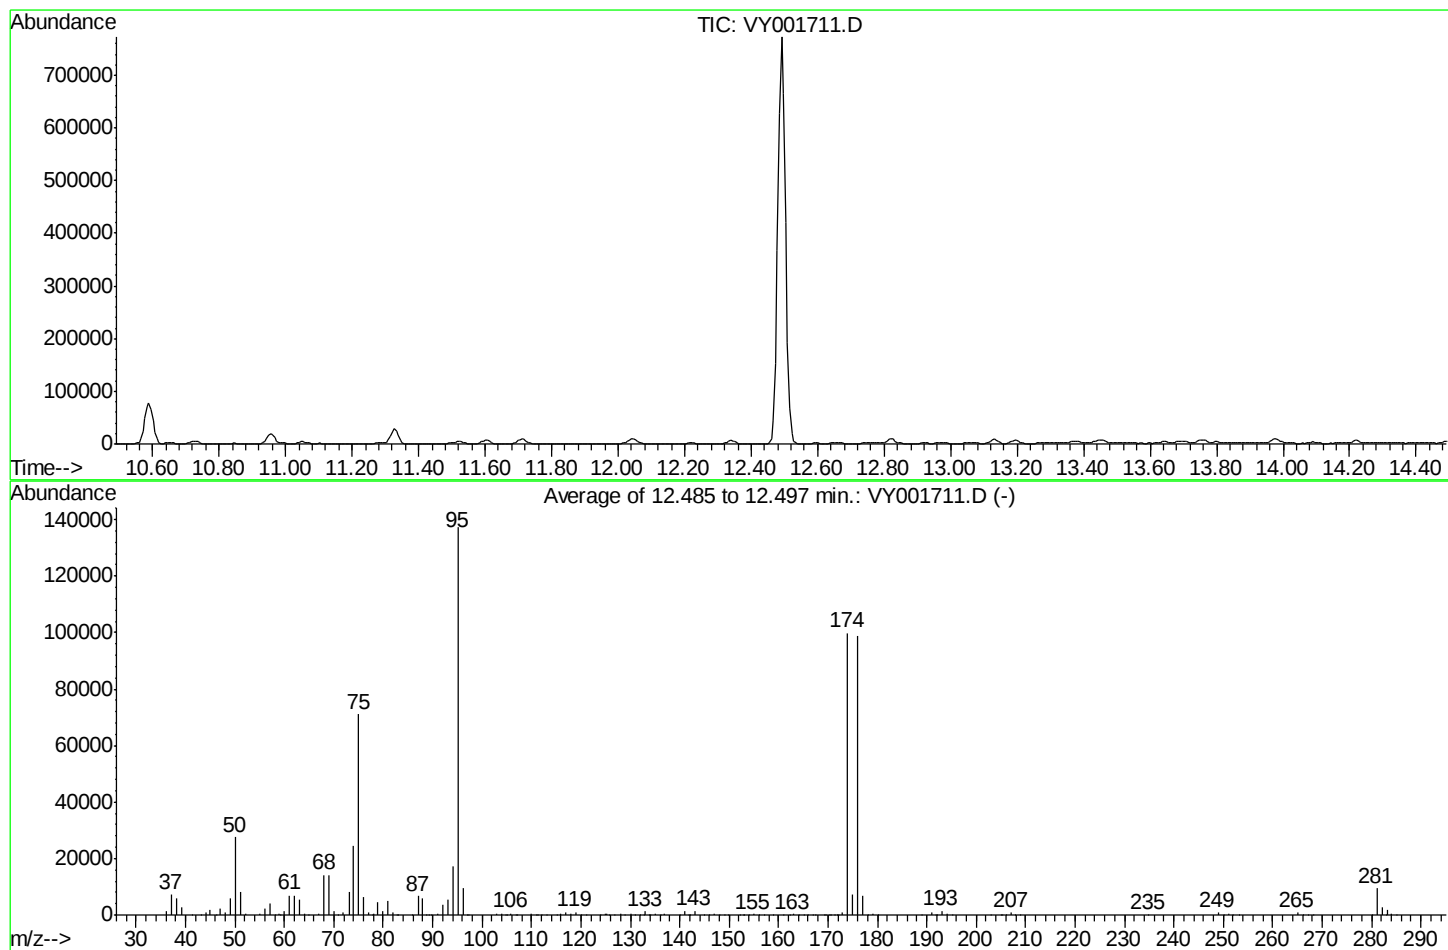

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	27496	PASS
75	95	30	60	51.7	71016	PASS
95	95	100	100	100.0	137272	PASS
96	95	5	9	7.0	9595	PASS
173	174	0.00	2	0.9	882	PASS
174	95	50	100	72.7	99864	PASS
175	174	5	9	7.4	7391	PASS
176	174	95	101	99.0	98888	PASS
177	176	5	9	6.9	6780	PASS