

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022124\
 Data File : VY017442.D
 Acq On : 21 Feb 2024 16:52
 Operator : SY/MD
 Sample : P1537-09
 Misc : 3.86g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 9

Quant Time: Feb 22 03:40:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021924S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 20 06:16:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	118795	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.703	114	230810	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.502	117	203083	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.434	152	70078	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	47084	46.395	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	92.780%
35) Dibromofluoromethane	7.728	113	55790	41.293	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	82.580%
50) Toluene-d8	10.191	98	194580	37.134	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	74.260%
62) 4-Bromofluorobenzene	12.489	95	49993	29.346	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	58.700%
Target Compounds						
					Qvalue	
20) Methylene Chloride	4.728	84	20772	10.606	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022124\
Data File : VY017442.D
Acq On : 21 Feb 2024 16:52
Operator : SY/MD
Sample : P1537-09
Misc : 3.86g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
9

Quant Time: Feb 22 03:40:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021924S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 20 06:16:24 2024
Response via : Initial Calibration




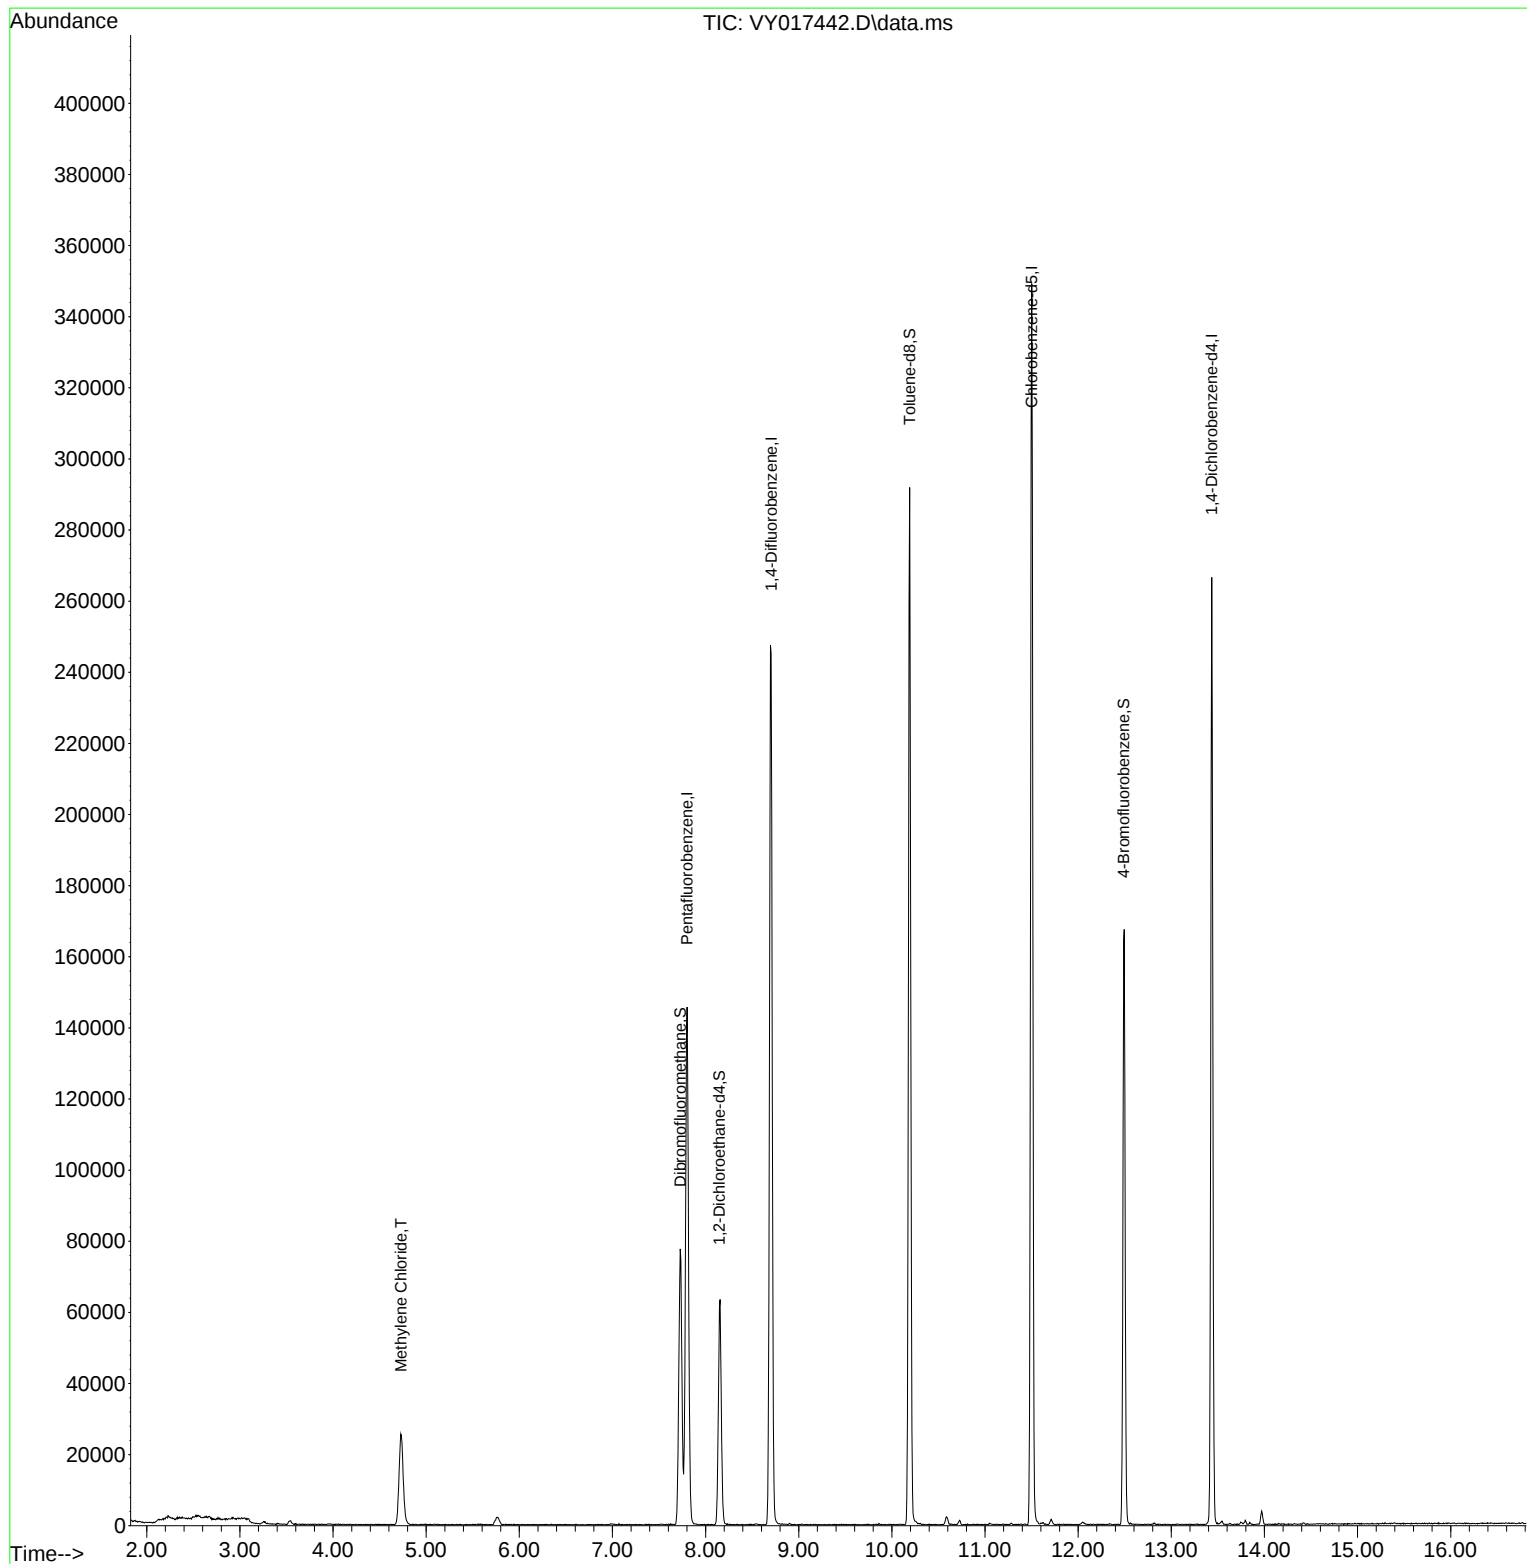


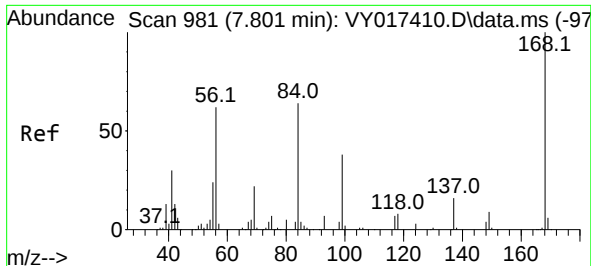

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY017442.D
Acq: 21 Feb 2024 16:52




Instrument :
MSVOA_Y
ClientSampleId :
9


Tgt Ion:168 Resp: 118795
Ion Ratio Lower Upper
168 100
99 48.3 39.1 58.7

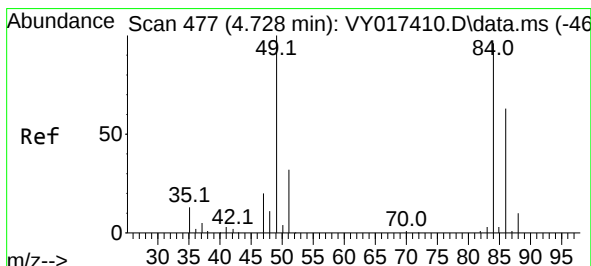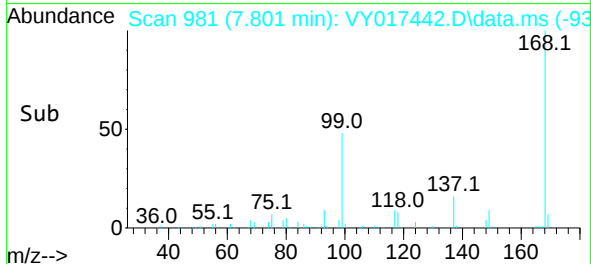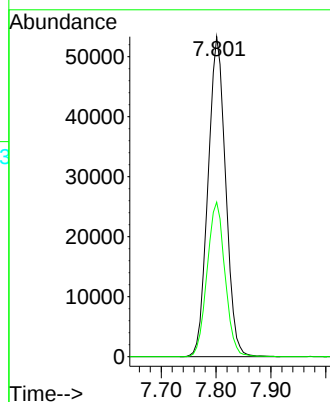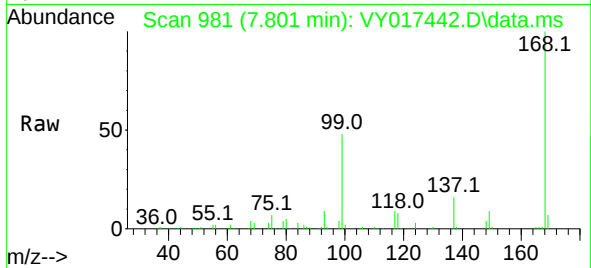

#20
Methylene Chloride
Concen: 10.606 ug/l
RT: 4.728 min Scan# 477
Delta R.T. 0.000 min
Lab File: VY017442.D
Acq: 21 Feb 2024 16:52

Tgt Ion: 84 Resp: 20772
Ion Ratio Lower Upper
84 100
49 108.8 84.4 126.6
51 33.1 26.0 39.0
86 68.6 49.5 74.3

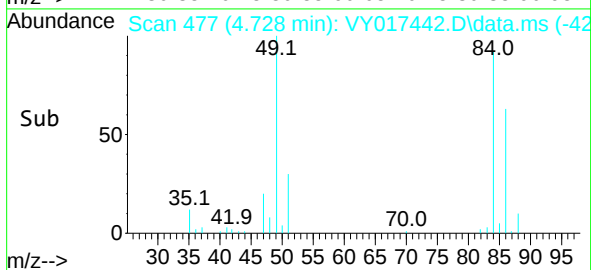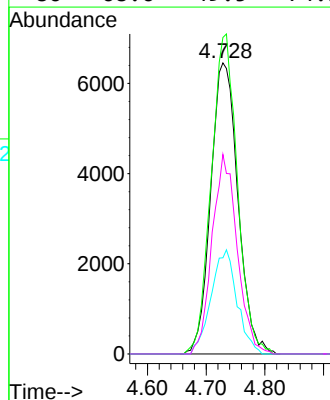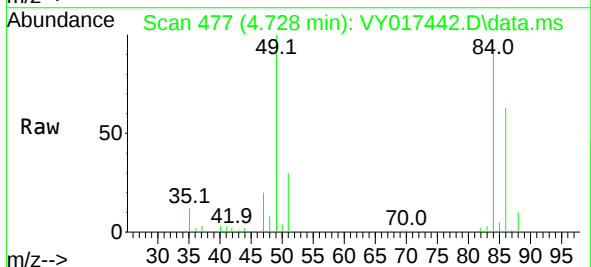

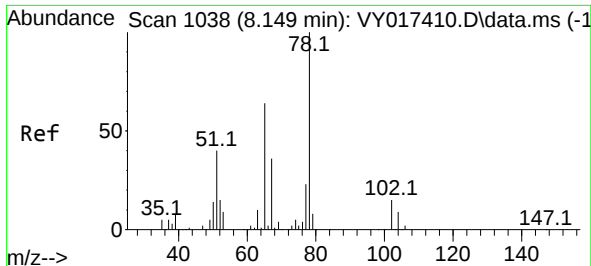

#33

1,2-Dichloroethane-d4

Concen: 46.395 ug/l

RT: 8.149 min Scan# 1109

Delta R.T. -0.000 min

Lab File: VY017442.D

Acq: 21 Feb 2024 16:52

Instrument :

MSVOA_Y

ClientSampleId :





9

Tgt Ion: 65 Resp: 47084

Ion Ratio Lower Upper

65 100

67 54.2 0.0 109.6

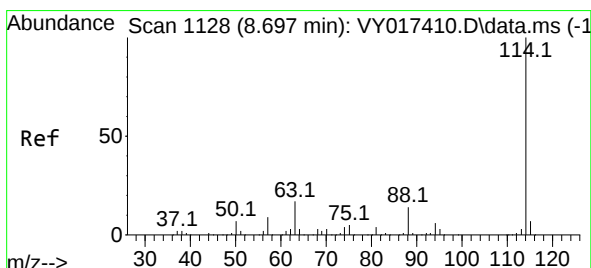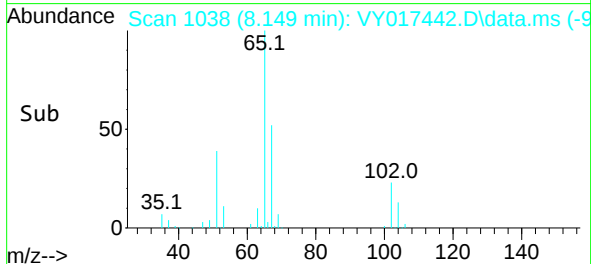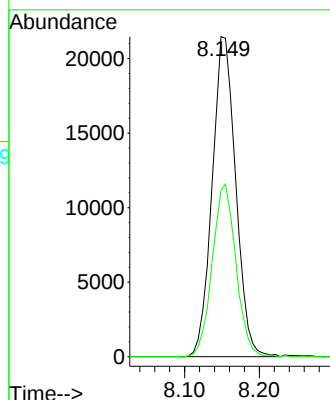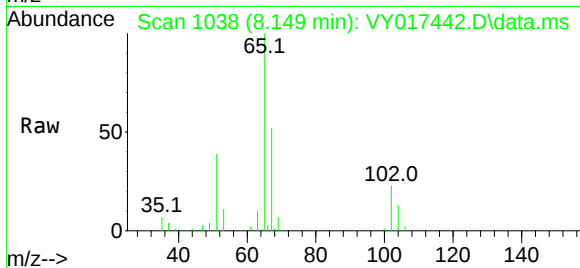

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.703 min Scan# 1129

Delta R.T. 0.006 min

Lab File: VY017442.D

Acq: 21 Feb 2024 16:52




Tgt Ion: 114 Resp: 230810


Ion Ratio Lower Upper

114 100

63 17.6 0.0 35.0


88 14.0 0.0 27.2

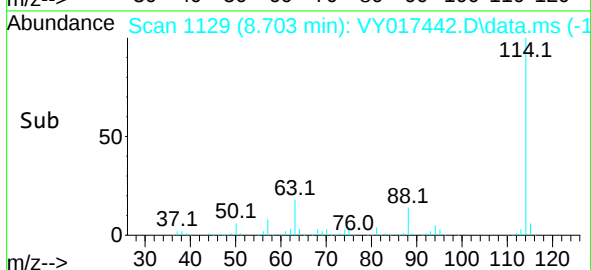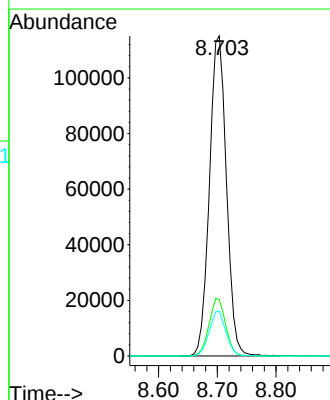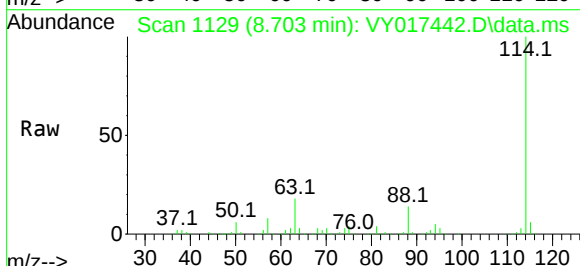



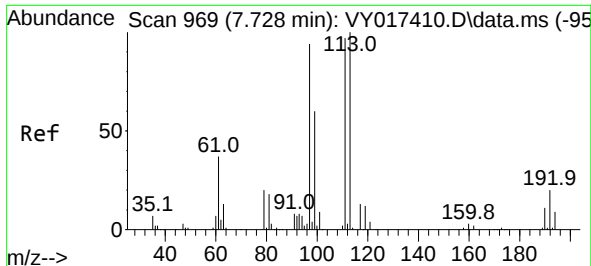


#35
Dibromofluoromethane
Concen: 41.293 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY017442.D
Acq: 21 Feb 2024 16:52

Instrument :
MSVOA_Y
ClientSampleId :
9



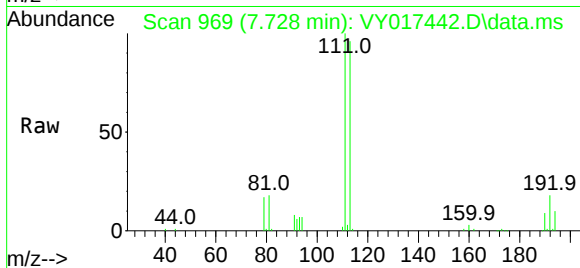



Tgt Ion:113 Resp: 55790
Ion Ratio Lower Upper
113 100
111 102.5 82.2 123.4
192 20.2 15.9 23.9

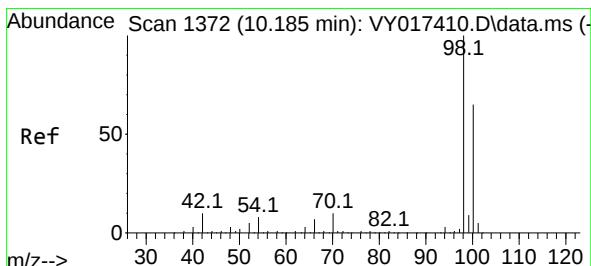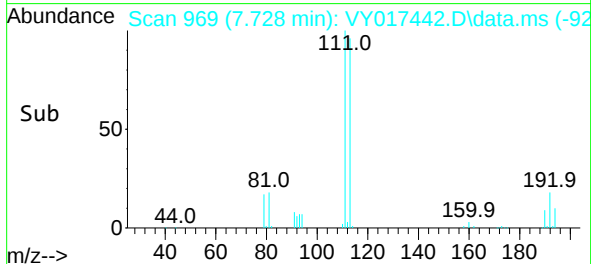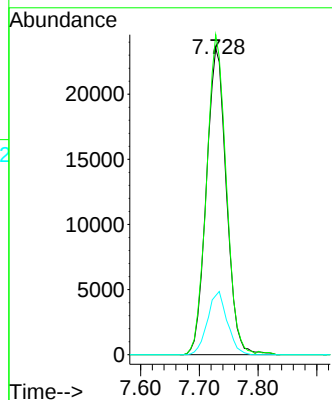

#50
Toluene-d8
Concen: 37.134 ug/l
RT: 10.191 min Scan# 1373
Delta R.T. 0.006 min
Lab File: VY017442.D
Acq: 21 Feb 2024 16:52

Tgt Ion: 98 Resp: 194580
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0


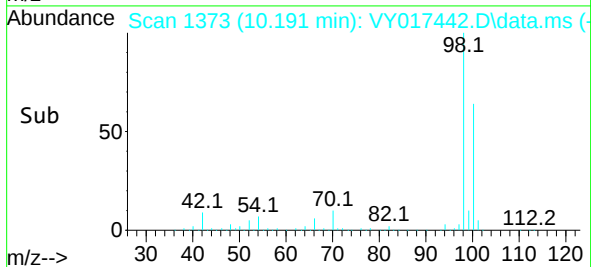
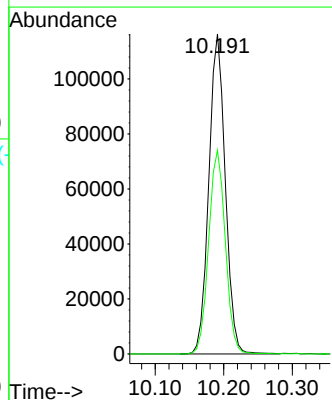
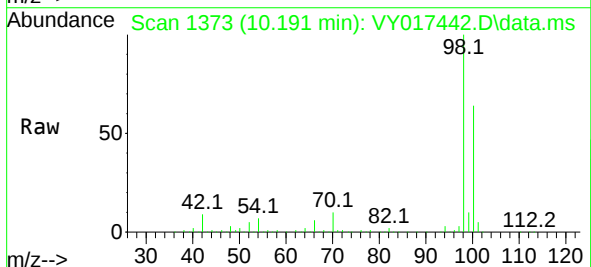


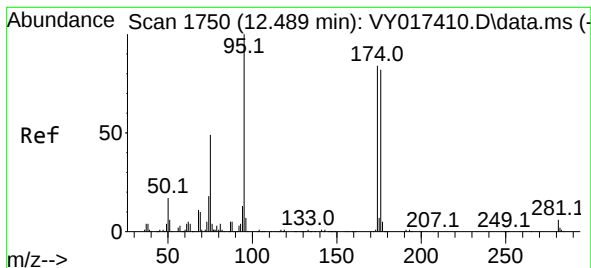

#62
4-Bromofluorobenzene
Concen: 29.346 ug/l
RT: 12.489 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY017442.D
Acq: 21 Feb 2024 16:52




Instrument :
MSVOA_Y
ClientSampleId :
9


Tgt Ion:	95	Resp:	49993
Ion	Ratio	Lower	Upper
95	100		
174	92.9	0.0	175.6
176	89.9	0.0	171.4

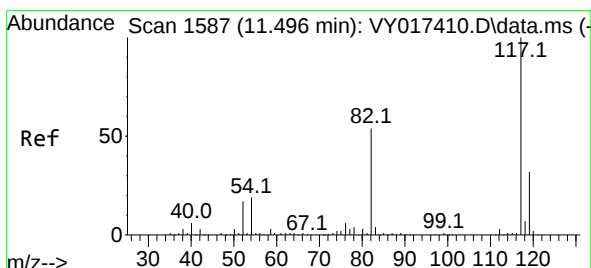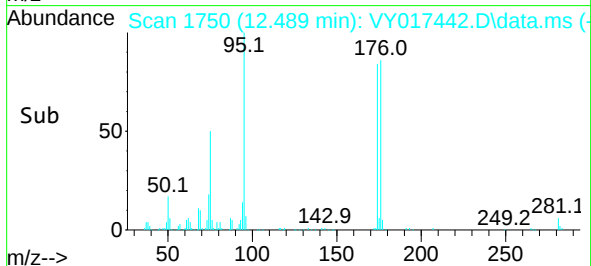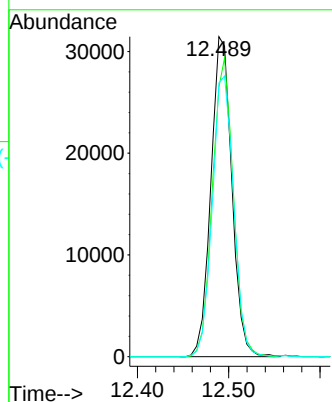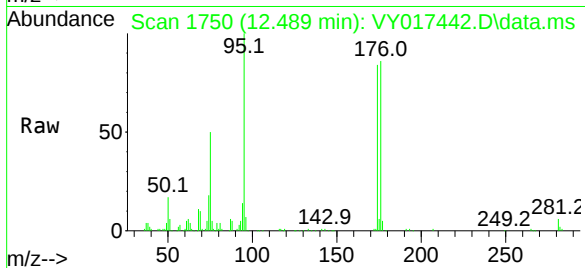

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.502 min Scan# 1588
Delta R.T. 0.006 min
Lab File: VY017442.D
Acq: 21 Feb 2024 16:52


Tgt Ion:	117	Resp:	203083
Ion	Ratio	Lower	Upper
117	100		
82	51.9	42.4	63.6
119	32.0	25.9	38.9

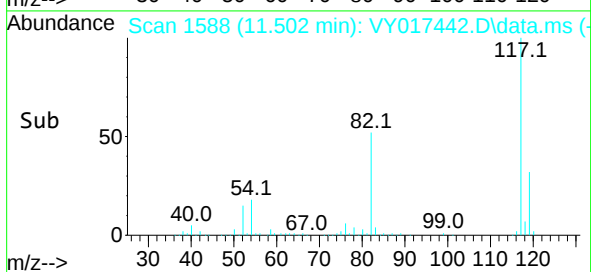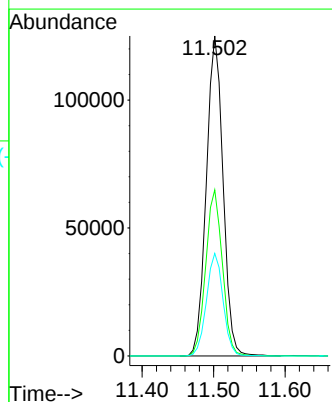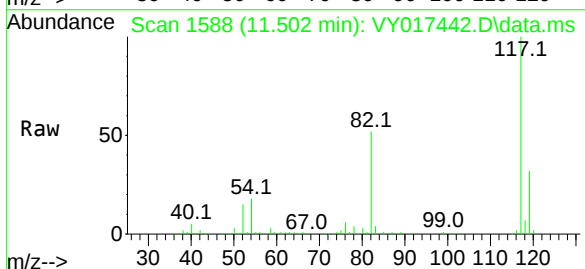

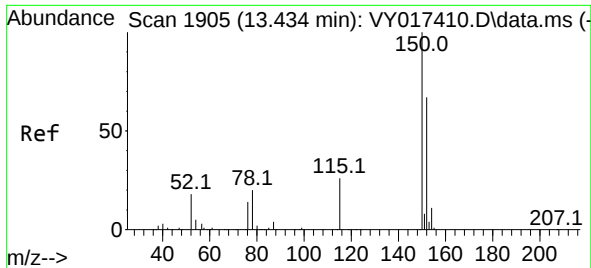

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.434 min Scan# 1905
Delta R.T. -0.000 min
Lab File: VY017442.D
Acq: 21 Feb 2024 16:52

Instrument :
MSVOA_Y
ClientSampleId :
9

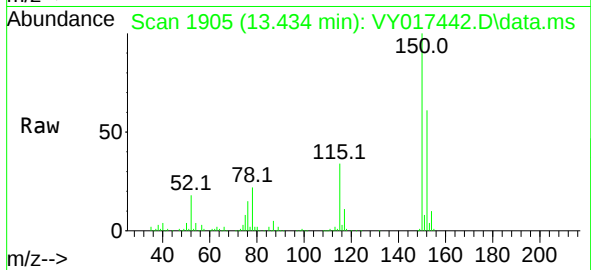

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.8	28.2	84.7
150	159.6	0.0	345.6

