
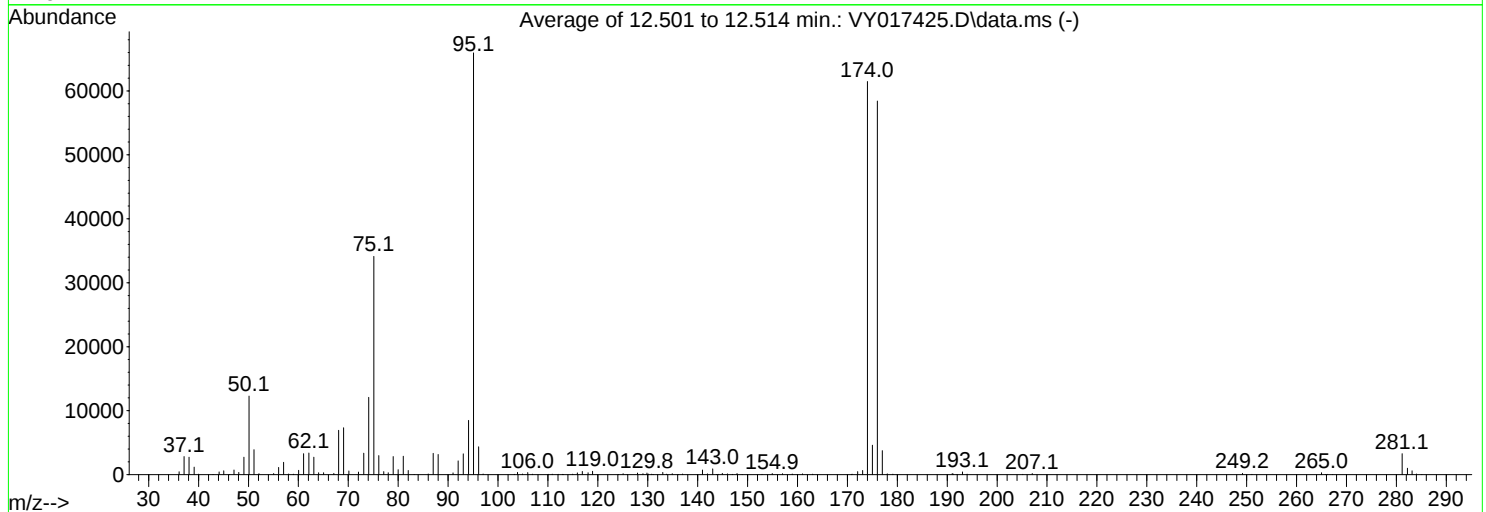


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022124\
Data File : VY017425.D
Acq On : 21 Feb 2024 08:34
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021924S.M
Title : SW846 8260
Last Update : Tue Feb 20 06:16:24 2024

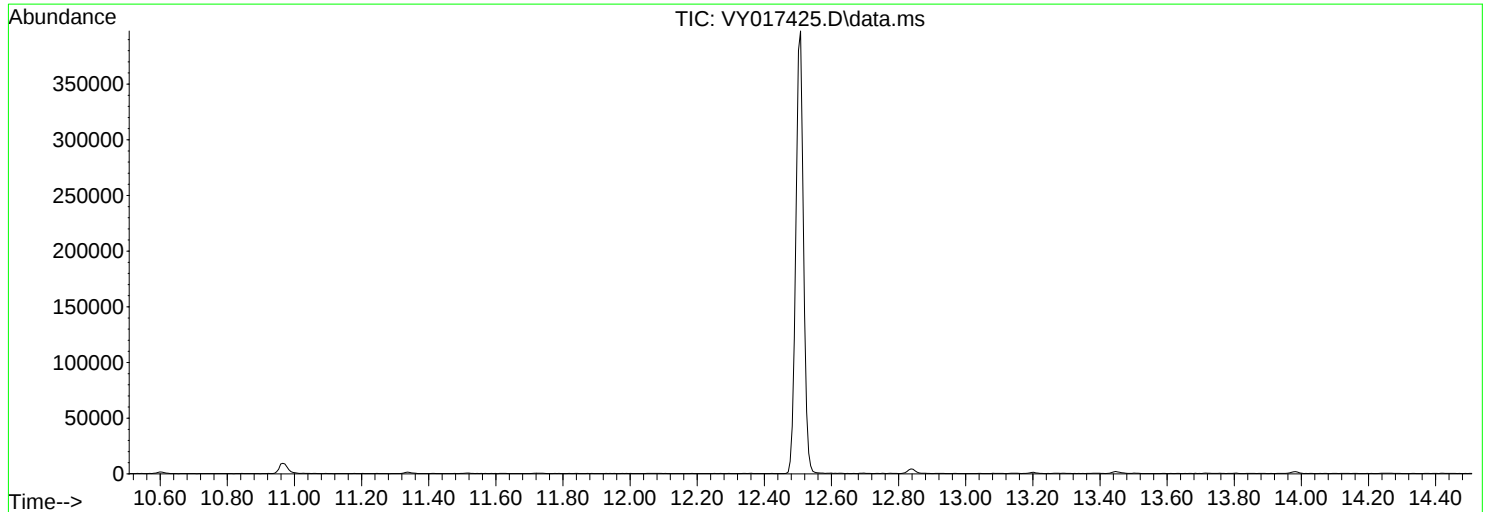

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	12289	PASS
75	95	30	60	51.7	34125	PASS
95	95	100	100	100.0	65949	PASS
96	95	5	9	6.6	4364	PASS
173	174	0.00	2	1.1	660	PASS
174	95	50	100	93.2	61472	PASS
175	174	5	9	7.5	4614	PASS
176	174	95	101	95.0	58408	PASS
177	176	5	9	6.4	3756	PASS