
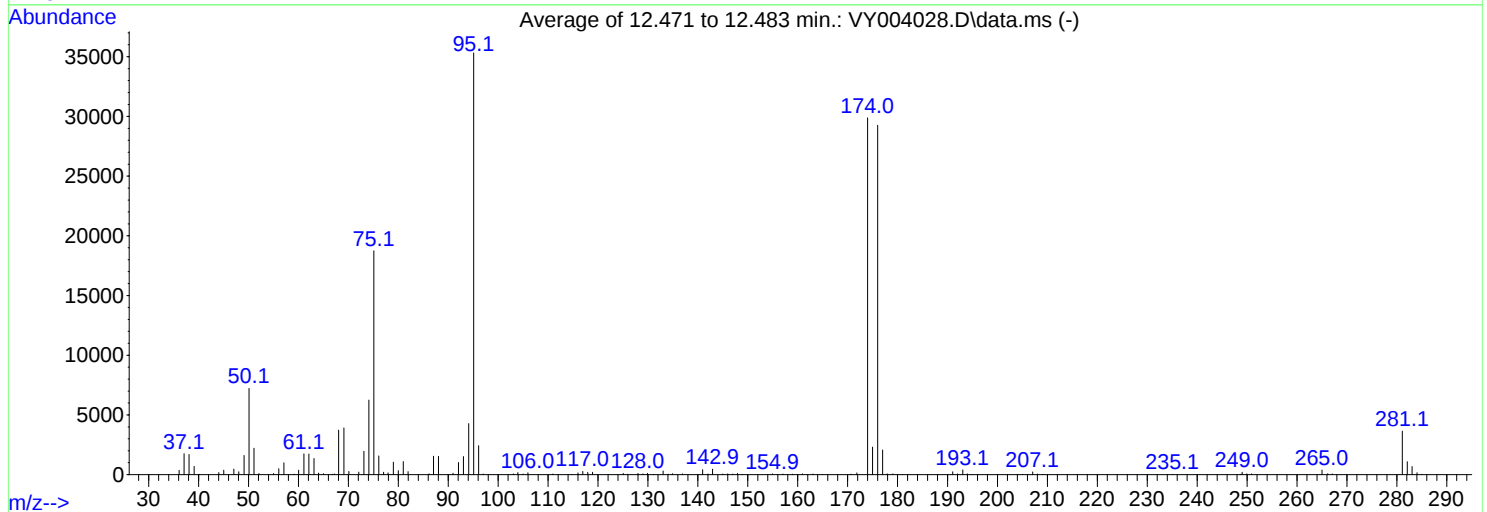


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY022221\  
 Data File : VY004028.D  
 Acq On : 22 Feb 2021 09:46  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00g/5mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y022221S.M  
 Title : SW846 8260  
 Last Update : Tue Feb 23 03:42:58 2021

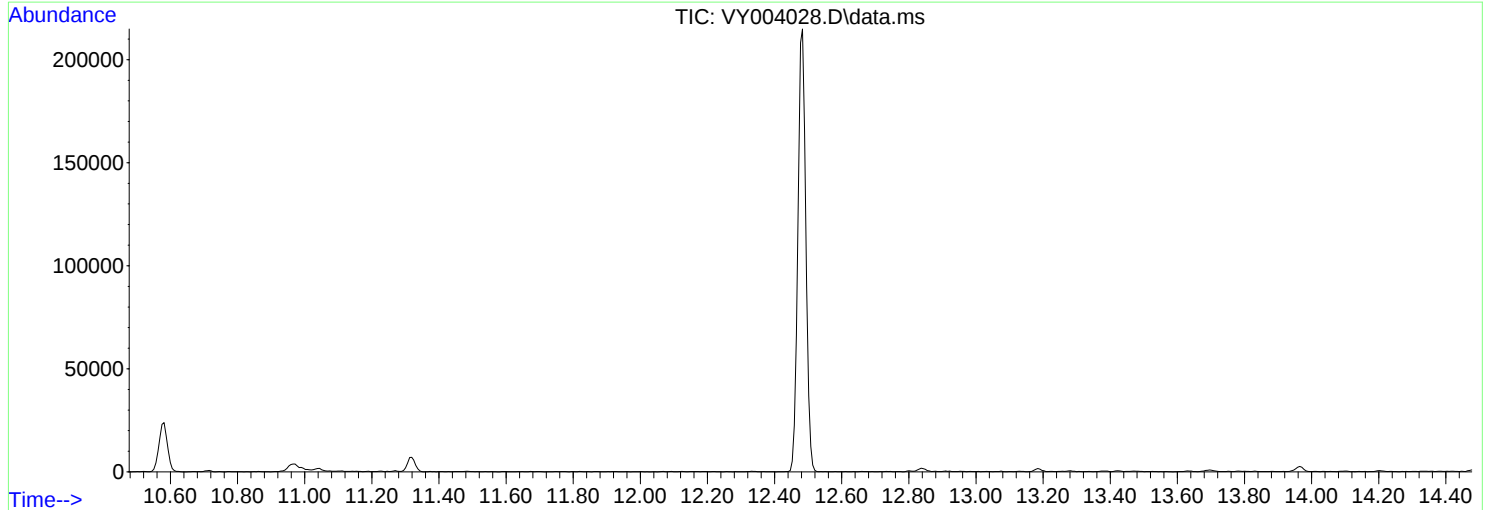

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.5         | 7224       | PASS                |
| 75             | 95              | 30              | 60              | 53.1         | 18743      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 35325      | PASS                |
| 96             | 95              | 5               | 9               | 6.9          | 2426       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 174            | 95              | 50              | 100             | 84.6         | 29883      | PASS                |
| 175            | 174             | 5               | 9               | 7.7          | 2304       | PASS                |
| 176            | 174             | 95              | 101             | 97.9         | 29253      | PASS                |
| 177            | 176             | 5               | 9               | 7.1          | 2068       | PASS                |