
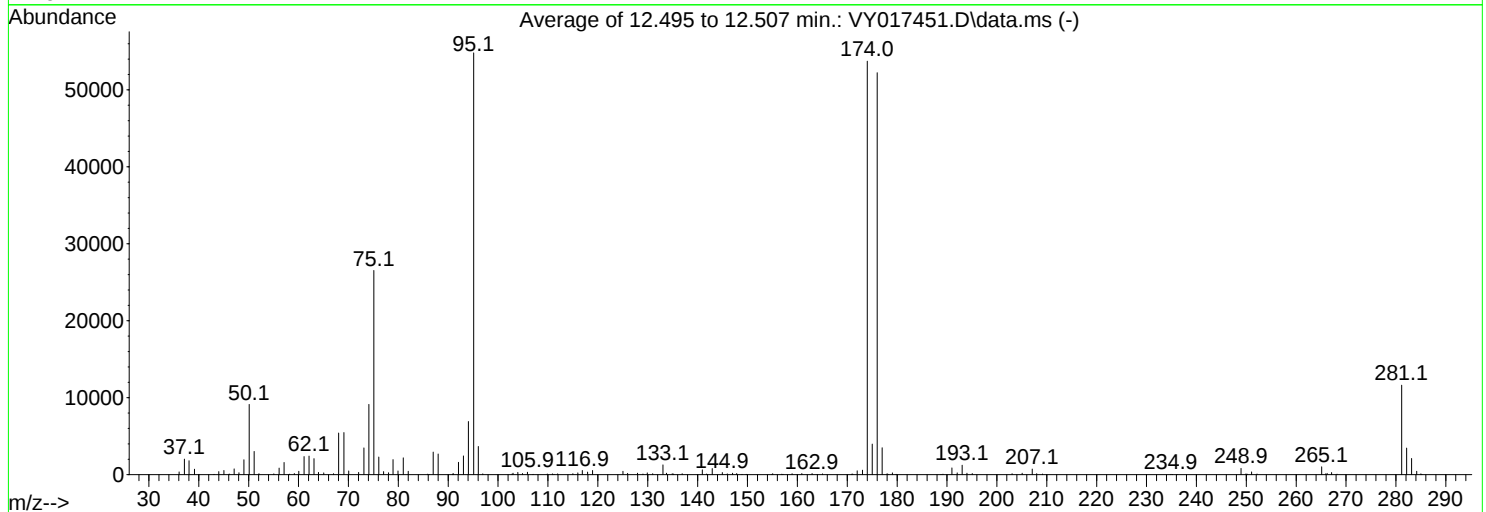


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022224\
Data File : VY017451.D
Acq On : 22 Feb 2024 08:58
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021924S.M
Title : SW846 8260
Last Update : Tue Feb 20 06:16:24 2024

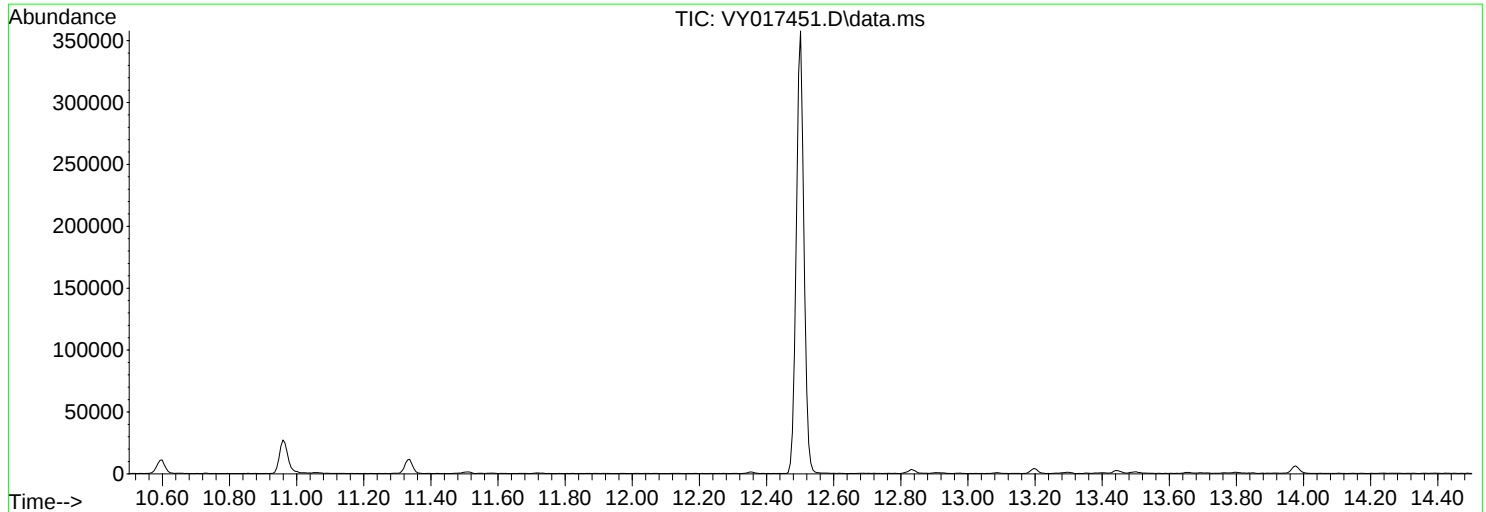

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	9123	PASS
75	95	30	60	48.4	26533	PASS
95	95	100	100	100.0	54811	PASS
96	95	5	9	6.7	3664	PASS
173	174	0.00	2	1.1	587	PASS
174	95	50	100	98.0	53731	PASS
175	174	5	9	7.4	3970	PASS
176	174	95	101	97.2	52224	PASS
177	176	5	9	6.7	3494	PASS