


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv022420\
 Data File : VY001760.D
 Acq On : 24 Feb 2020 09:21
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y021720S.M
 Title : SW846 8260
 Last Update : Mon Feb 17 12:19:53 2020

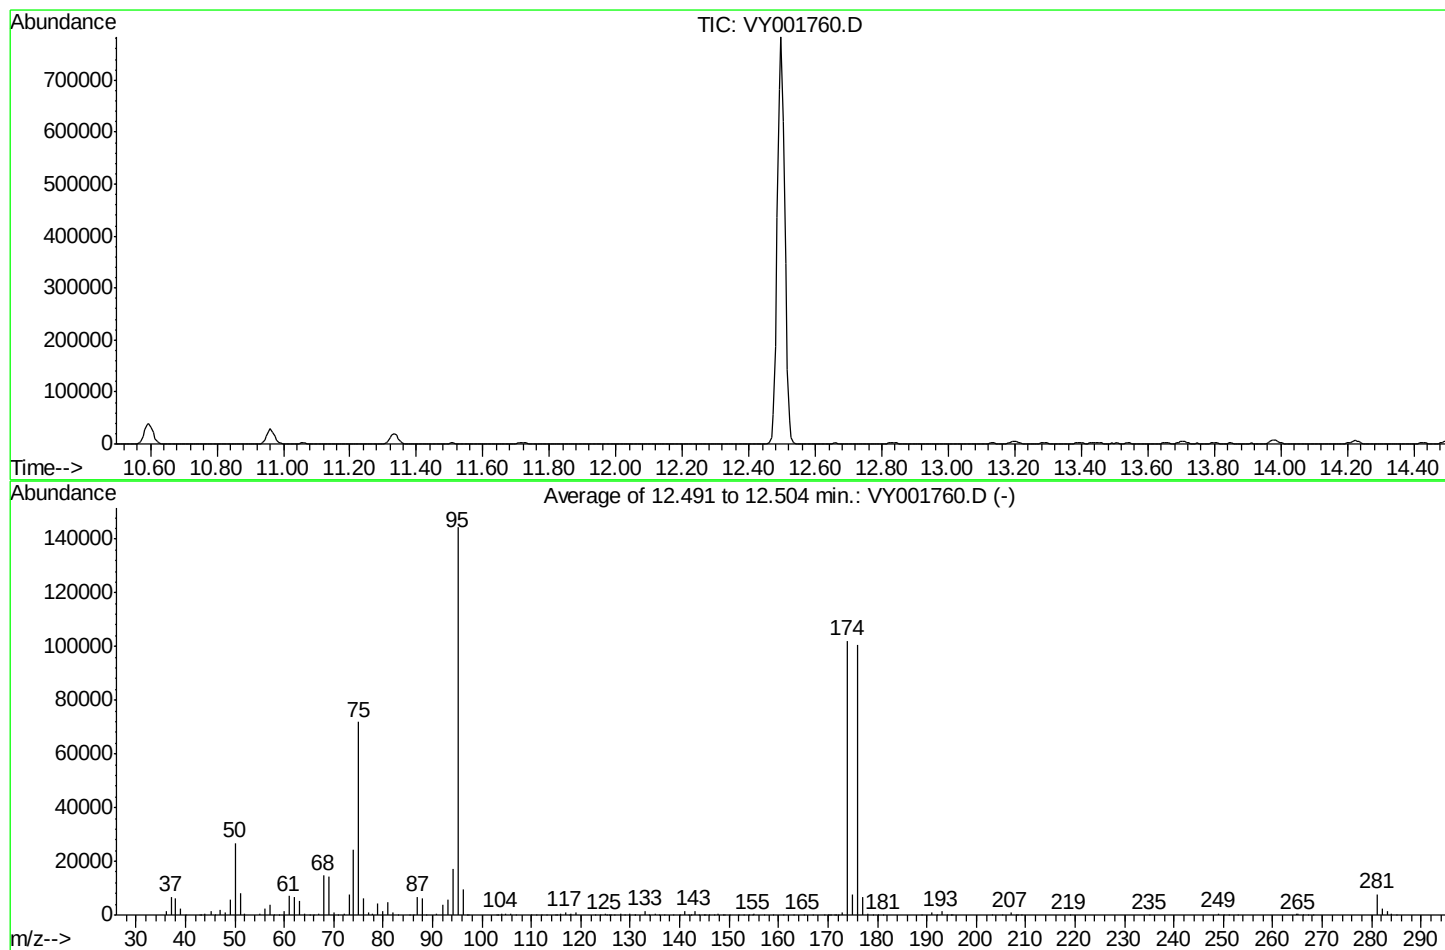

AutoFind: Scans 1764, 1765, 1766; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	26704	PASS
75	95	30	60	49.8	71960	PASS
95	95	100	100	100.0	144384	PASS
96	95	5	9	6.7	9632	PASS
173	174	0.00	2	0.8	843	PASS
174	95	50	100	70.7	102040	PASS
175	174	5	9	7.4	7528	PASS
176	174	95	101	98.6	100581	PASS
177	176	5	9	6.7	6747	PASS