
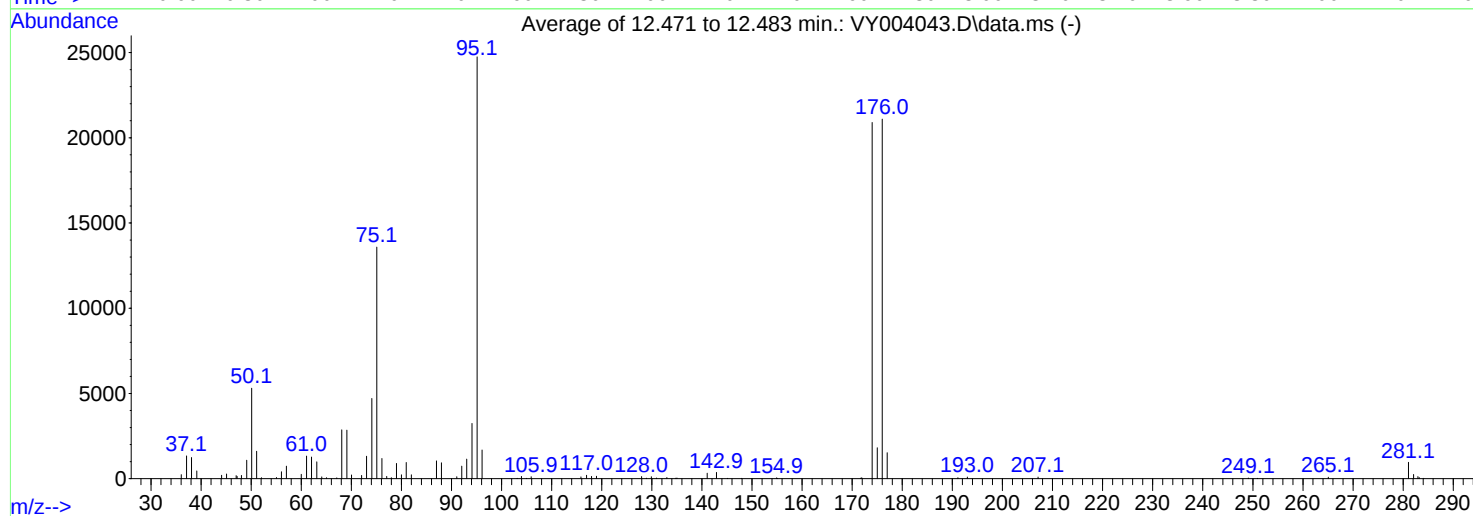


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022421\
 Data File : VY004043.D
 Acq On : 24 Feb 2021 09:42
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022215.M
 Title : SW846 8260
 Last Update : Tue Feb 23 03:42:58 2021

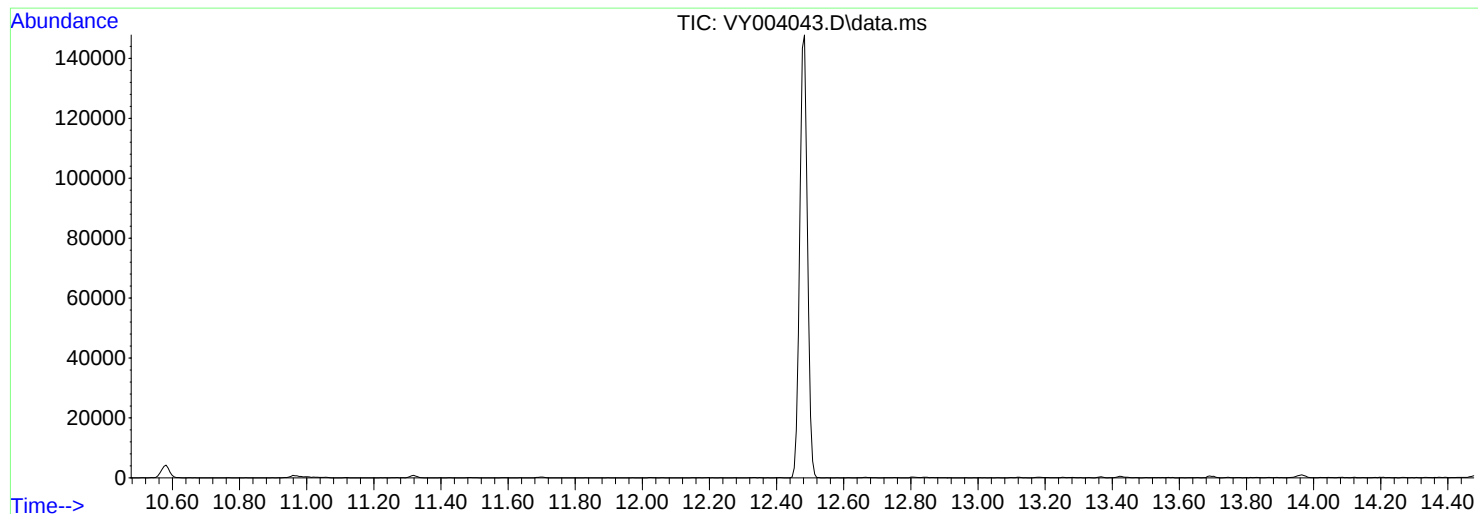

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	5301	PASS
75	95	30	60	54.9	13583	PASS
95	95	100	100	100.0	24752	PASS
96	95	5	9	6.8	1678	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.4	20897	PASS
175	174	5	9	8.7	1811	PASS
176	174	95	101	101.0	21101	PASS
177	176	5	9	7.2	1523	PASS