
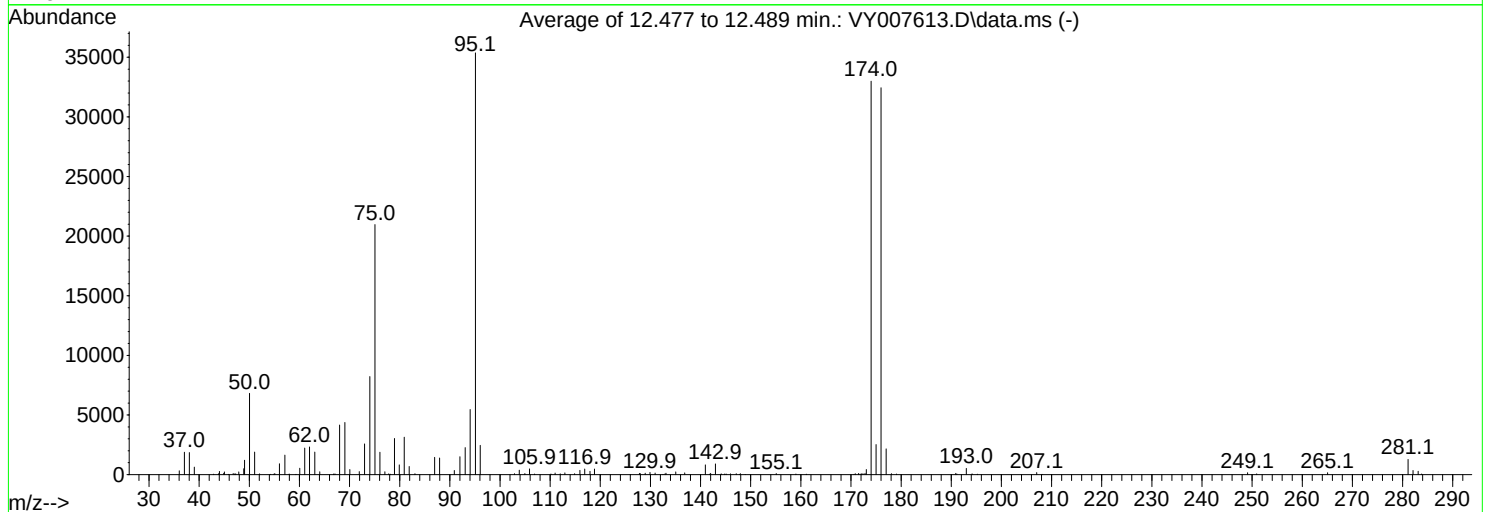


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022422\
 Data File : VY007613.D
 Acq On : 24 Feb 2022 10:03
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022322S.M
 Title : SW846 8260
 Last Update : Thu Feb 24 07:13:58 2022

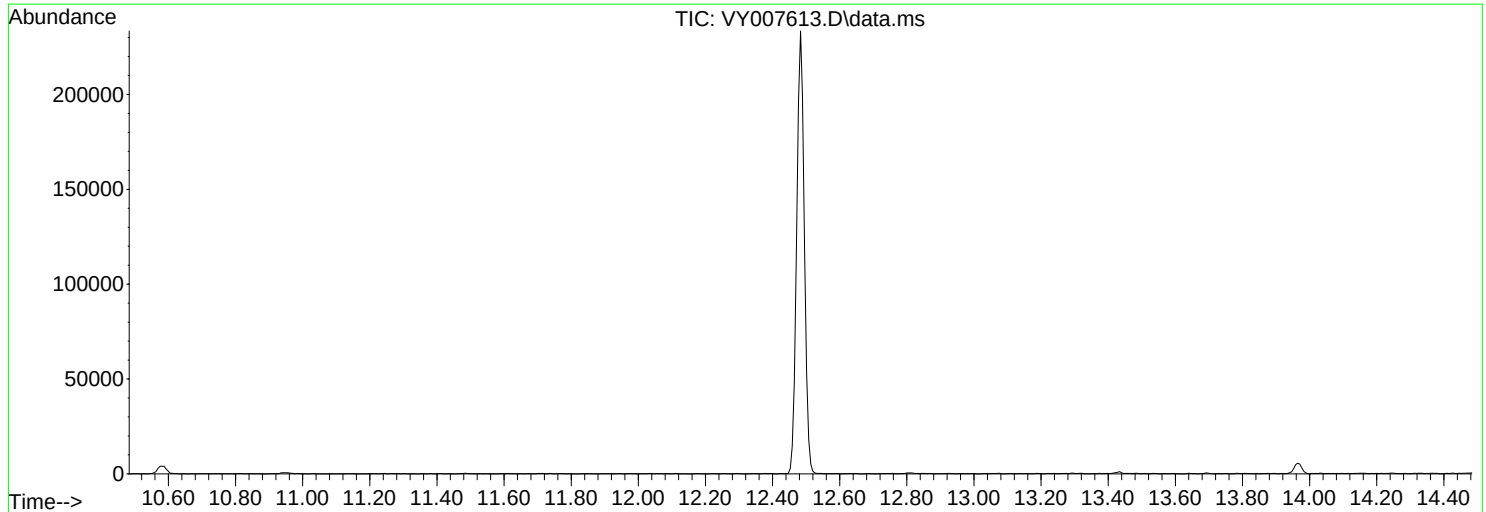

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	6811	PASS
75	95	30	60	59.3	20971	PASS
95	95	100	100	100.0	35368	PASS
96	95	5	9	6.9	2457	PASS
173	174	0.00	2	1.3	426	PASS
174	95	50	100	93.3	32992	PASS
175	174	5	9	7.6	2519	PASS
176	174	95	101	98.3	32445	PASS
177	176	5	9	6.7	2167	PASS