


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv022620\
 Data File : VY001772.D
 Acq On : 26 Feb 2020 09:39
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y021720S.M
 Title : SW846 8260
 Last Update : Mon Feb 17 12:19:53 2020

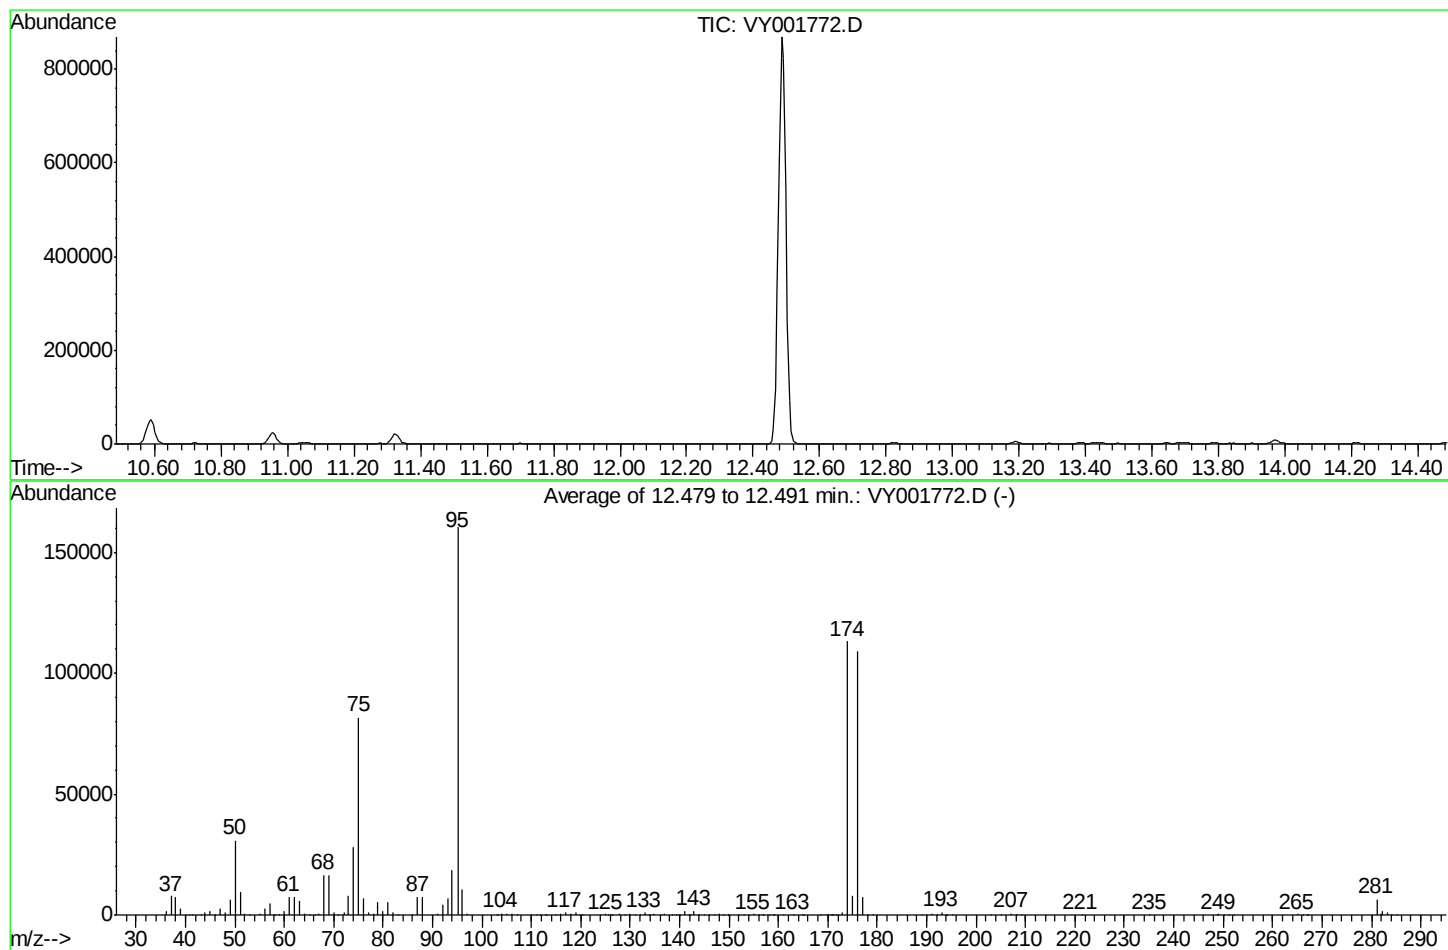

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	30928	PASS
75	95	30	60	50.9	81666	PASS
95	95	100	100	100.0	160384	PASS
96	95	5	9	6.7	10771	PASS
173	174	0.00	2	0.9	982	PASS
174	95	50	100	70.5	113082	PASS
175	174	5	9	7.3	8213	PASS
176	174	95	101	96.5	109072	PASS
177	176	5	9	6.7	7359	PASS