
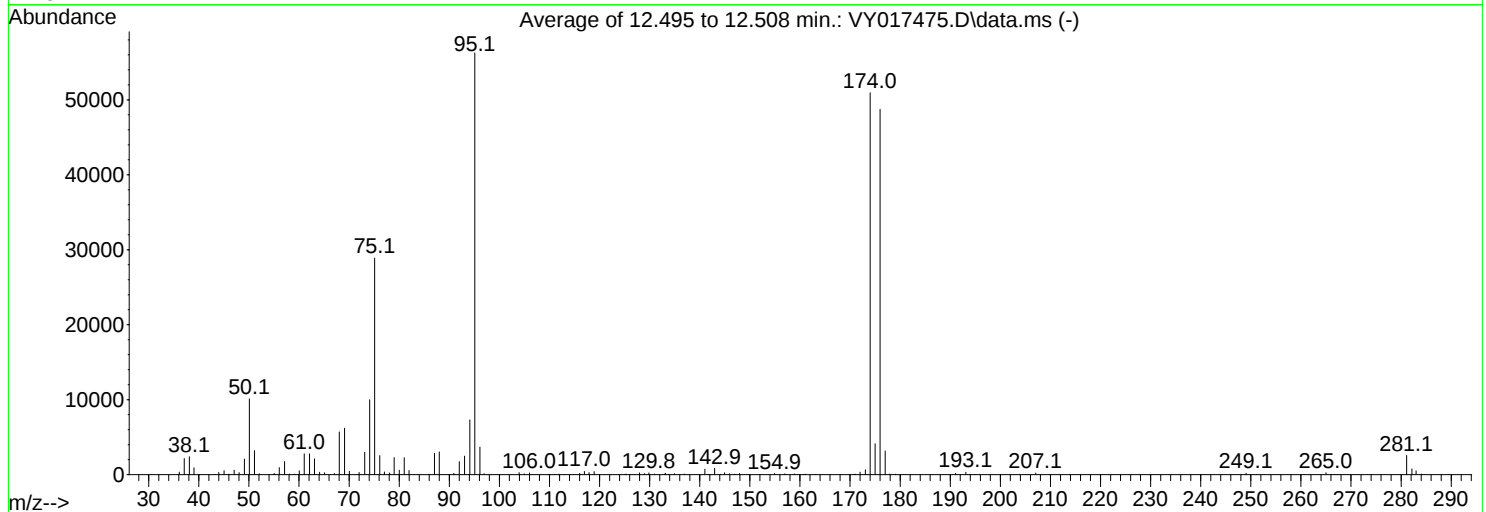


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022624\
Data File : VY017475.D
Acq On : 26 Feb 2024 08:26
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
Title : SW846 8260
Last Update : Sat Feb 24 04:41:20 2024

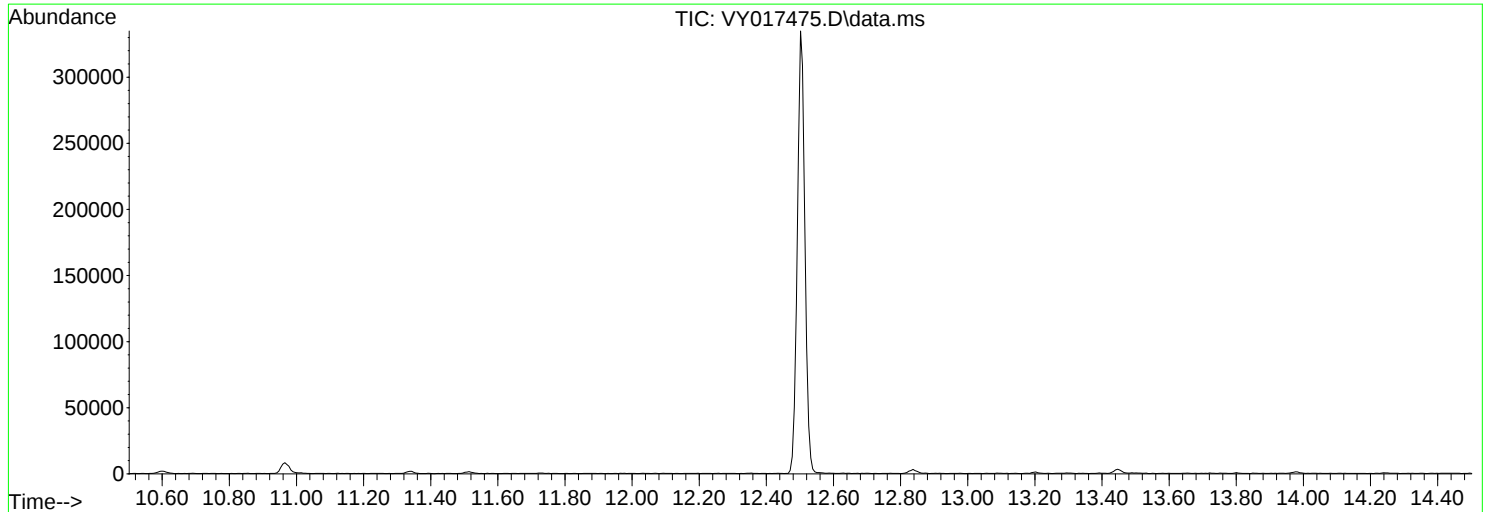

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	10120	PASS
75	95	30	60	51.3	28875	PASS
95	95	100	100	100.0	56269	PASS
96	95	5	9	6.5	3669	PASS
173	174	0.00	2	1.2	636	PASS
174	95	50	100	90.5	50947	PASS
175	174	5	9	8.1	4110	PASS
176	174	95	101	95.7	48741	PASS
177	176	5	9	6.5	3168	PASS