

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022723\
 Data File : VY012736.D
 Acq On : 27 Feb 2023 14:57
 Operator : KP/MD
 Sample : 01703-05
 Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 T2-STONE

Quant Time: Feb 28 00:22:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022123S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 22 01:21:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	147439	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	239028	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	209207	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	94640	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	89978	51.672	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.340%
35) Dibromofluoromethane	7.716	113	87702	54.322	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.640%
50) Toluene-d8	10.179	98	317354	52.468	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.940%
62) 4-Bromofluorobenzene	12.483	95	97661	50.456	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	100.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022723\
Data File : VY012736.D
Acq On : 27 Feb 2023 14:57
Operator : KP/MD
Sample : 01703-05
Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
T2-STONE

Quant Time: Feb 28 00:22:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022123S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 22 01:21:05 2023
Response via : Initial Calibration




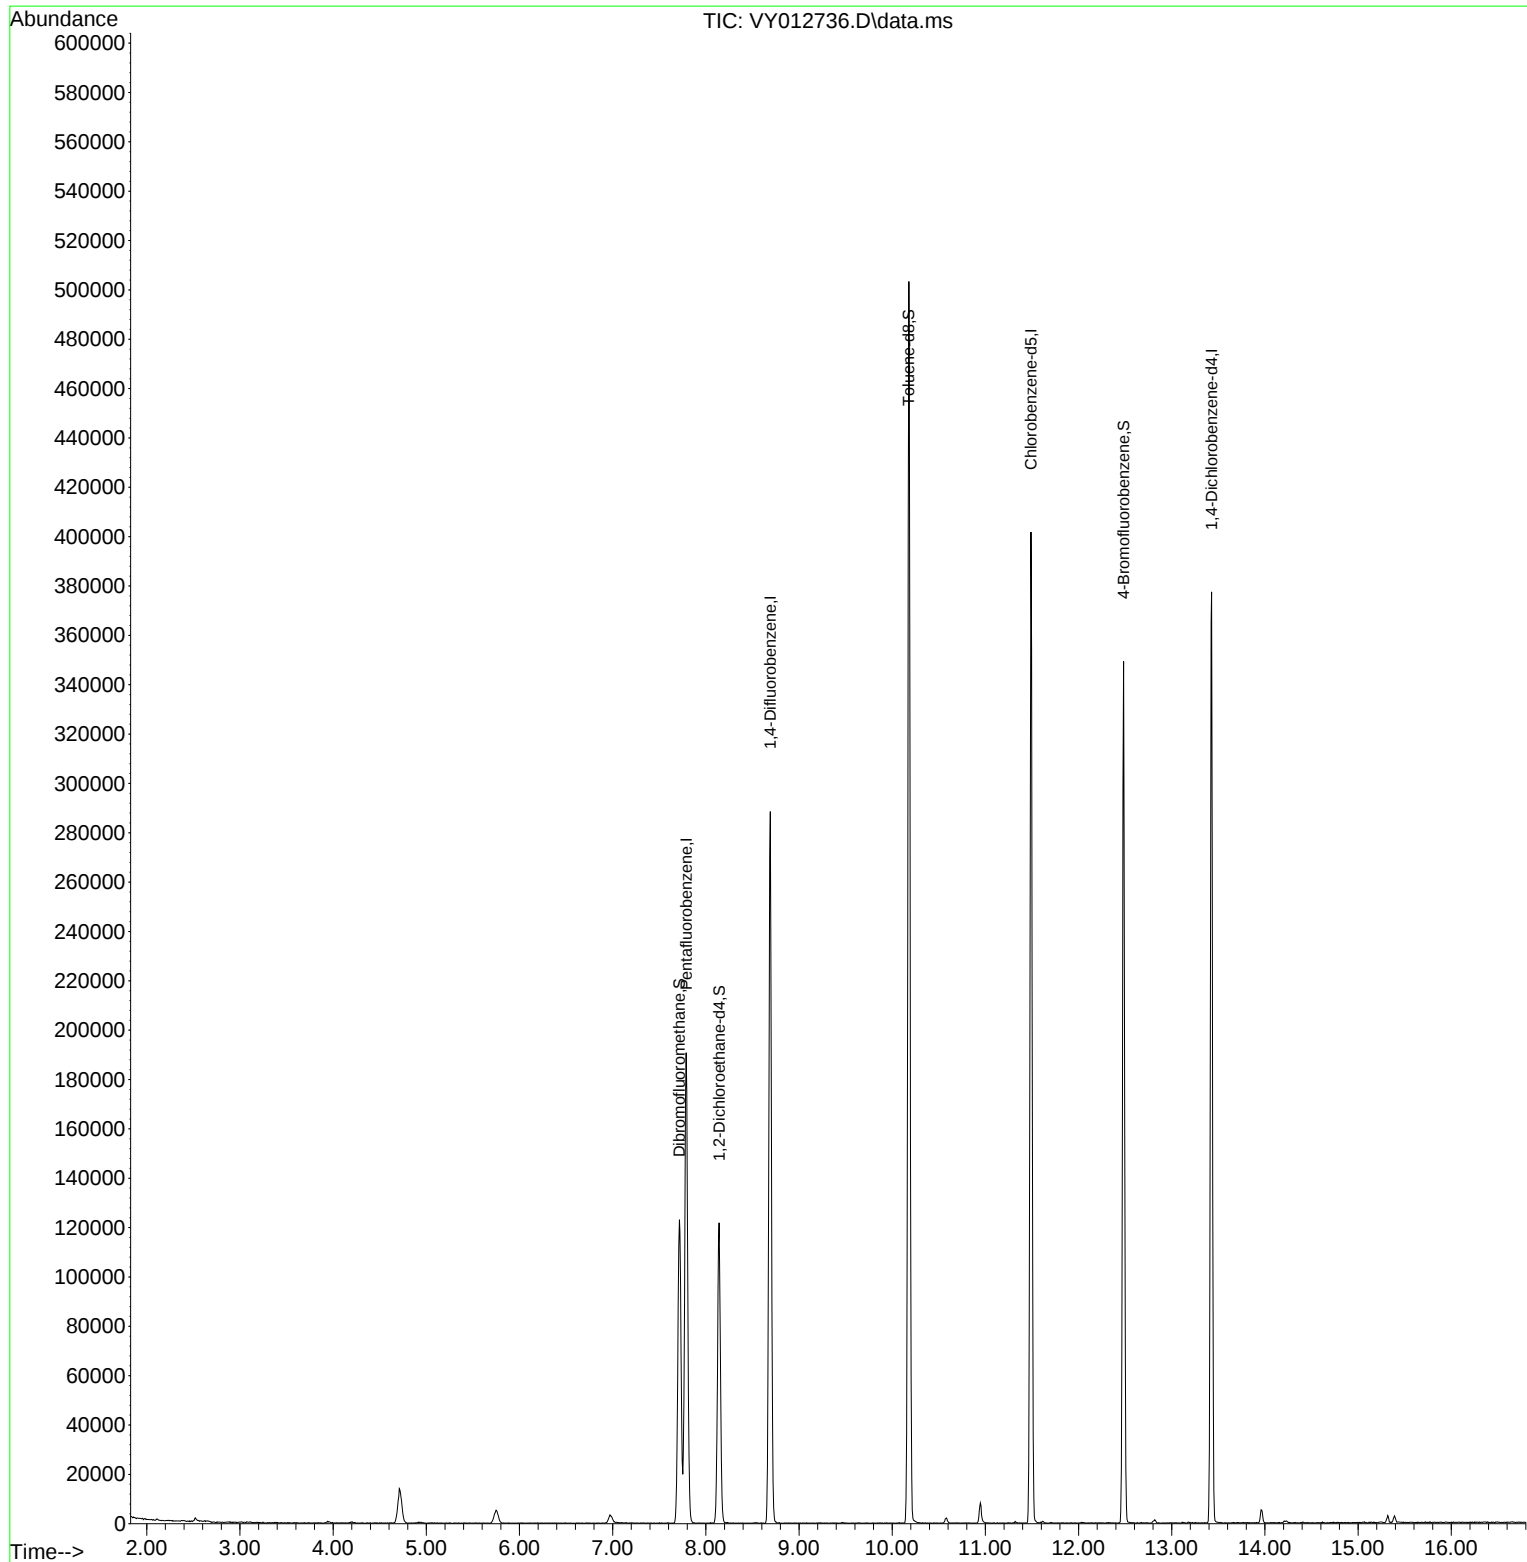


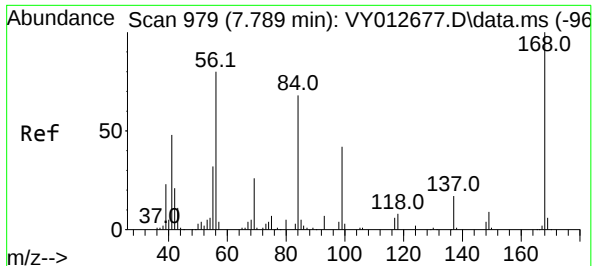

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012736.D
Acq: 27 Feb 2023 14:57




Instrument :
MSVOA_Y
ClientSampleId :
T2-STONE


Tgt Ion:168 Resp: 147439
Ion Ratio Lower Upper
168 100
99 55.5 45.4 68.2

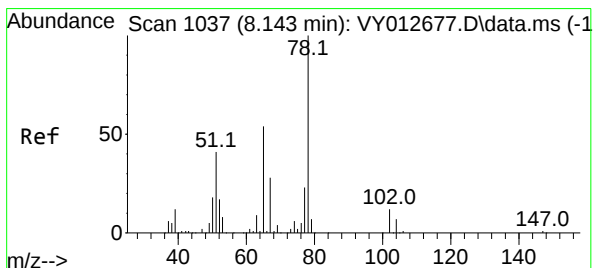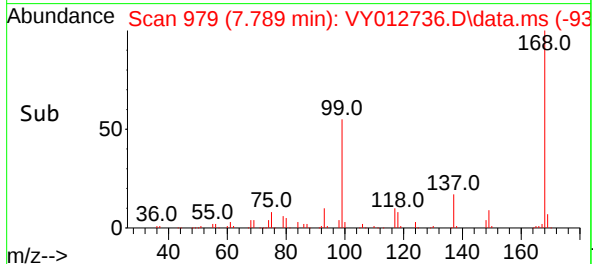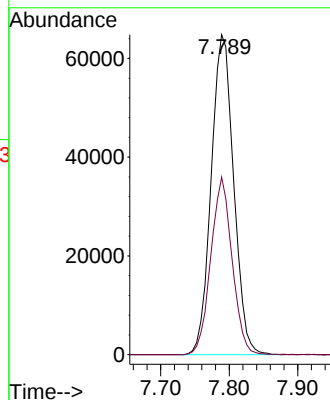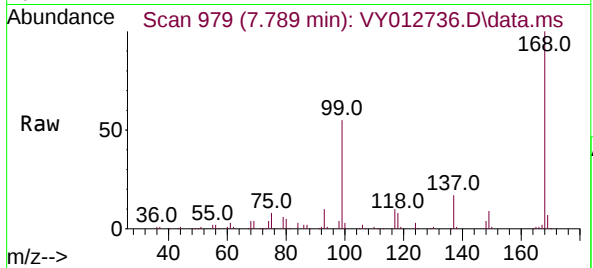

#33
1,2-Dichloroethane-d4
Concen: 51.672 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY012736.D
Acq: 27 Feb 2023 14:57

Tgt Ion: 65 Resp: 89978
Ion Ratio Lower Upper
65 100
67 54.0 0.0 104.6

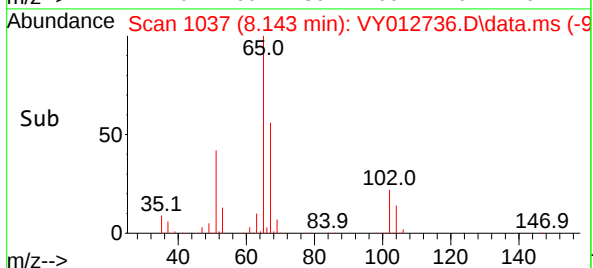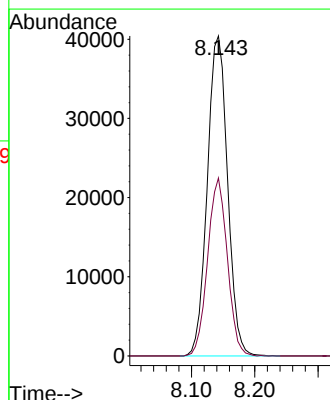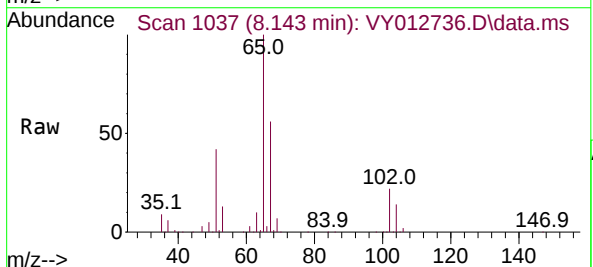

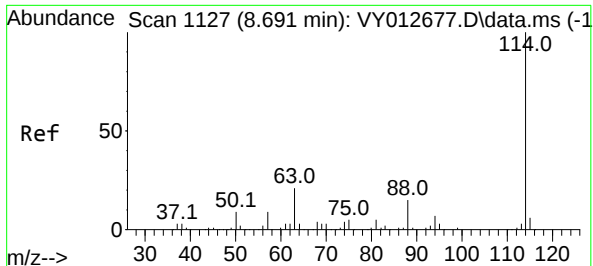

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY012736.D

Acq: 27 Feb 2023 14:57

Instrument :

MSVOA_Y

ClientSampleId :

T2-STONE





Tgt Ion:114 Resp: 239028

Ion Ratio Lower Upper

114 100

63 20.3 0.0 42.8

88 14.7 0.0 29.6

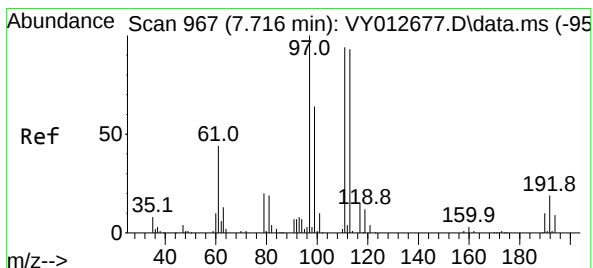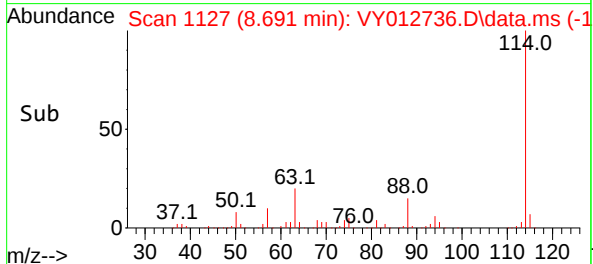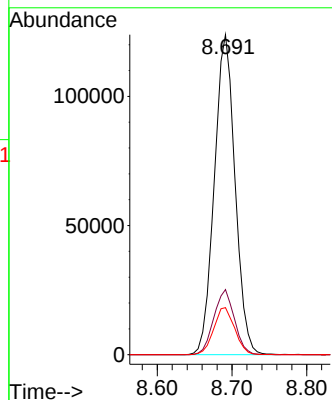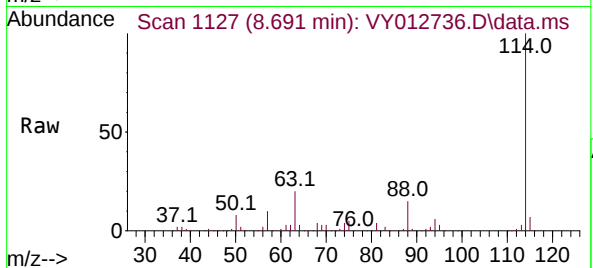

#35

Dibromofluoromethane

Concen: 54.322 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012736.D

Acq: 27 Feb 2023 14:57




Tgt Ion:113 Resp: 87702


Ion Ratio Lower Upper

113 100

111 102.8 82.0 123.0

192 20.6 16.2 24.2


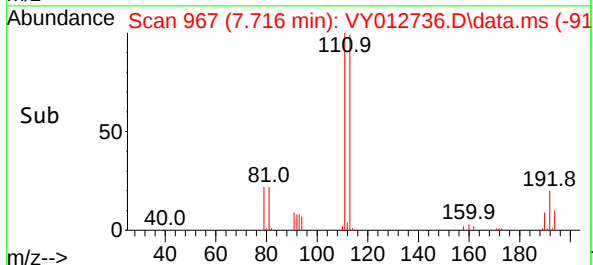
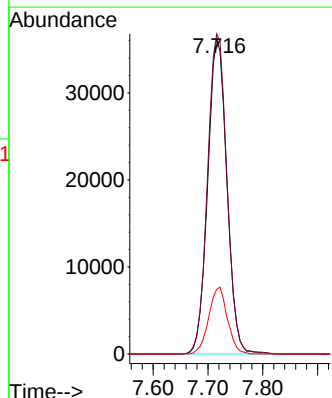
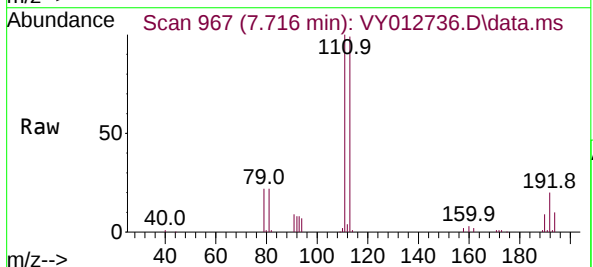


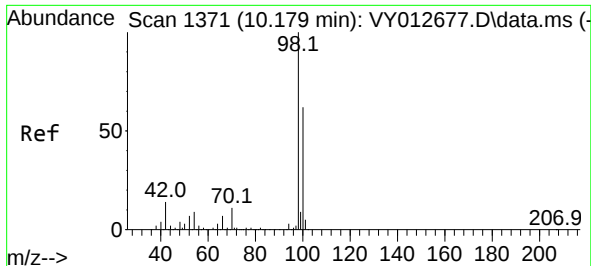

#50
Toluene-d8
Concen: 52.468 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY012736.D
Acq: 27 Feb 2023 14:57




Instrument :
MSVOA_Y
ClientSampleId :
T2-STONE


Tgt Ion: 98 Resp: 317354
Ion Ratio Lower Upper
98 100
100 63.7 51.2 76.8

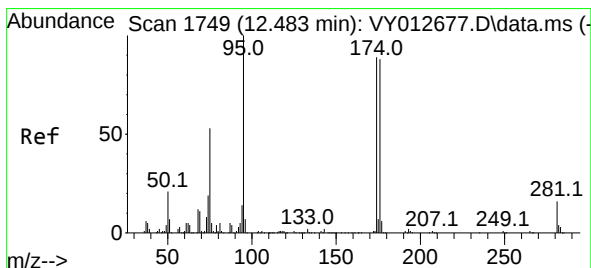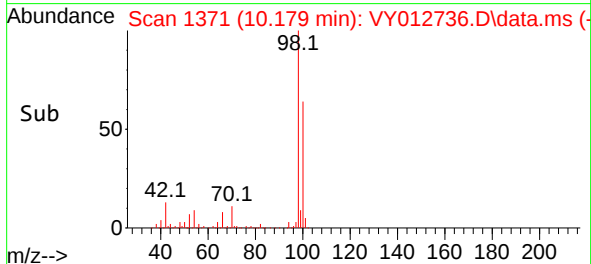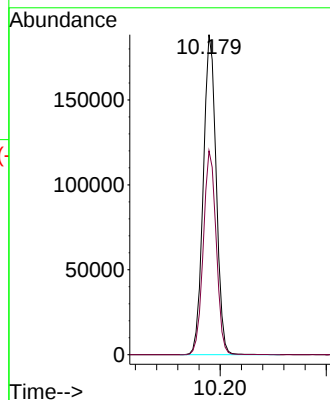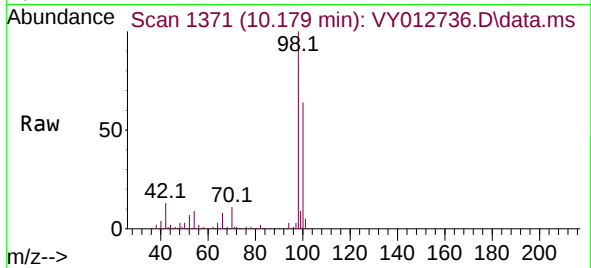

#62
4-Bromofluorobenzene
Concen: 50.456 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012736.D
Acq: 27 Feb 2023 14:57

Tgt Ion: 95 Resp: 97661
Ion Ratio Lower Upper
95 100
174 89.4 0.0 172.8
176 85.2 0.0 169.4

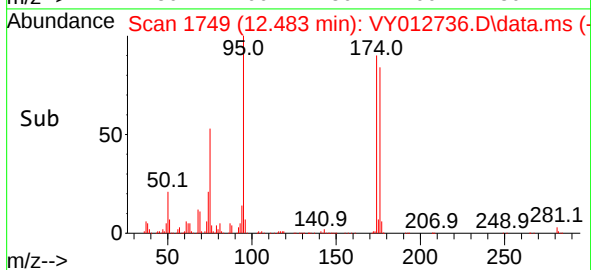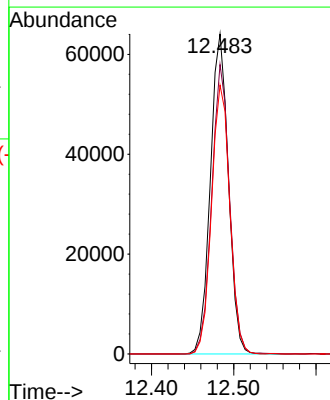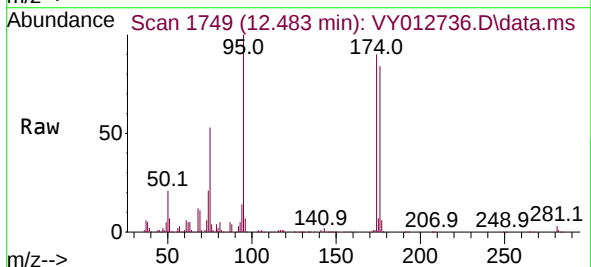

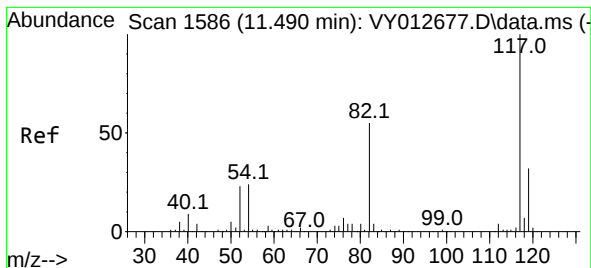

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY012736.D

Acq: 27 Feb 2023 14:57

Instrument :

MSVOA_Y

ClientSampleId :

T2-STONE





Tgt Ion:117 Resp: 209207

Ion Ratio Lower Upper

117 100

82 53.9 44.1 66.1

119 32.3 25.5 38.3

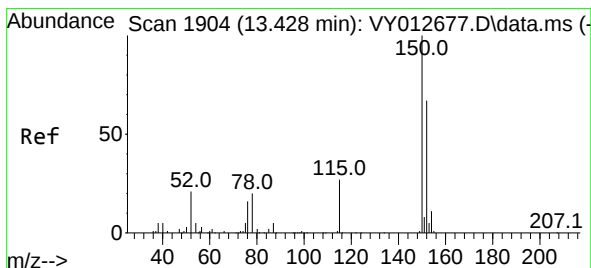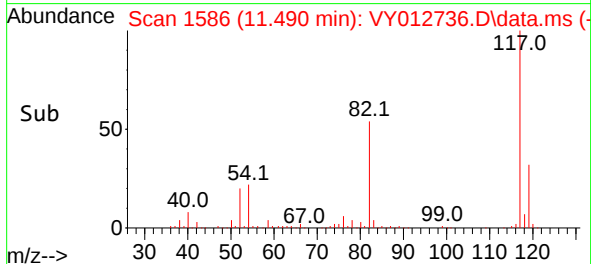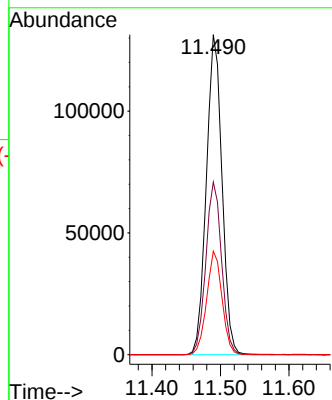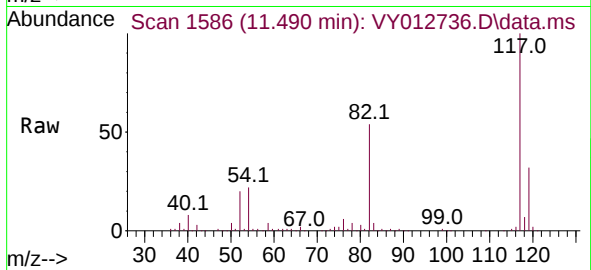

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY012736.D

Acq: 27 Feb 2023 14:57

Tgt Ion:152 Resp: 94640

Ion Ratio Lower Upper

152 100

115 55.6 28.7 86.3

150 158.2 0.0 347.6

