
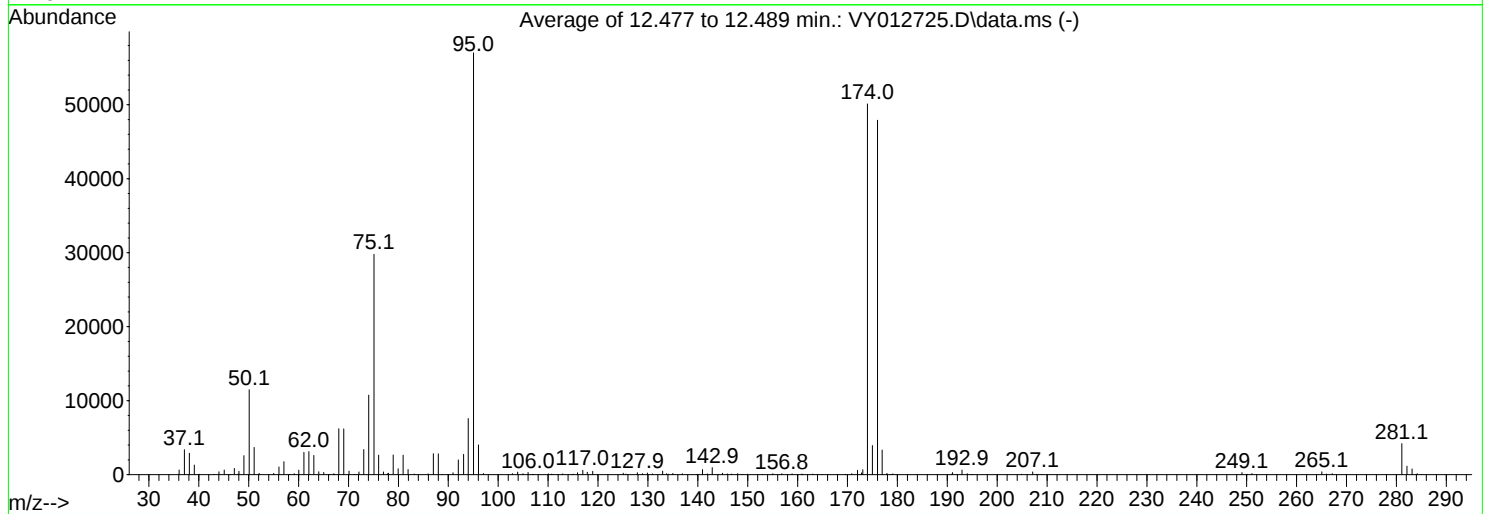


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022723\
 Data File : VY012725.D
 Acq On : 27 Feb 2023 09:35
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022123S.M
 Title : SW846 8260
 Last Update : Wed Feb 22 01:21:05 2023

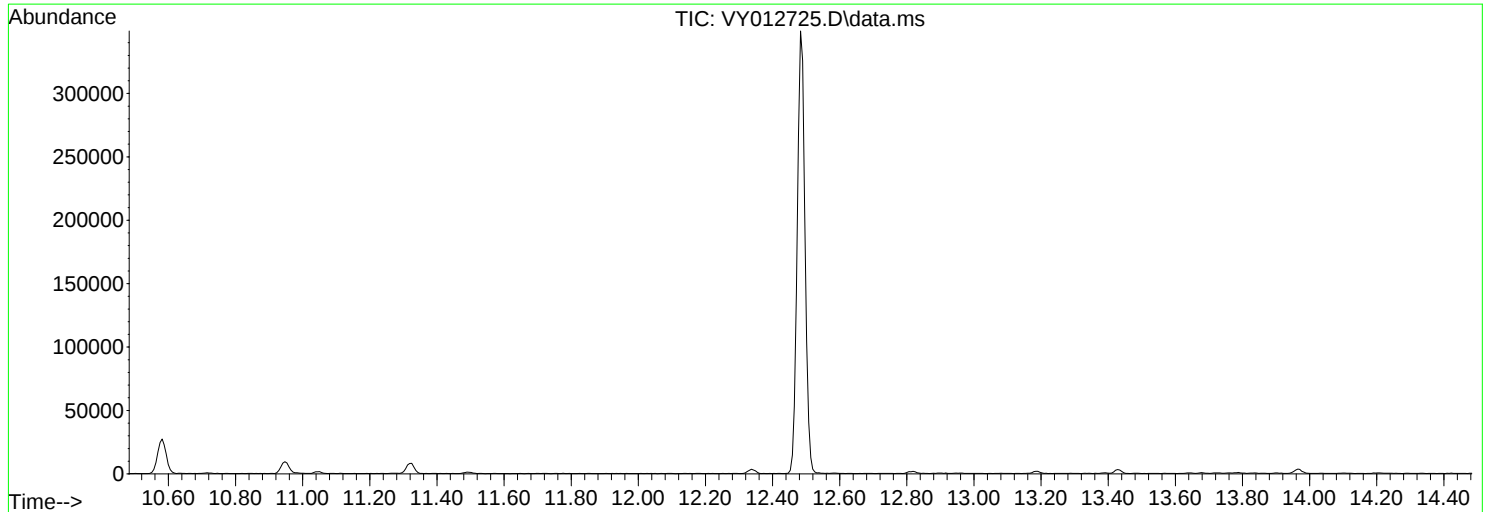

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	11486	PASS
75	95	30	60	52.2	29787	PASS
95	95	100	100	100.0	57019	PASS
96	95	5	9	7.1	4024	PASS
173	174	0.00	2	1.3	675	PASS
174	95	50	100	87.9	50107	PASS
175	174	5	9	7.9	3939	PASS
176	174	95	101	95.6	47917	PASS
177	176	5	9	6.9	3327	PASS