


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022725\
Data File : VY021345.D
Acq On : 27 Feb 2025 09:41
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022525S.M
Title : SW846 8260
Last Update : Wed Feb 26 02:09:13 2025

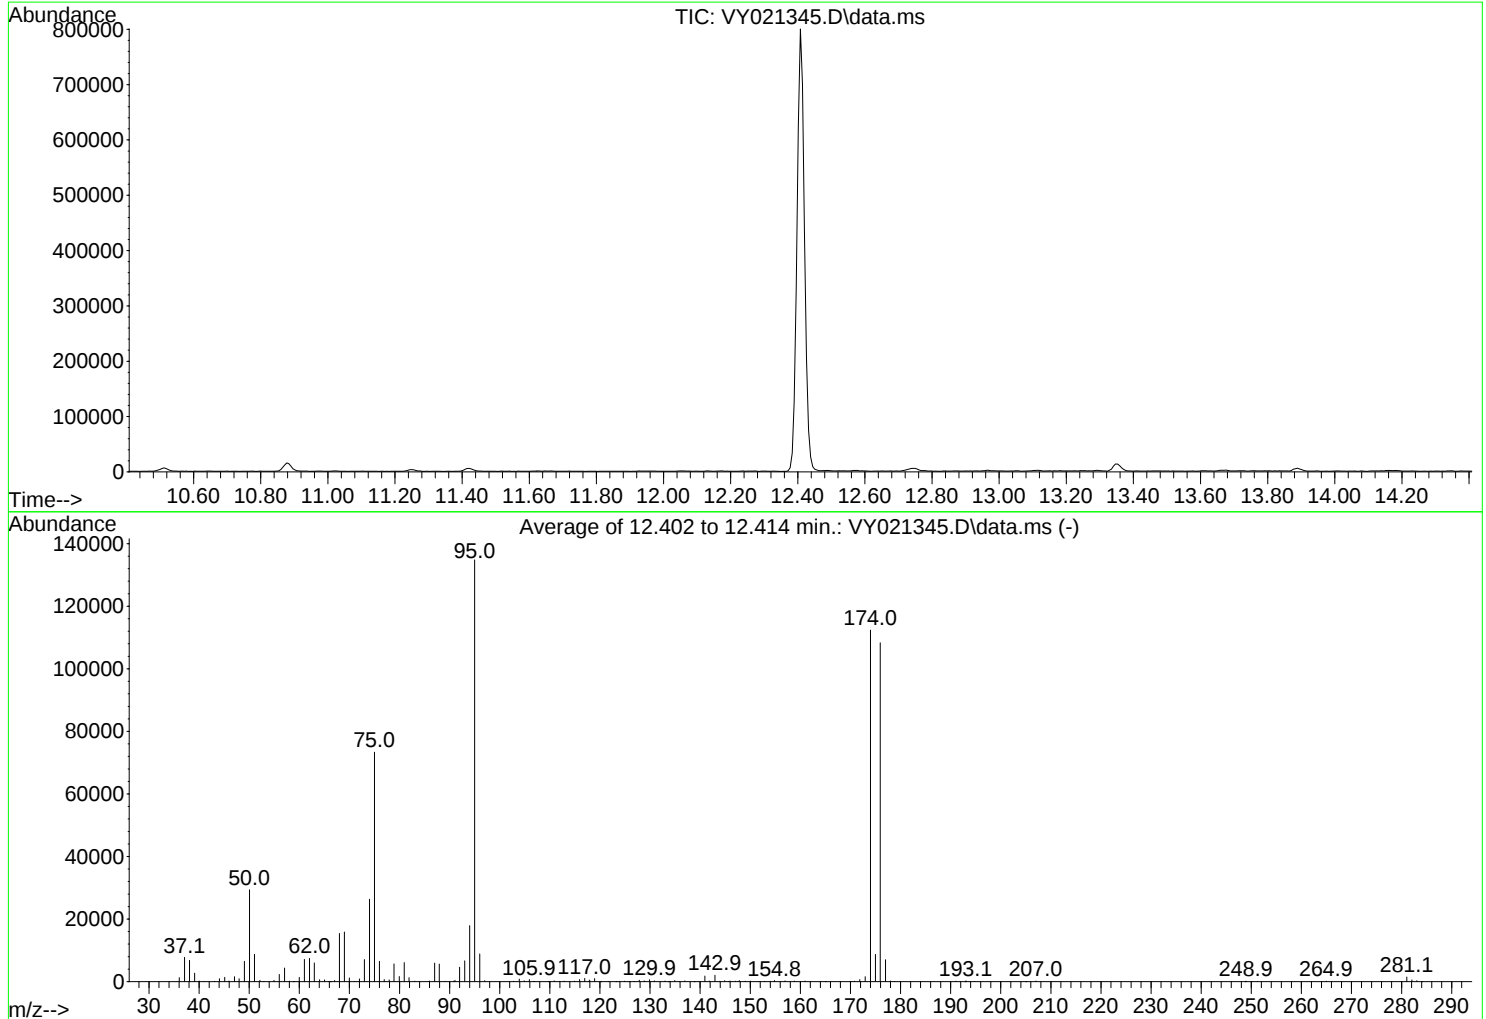

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.8	29339	PASS
75	95	30	60	54.4	73368	PASS
95	95	100	100	100.0	134840	PASS
96	95	5	9	6.6	8843	PASS
173	174	0.00	2	1.4	1606	PASS
174	95	50	100	83.3	112365	PASS
175	174	5	9	7.8	8726	PASS
176	174	95	101	96.4	108357	PASS
177	176	5	9	6.5	7010	PASS