
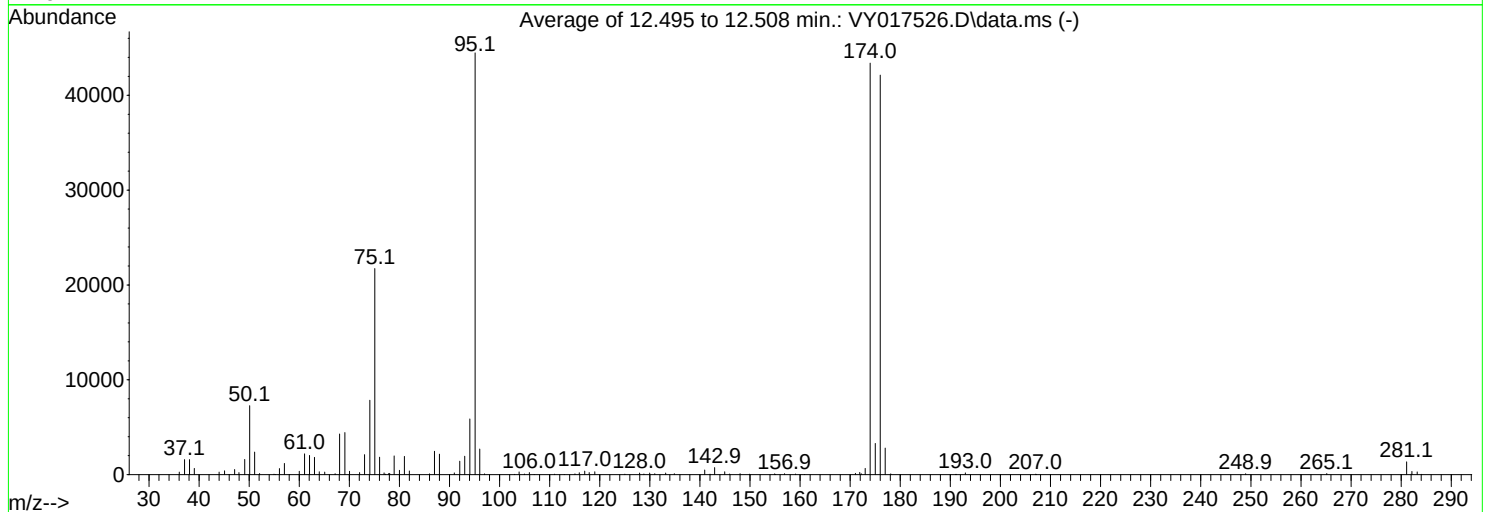


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022924\
Data File : VY017526.D
Acq On : 29 Feb 2024 08:29
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
Title : SW846 8260
Last Update : Sat Feb 24 04:41:20 2024

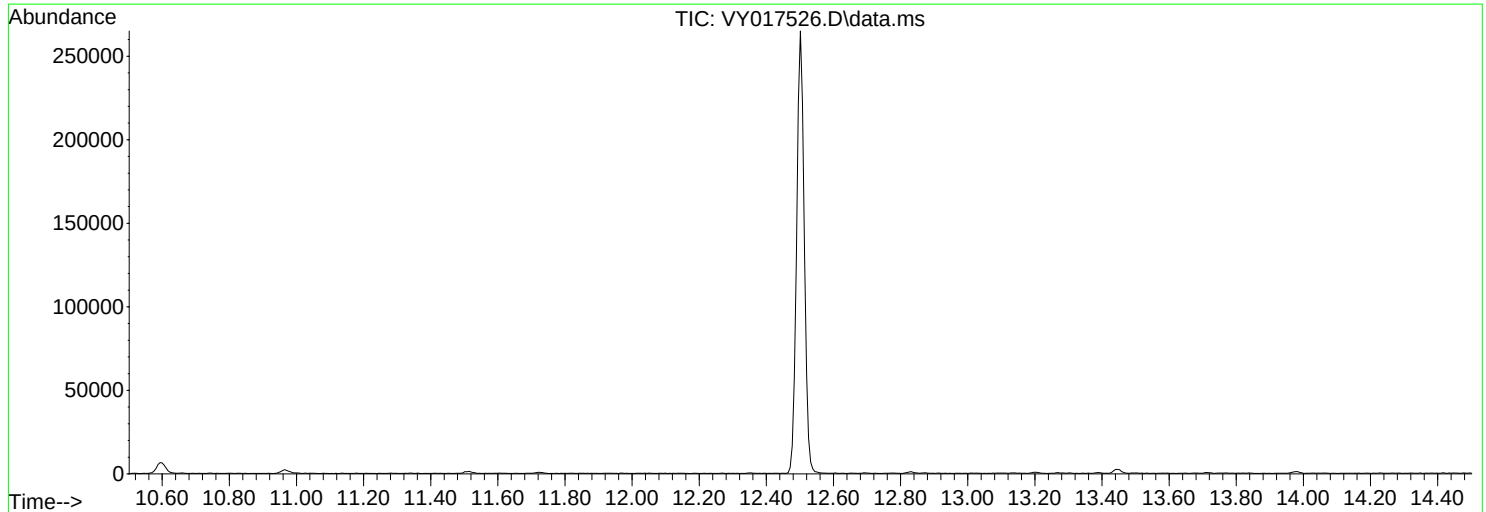

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	7272	PASS
75	95	30	60	48.9	21739	PASS
95	95	100	100	100.0	44475	PASS
96	95	5	9	6.1	2706	PASS
173	174	0.00	2	1.5	652	PASS
174	95	50	100	97.6	43389	PASS
175	174	5	9	7.6	3285	PASS
176	174	95	101	97.1	42128	PASS
177	176	5	9	6.7	2803	PASS