

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030124\
 Data File : VY017552.D
 Acq On : 01 Mar 2024 15:50
 Operator : SY/MD
 Sample : P1639-31
 Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SP-8

Quant Time: Mar 02 00:19:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 24 04:41:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	103662	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	191907	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	165573	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.434	152	59775	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	50864	51.773	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.540%
35) Dibromofluoromethane	7.728	113	61498	45.988	ug/l	0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	91.980%
50) Toluene-d8	10.185	98	216509	46.306	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	92.620%
62) 4-Bromofluorobenzene	12.489	95	55297	37.632	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	75.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030124\
Data File : VY017552.D
Acq On : 01 Mar 2024 15:50
Operator : SY/MD
Sample : P1639-31
Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SP-8

Quant Time: Mar 02 00:19:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
Quant Title : SW846 8260
QLast Update : Sat Feb 24 04:41:20 2024
Response via : Initial Calibration




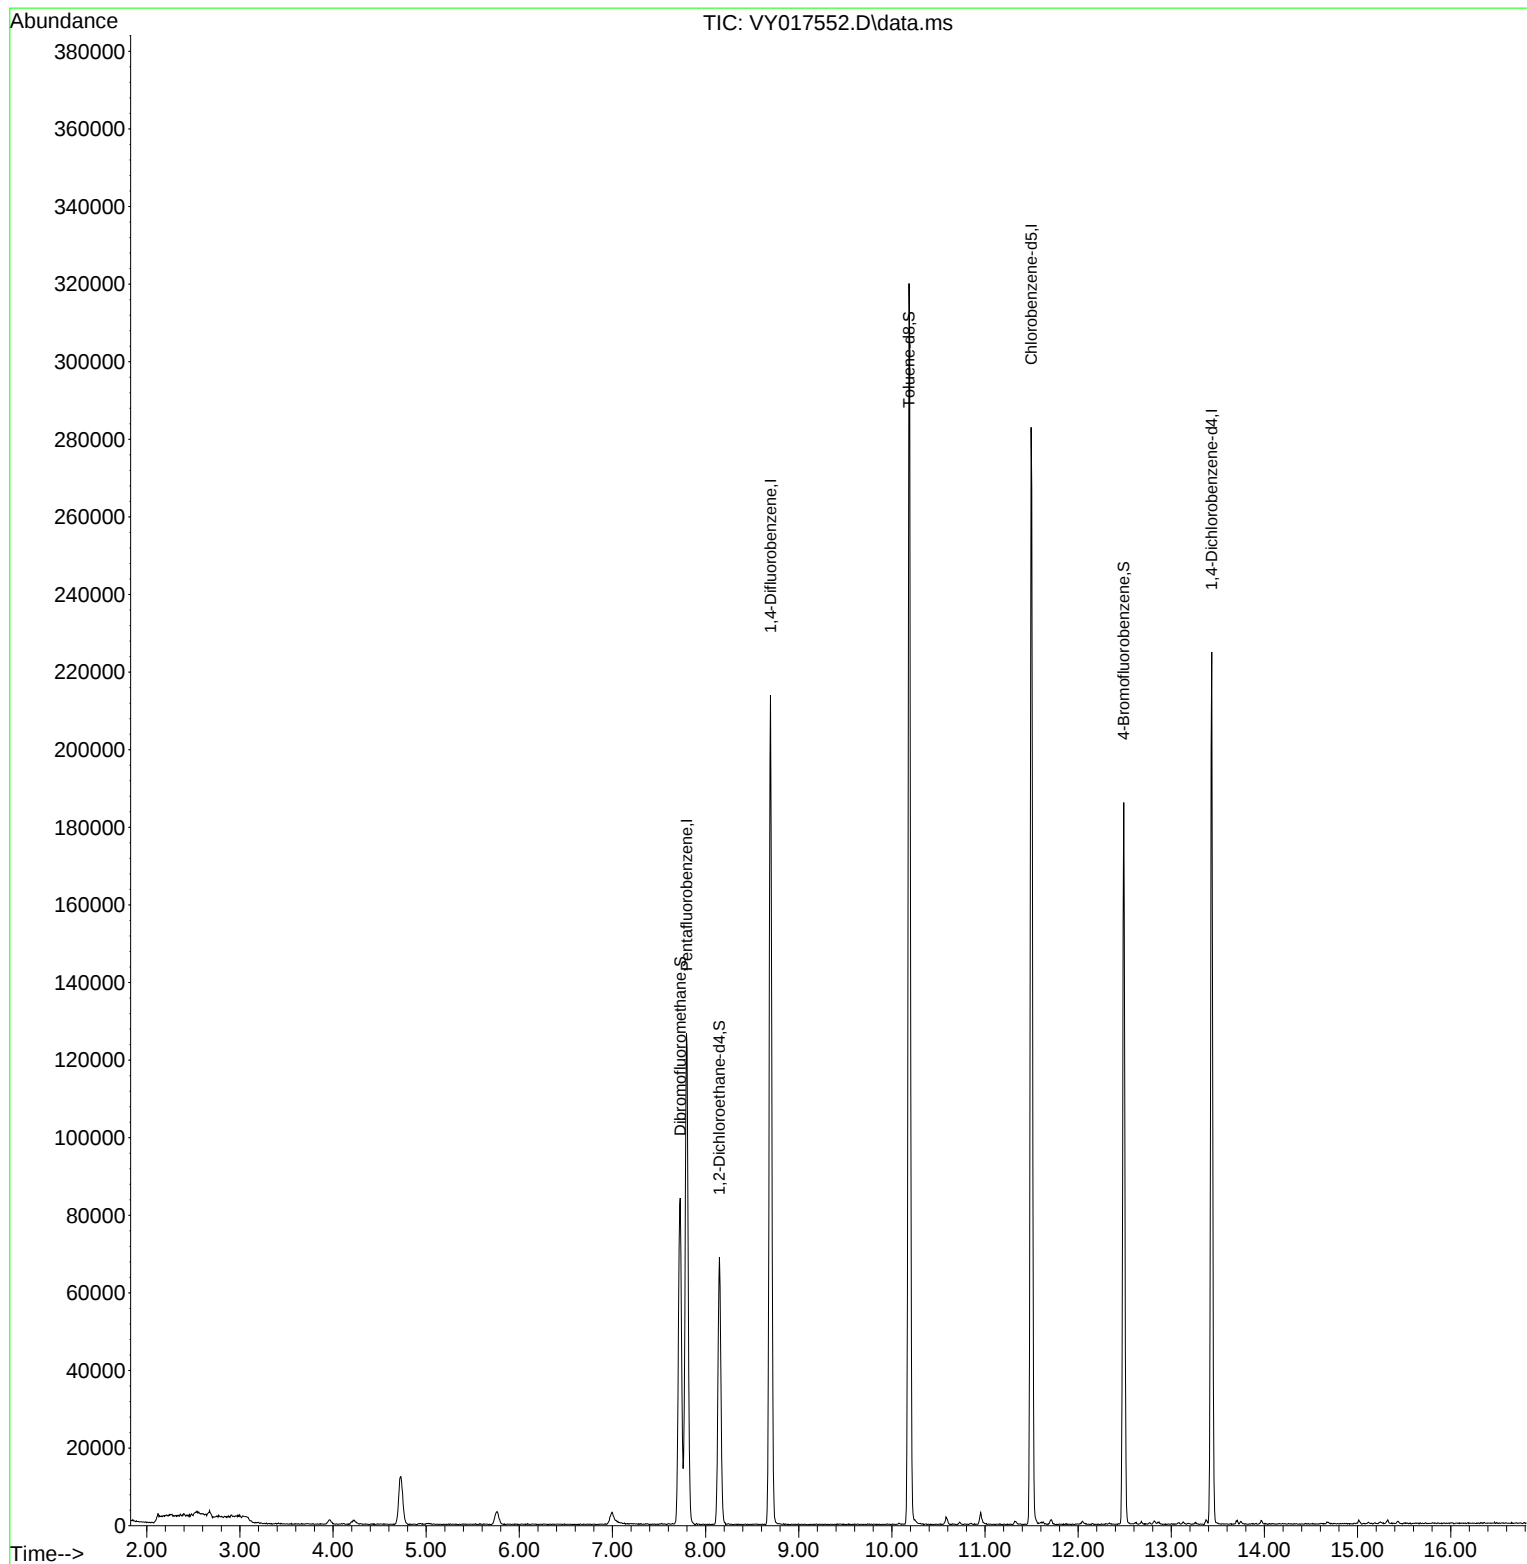


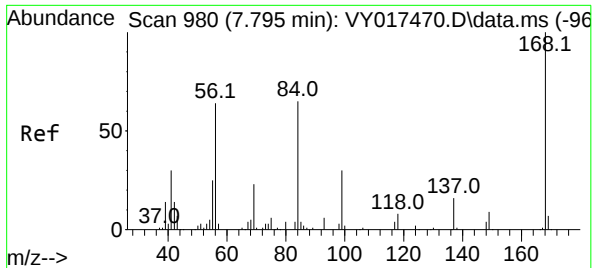

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY017552.D
Acq: 01 Mar 2024 15:50




Instrument :
MSVOA_Y
ClientSampleId :
SP-8


Tgt Ion:168 Resp: 103662
Ion Ratio Lower Upper
168 100
99 48.5 39.1 58.7

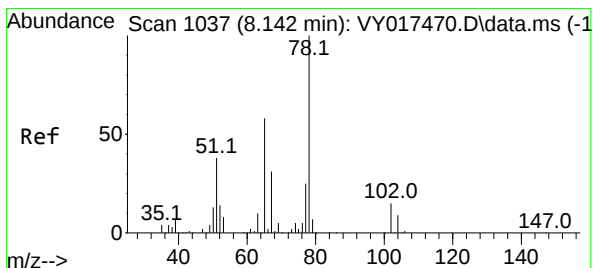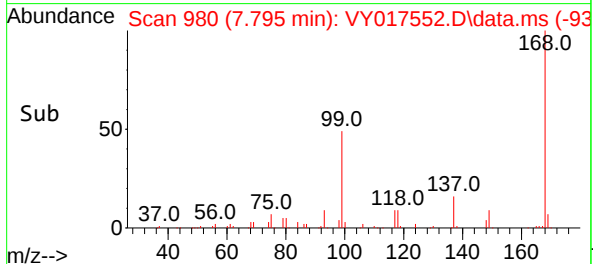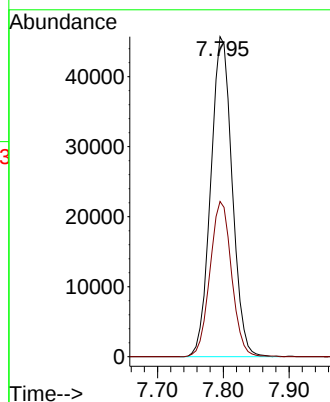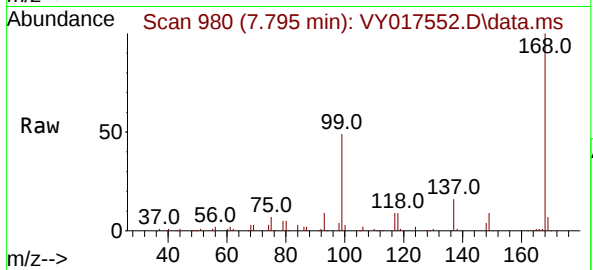

#33
1,2-Dichloroethane-d4
Concen: 51.773 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.006 min
Lab File: VY017552.D
Acq: 01 Mar 2024 15:50

Tgt Ion: 65 Resp: 50864
Ion Ratio Lower Upper
65 100
67 56.7 0.0 109.6

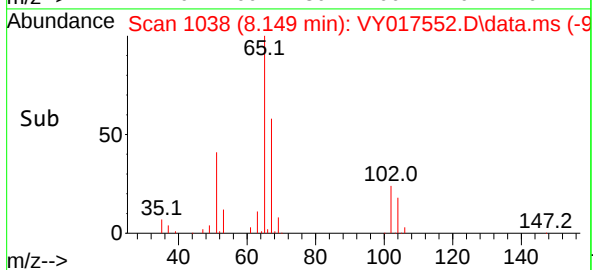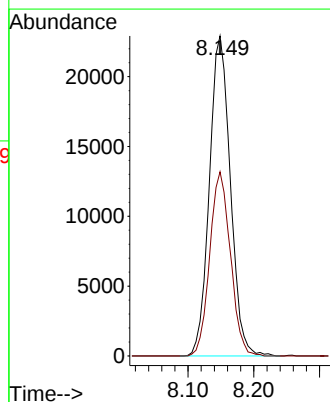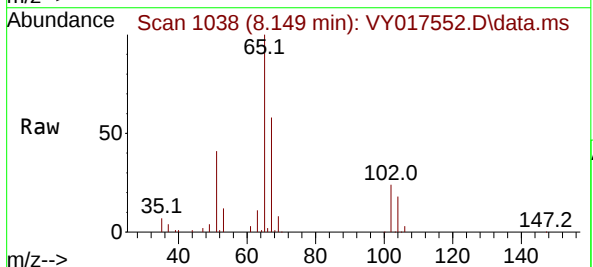

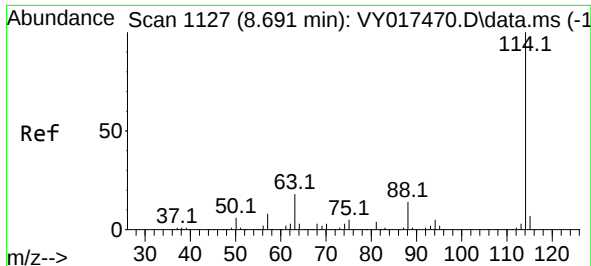

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.697 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY017552.D

Acq: 01 Mar 2024 15:50

Instrument :

MSVOA_Y

ClientSampleId :

SP-8




Tgt Ion:114 Resp: 191907

Ion Ratio Lower Upper

114 100

63 17.9 0.0 35.0

88 13.5 0.0 27.2

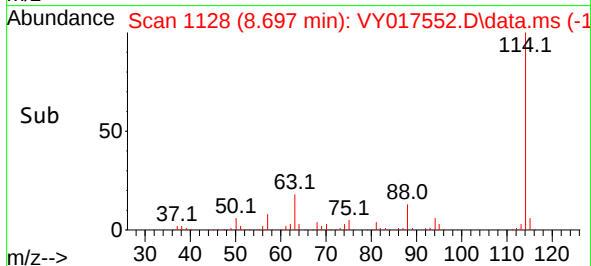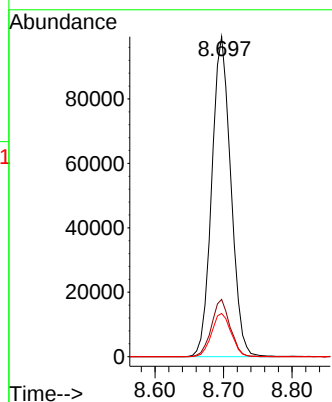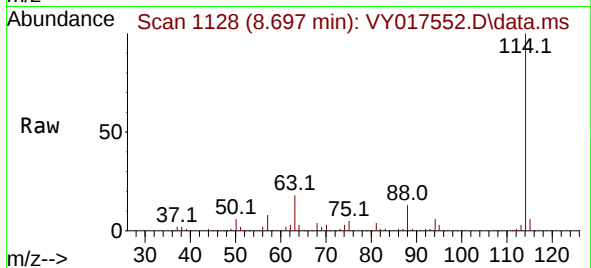

#35

Dibromofluoromethane

Concen: 45.988 ug/l

RT: 7.728 min Scan# 969

Delta R.T. 0.012 min

Lab File: VY017552.D

Acq: 01 Mar 2024 15:50




Tgt Ion:113 Resp: 61498


Ion Ratio Lower Upper

113 100

111 102.3 82.2 123.4

192 20.4 15.9 23.9

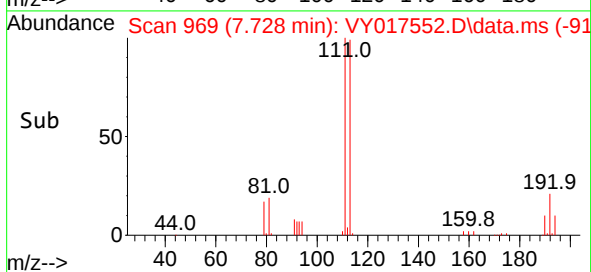
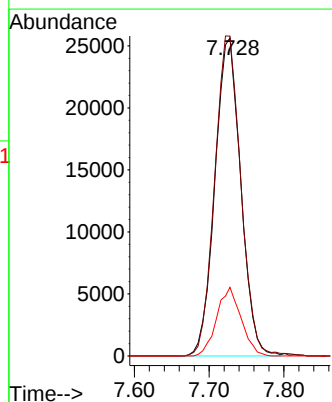
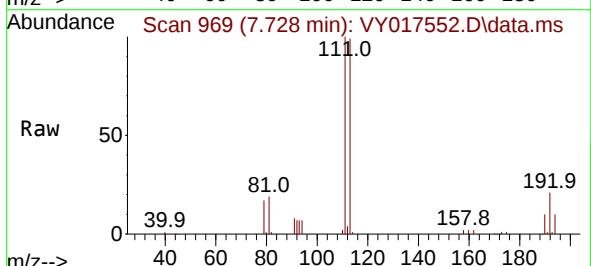


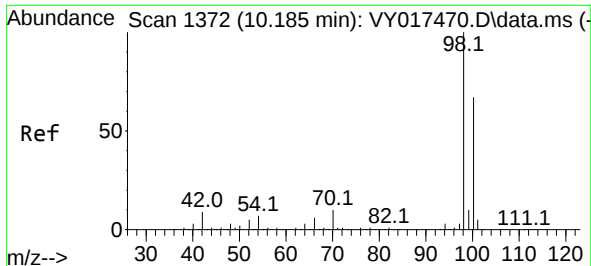

#50
Toluene-d8
Concen: 46.306 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY017552.D
Acq: 01 Mar 2024 15:50




Instrument :
MSVOA_Y
ClientSampleId :
SP-8


Tgt Ion: 98 Resp: 216509
Ion Ratio Lower Upper
98 100
100 64.7 52.0 78.0

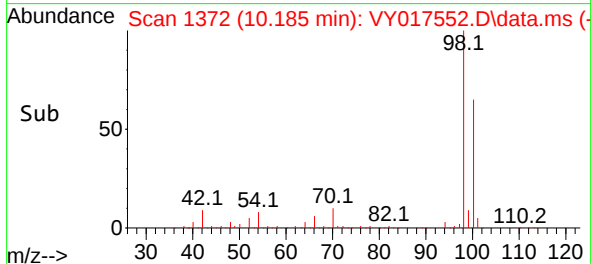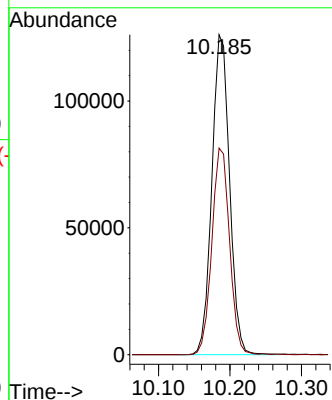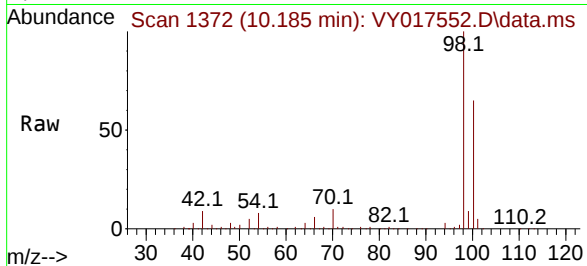

#62
4-Bromofluorobenzene
Concen: 37.632 ug/l
RT: 12.489 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VY017552.D
Acq: 01 Mar 2024 15:50

Tgt Ion: 95 Resp: 55297
Ion Ratio Lower Upper
95 100
174 94.3 0.0 175.6
176 88.4 0.0 171.4

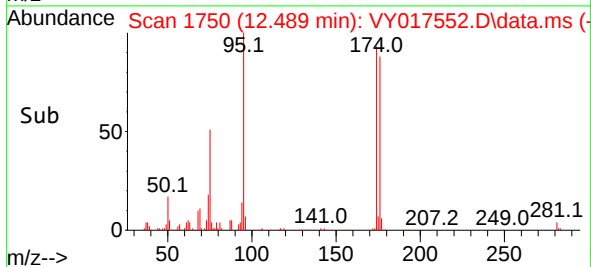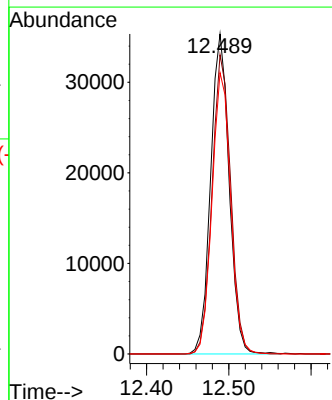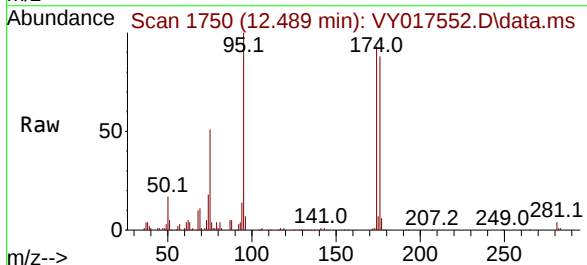

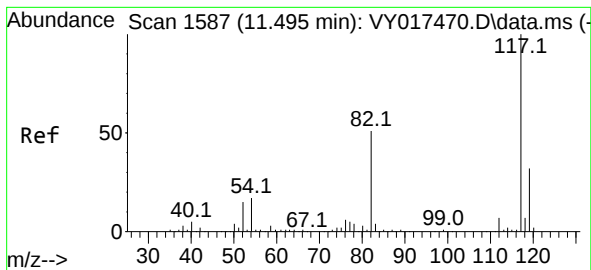

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.496 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY017552.D

Acq: 01 Mar 2024 15:50

Instrument :

MSVOA_Y

ClientSampleId :

SP-8





Tgt Ion:117 Resp: 165573

Ion Ratio Lower Upper

117 100

82 52.1 42.4 63.6

119 32.3 25.9 38.9

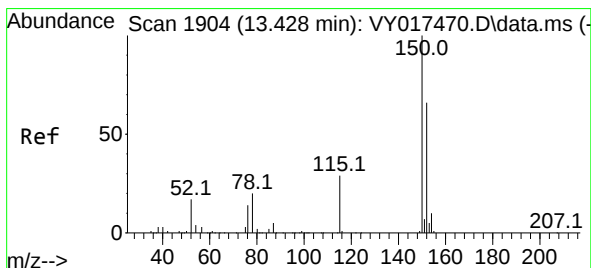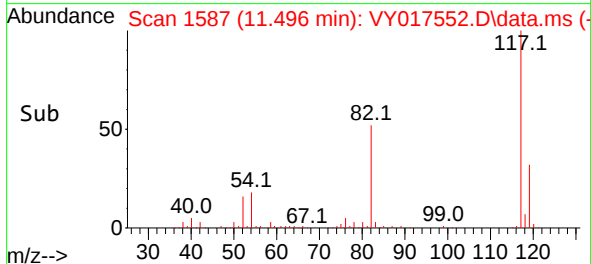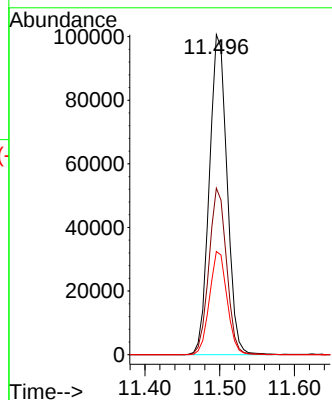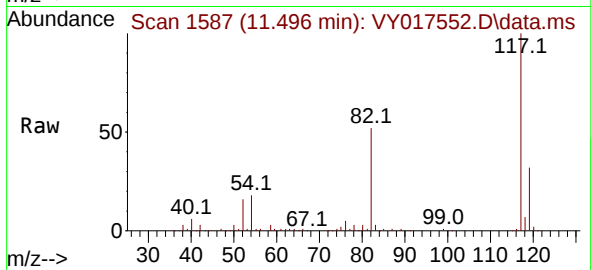

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.434 min Scan# 1905

Delta R.T. 0.006 min

Lab File: VY017552.D

Acq: 01 Mar 2024 15:50

Tgt Ion:152 Resp: 59775

Ion Ratio Lower Upper

152 100

115 54.2 28.2 84.7

150 155.8 0.0 345.6

