


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv030220\
 Data File : VY001808.D
 Acq On : 02 Mar 2020 09:21
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y021720S.M
 Title : SW846 8260
 Last Update : Mon Feb 17 12:19:53 2020

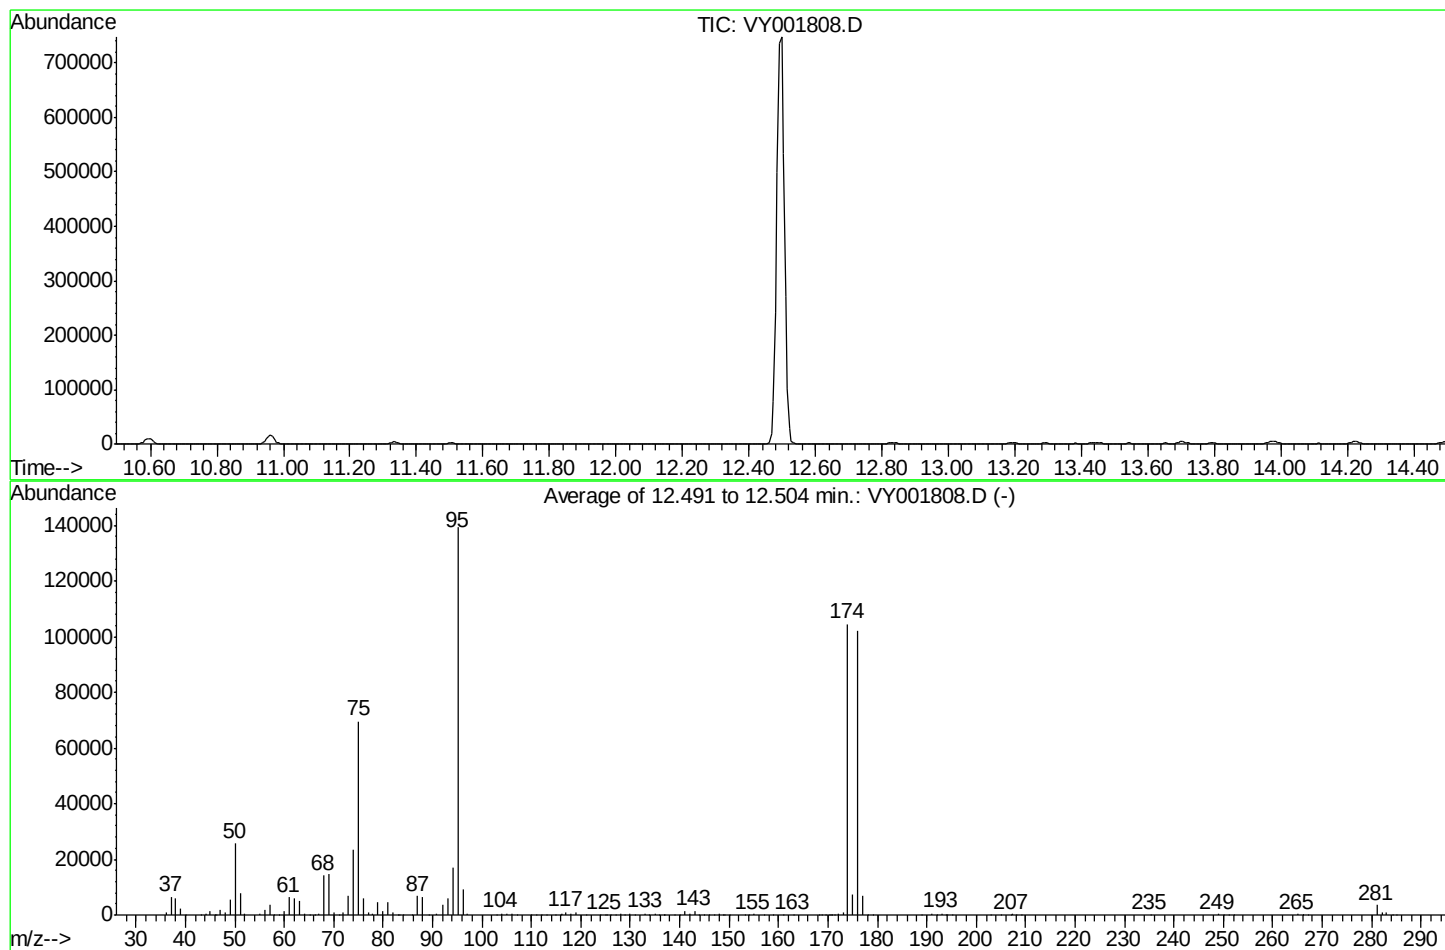

AutoFind: Scans 1764, 1765, 1766; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	25597	PASS
75	95	30	60	50.0	69602	PASS
95	95	100	100	100.0	139256	PASS
96	95	5	9	6.7	9391	PASS
173	174	0.00	2	0.8	828	PASS
174	95	50	100	75.1	104560	PASS
175	174	5	9	7.2	7506	PASS
176	174	95	101	97.6	102037	PASS
177	176	5	9	6.6	6748	PASS