

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030223\
 Data File : VY012770.D
 Acq On : 02 Mar 2023 19:39
 Operator : KP/MD
 Sample : 01739-04
 Misc : 9.06g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TOTAL-VOC-1-GRAB-7

Quant Time: Mar 03 01:59:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 03 01:13:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	129453	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	216307	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	169514	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	64197	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	76119	59.223	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.440%
35) Dibromofluoromethane	7.716	113	75258	57.651	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	115.300%
50) Toluene-d8	10.179	98	230916	48.387	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.780%
62) 4-Bromofluorobenzene	12.483	95	69590	43.203	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	86.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030223\
Data File : VY012770.D
Acq On : 02 Mar 2023 19:39
Operator : KP/MD
Sample : 01739-04
Misc : 9.06g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TOTAL-VOC-1-GRAB-7

Quant Time: Mar 03 01:59:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 03 01:13:13 2023
Response via : Initial Calibration




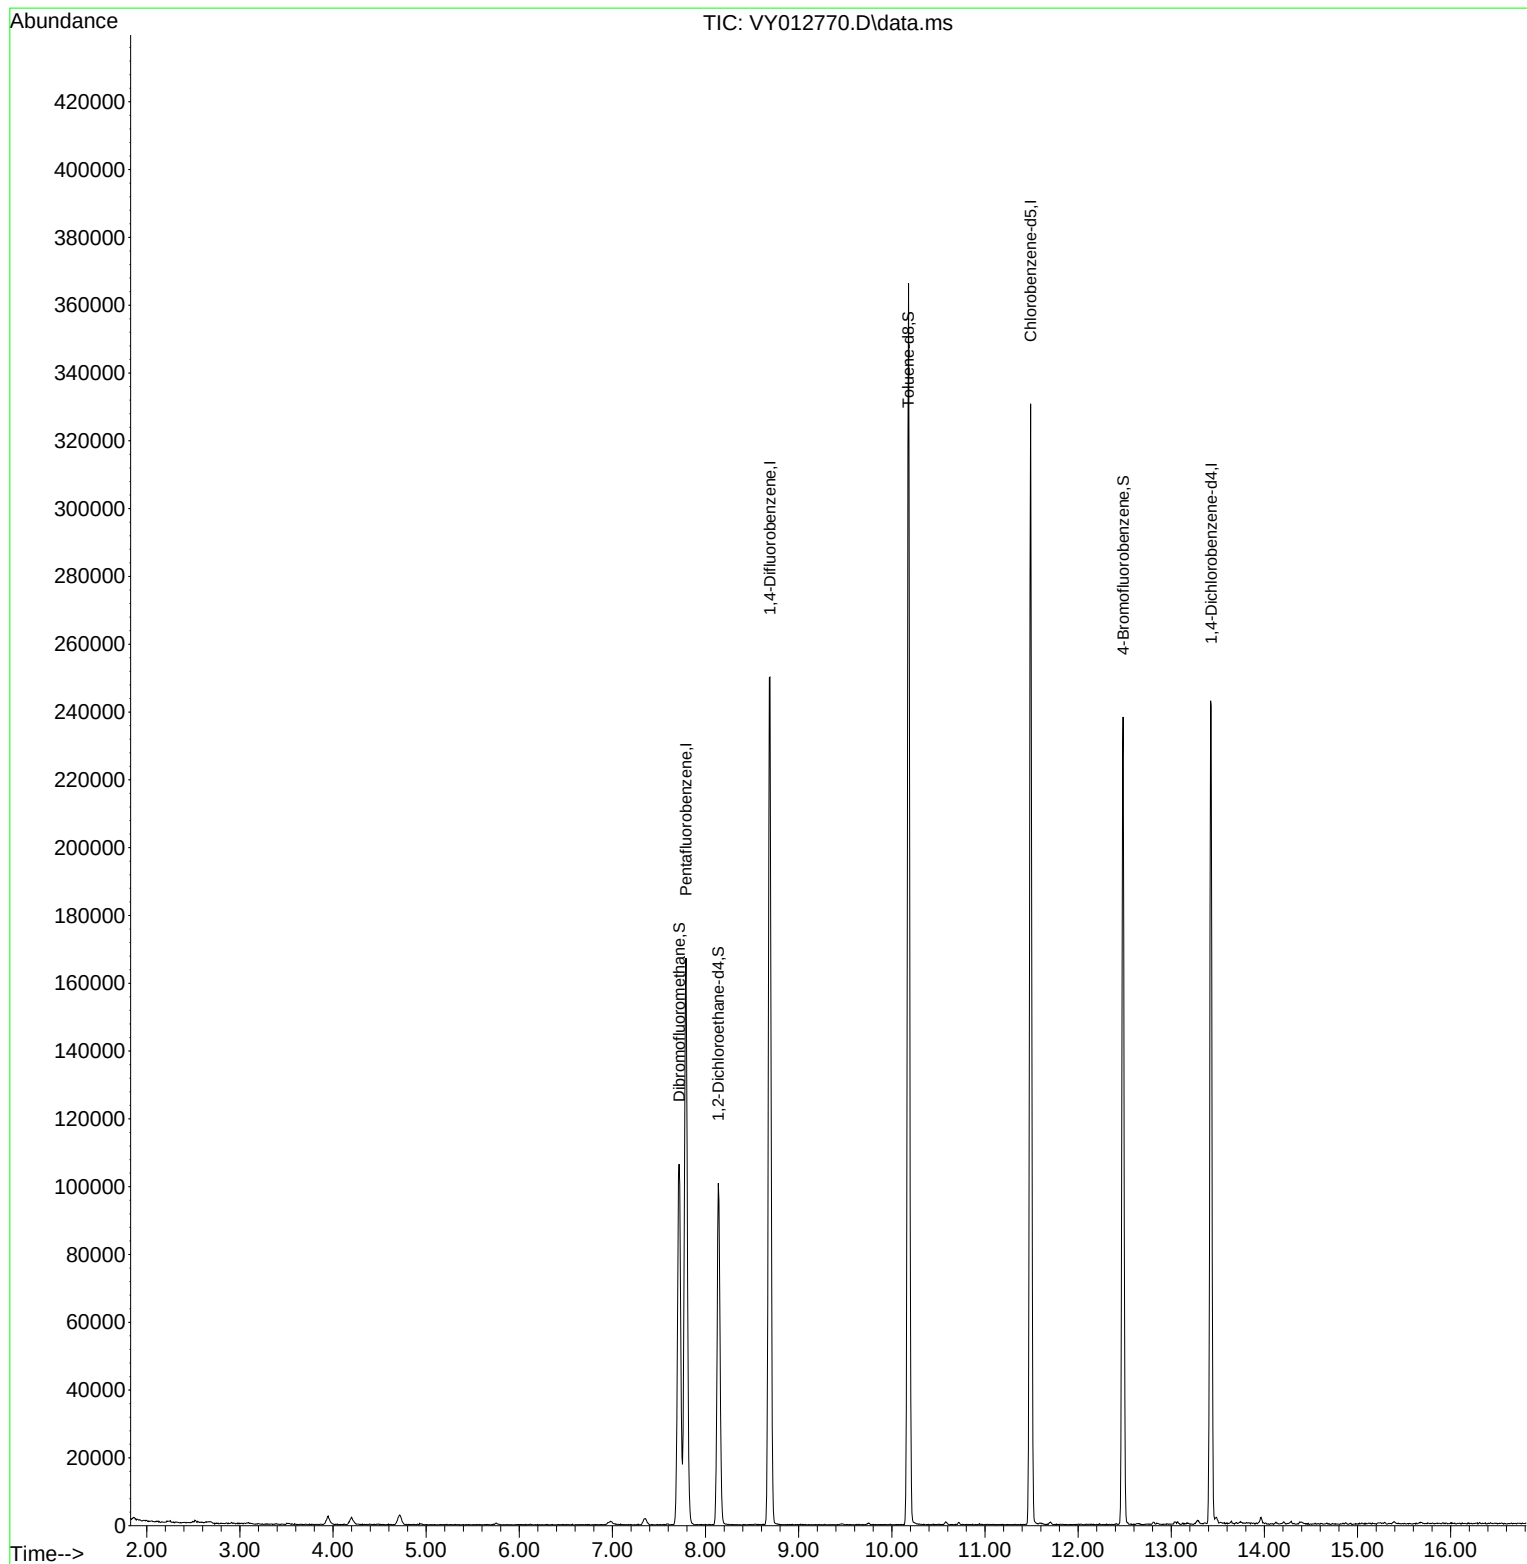


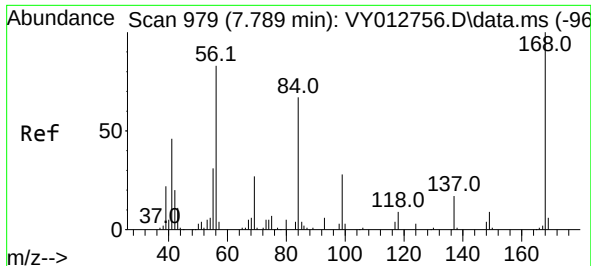

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY012770.D
Acq: 02 Mar 2023 19:39




Instrument :
MSVOA_Y
ClientSampleId :
TOTAL-VOC-1-GRAB-7


Tgt Ion:168 Resp: 129453
Ion Ratio Lower Upper
168 100
99 54.5 41.7 62.5

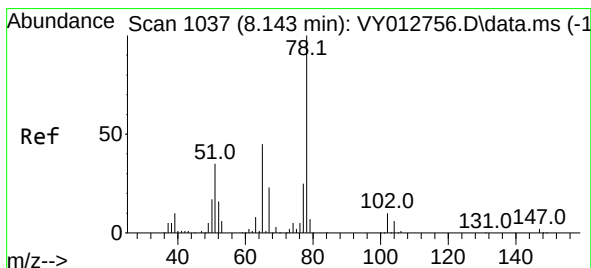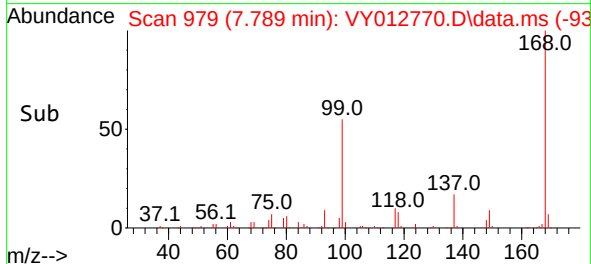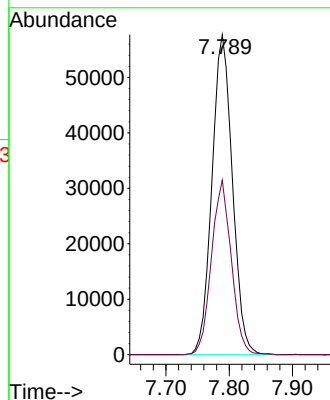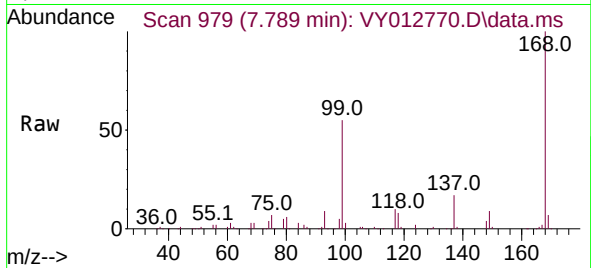

#33
1,2-Dichloroethane-d4
Concen: 59.223 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY012770.D
Acq: 02 Mar 2023 19:39

Tgt Ion: 65 Resp: 76119
Ion Ratio Lower Upper
65 100
67 52.5 0.0 104.0

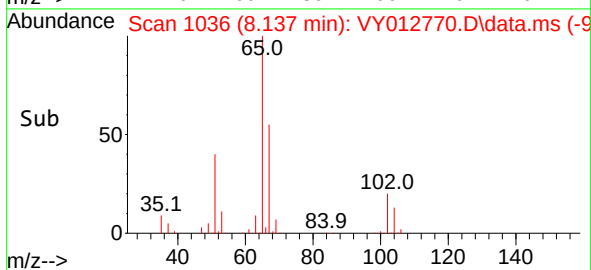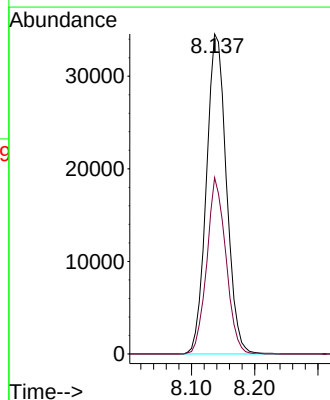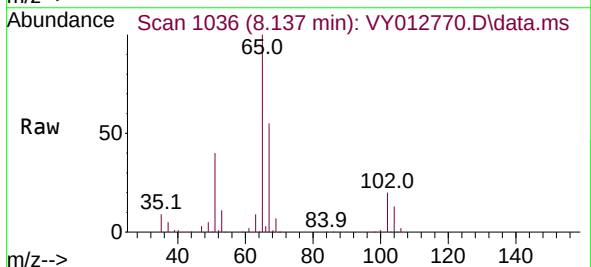

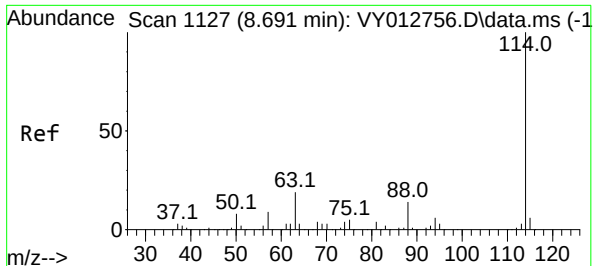

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012770.D

Acq: 02 Mar 2023 19:39

Instrument :

MSVOA_Y

ClientSampleId :

TOTAL-VOC-1-GRAB-7





Tgt Ion:114 Resp: 216307

Ion Ratio Lower Upper

114 100

63 20.1 0.0 37.4

88 15.2 0.0 28.6

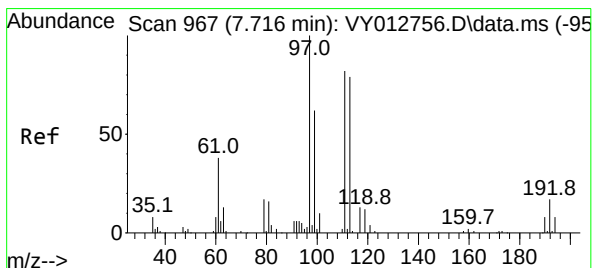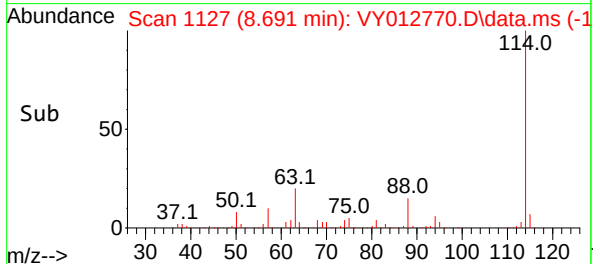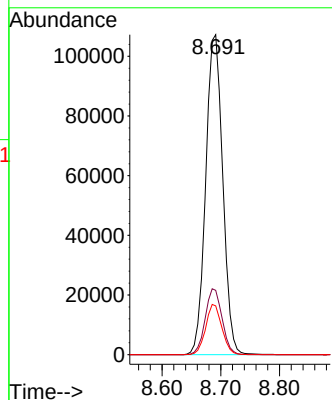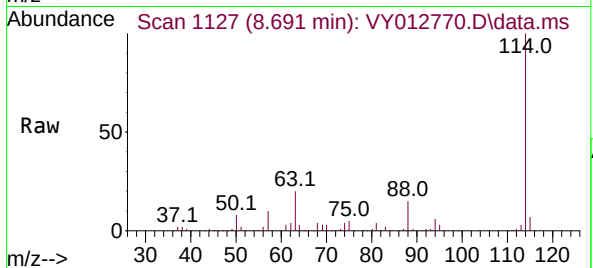

#35

Dibromofluoromethane

Concen: 57.651 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY012770.D

Acq: 02 Mar 2023 19:39




Tgt Ion:113 Resp: 75258


Ion Ratio Lower Upper

113 100

111 103.2 82.2 123.2

192 20.8 16.8 25.2


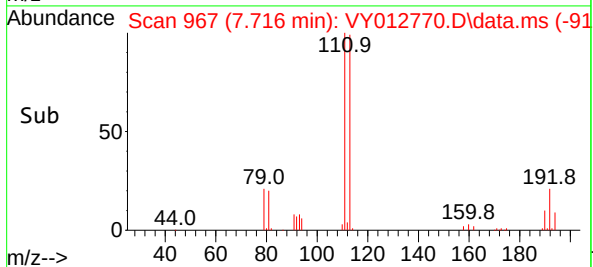
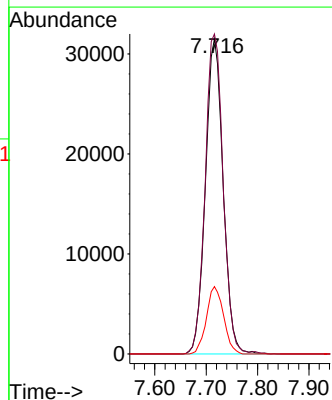
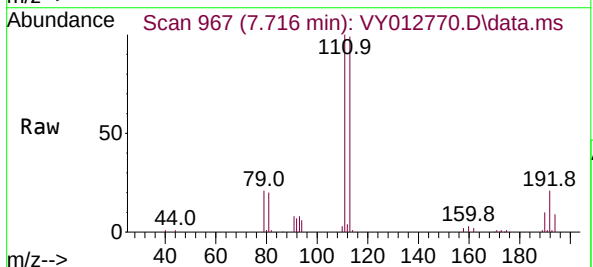


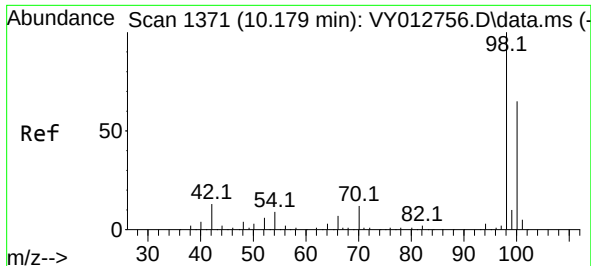

#50
Toluene-d8
Concen: 48.387 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY012770.D
Acq: 02 Mar 2023 19:39




Instrument :
MSVOA_Y
ClientSampleId :
TOTAL-VOC-1-GRAB-7


Tgt Ion: 98 Resp: 230916
Ion Ratio Lower Upper
98 100
100 64.3 50.9 76.3

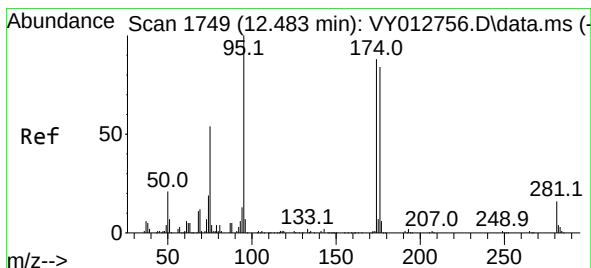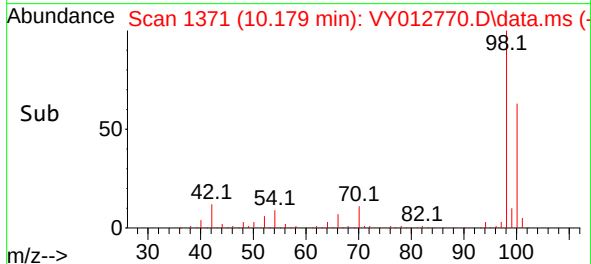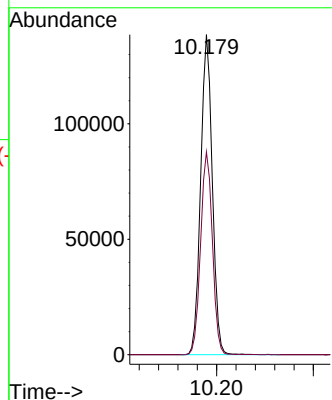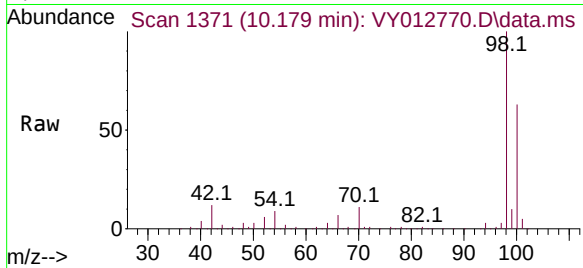

#62
4-Bromofluorobenzene
Concen: 43.203 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012770.D
Acq: 02 Mar 2023 19:39

Tgt Ion: 95 Resp: 69590
Ion Ratio Lower Upper
95 100
174 89.6 0.0 176.6
176 86.3 0.0 170.2


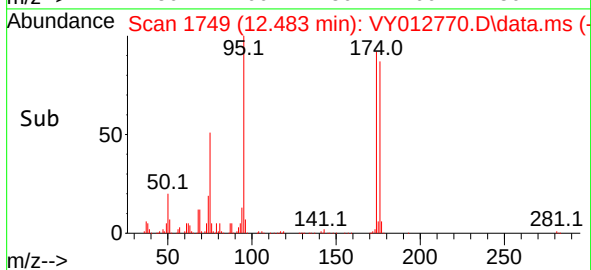
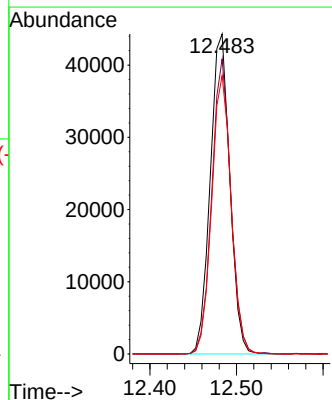
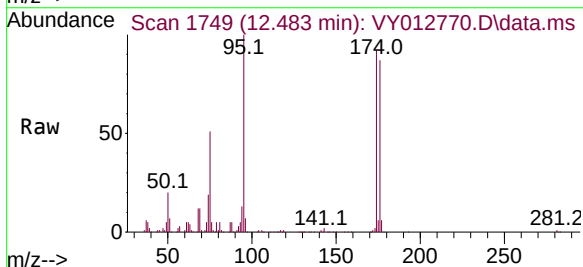


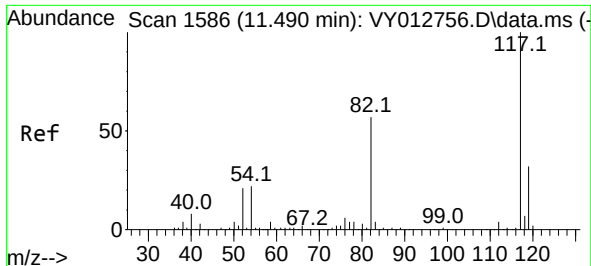

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY012770.D
Acq: 02 Mar 2023 19:39

Instrument :
MSVOA_Y
ClientSampleId :
TOTAL-VOC-1-GRAB-7

Tgt Ion:117 Resp: 169514
Ion Ratio Lower Upper
117 100
82 52.5 45.4 68.0
119 31.8 25.6 38.4

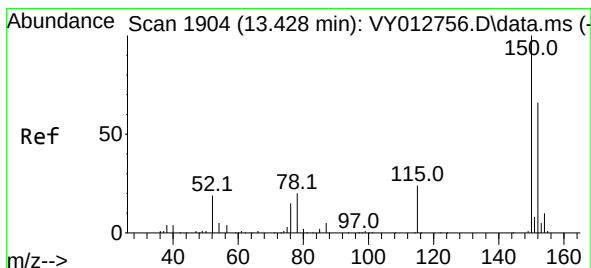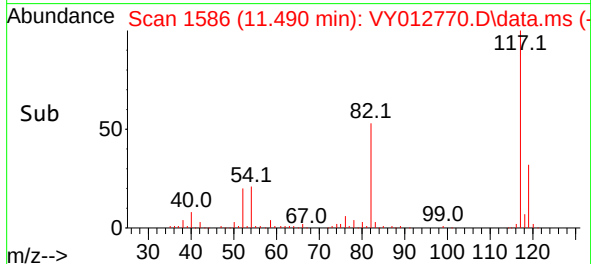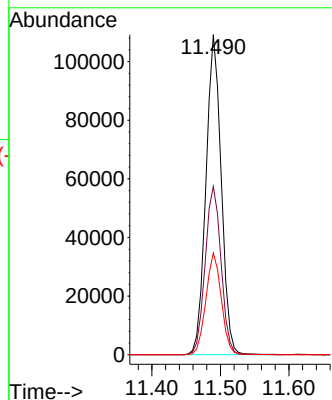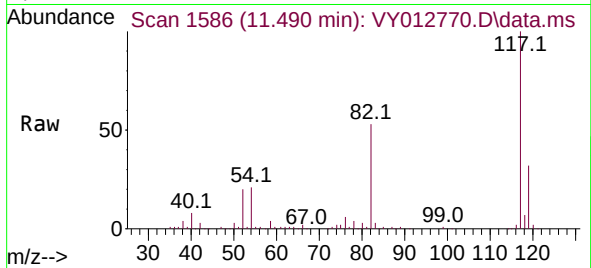

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY012770.D
Acq: 02 Mar 2023 19:39

Tgt Ion:152 Resp: 64197
Ion Ratio Lower Upper
152 100
115 55.2 27.1 81.3
150 155.6 0.0 347.8

