


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030223\
Data File : VY012761.D
Acq On : 02 Mar 2023 15:33
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
Title : SW846 8260
Last Update : Fri Mar 03 01:13:13 2023

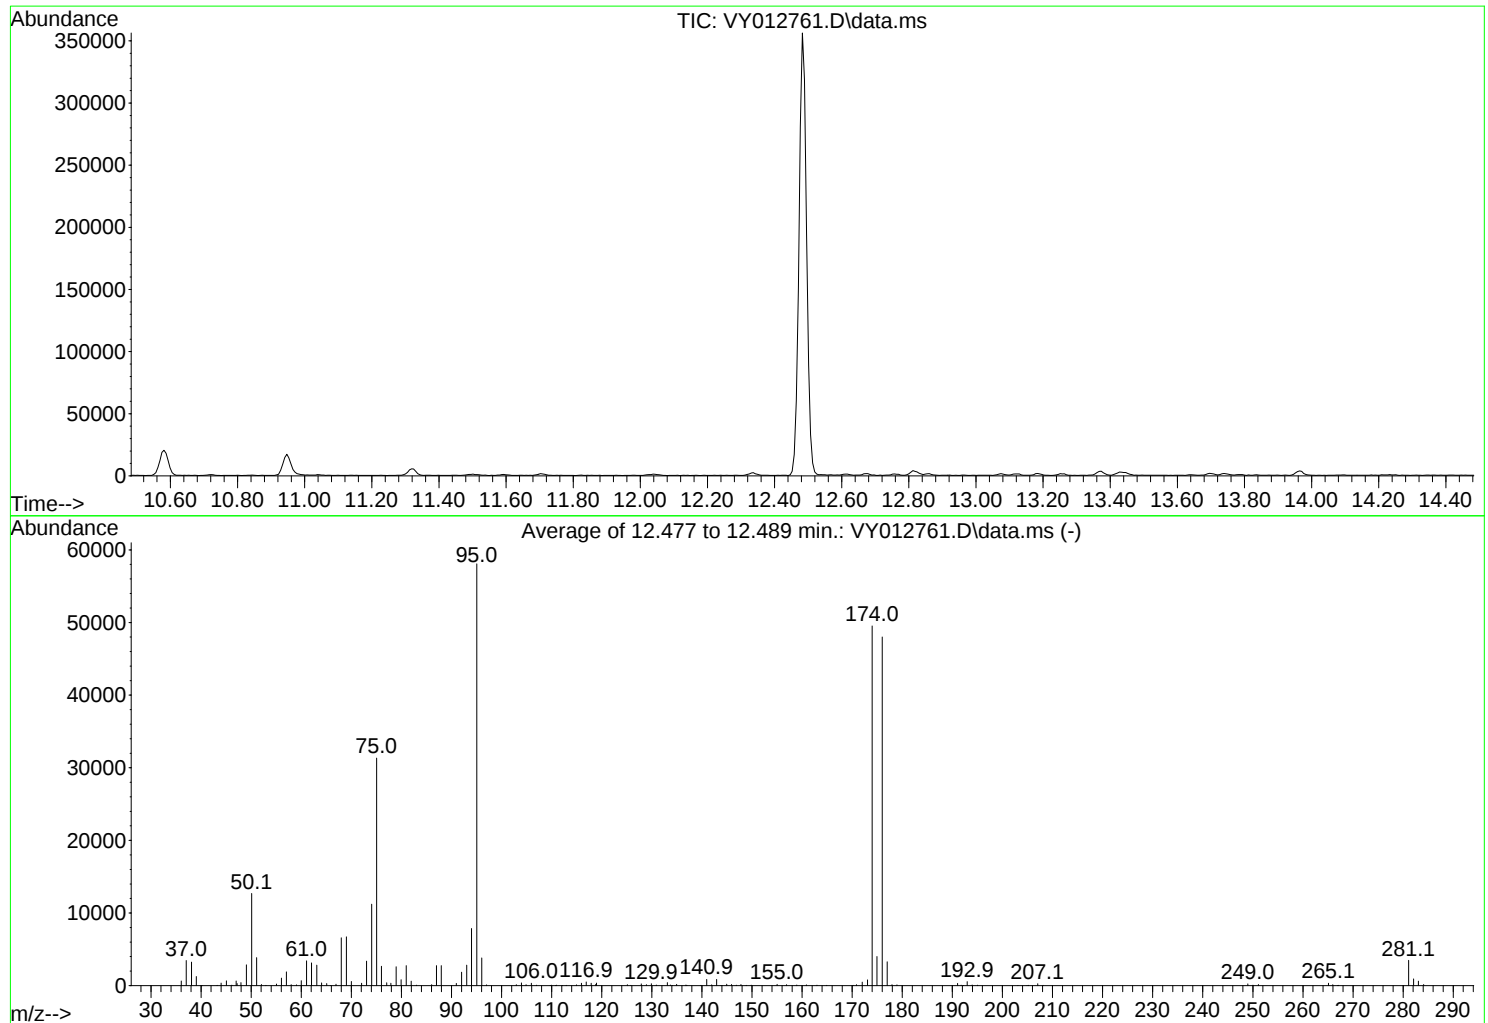

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	12696	PASS
75	95	30	60	53.9	31328	PASS
95	95	100	100	100.0	58080	PASS
96	95	5	9	6.6	3823	PASS
173	174	0.00	2	1.6	784	PASS
174	95	50	100	85.3	49539	PASS
175	174	5	9	8.1	4005	PASS
176	174	95	101	96.9	48003	PASS
177	176	5	9	6.8	3280	PASS