


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv030320\
 Data File : VY001824.D
 Acq On : 03 Mar 2020 09:28
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y021720S.M
 Title : SW846 8260
 Last Update : Wed Mar 04 04:35:40 2020

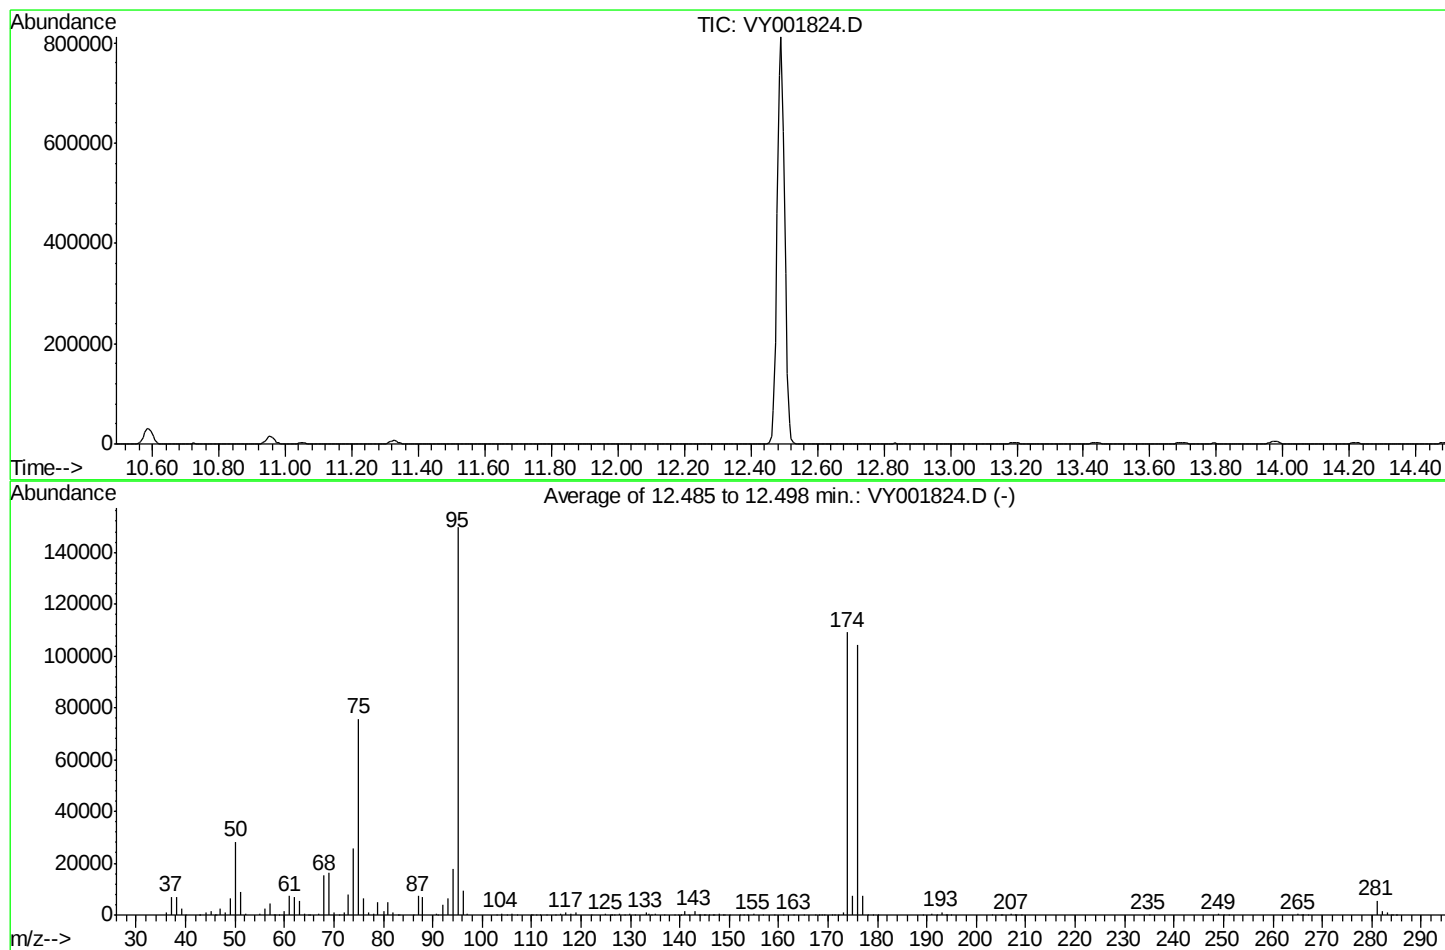

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	28320	PASS
75	95	30	60	50.6	75744	PASS
95	95	100	100	100.0	149680	PASS
96	95	5	9	6.4	9589	PASS
173	174	0.00	2	0.9	946	PASS
174	95	50	100	72.9	109098	PASS
175	174	5	9	7.0	7664	PASS
176	174	95	101	95.5	104218	PASS
177	176	5	9	6.9	7191	PASS