
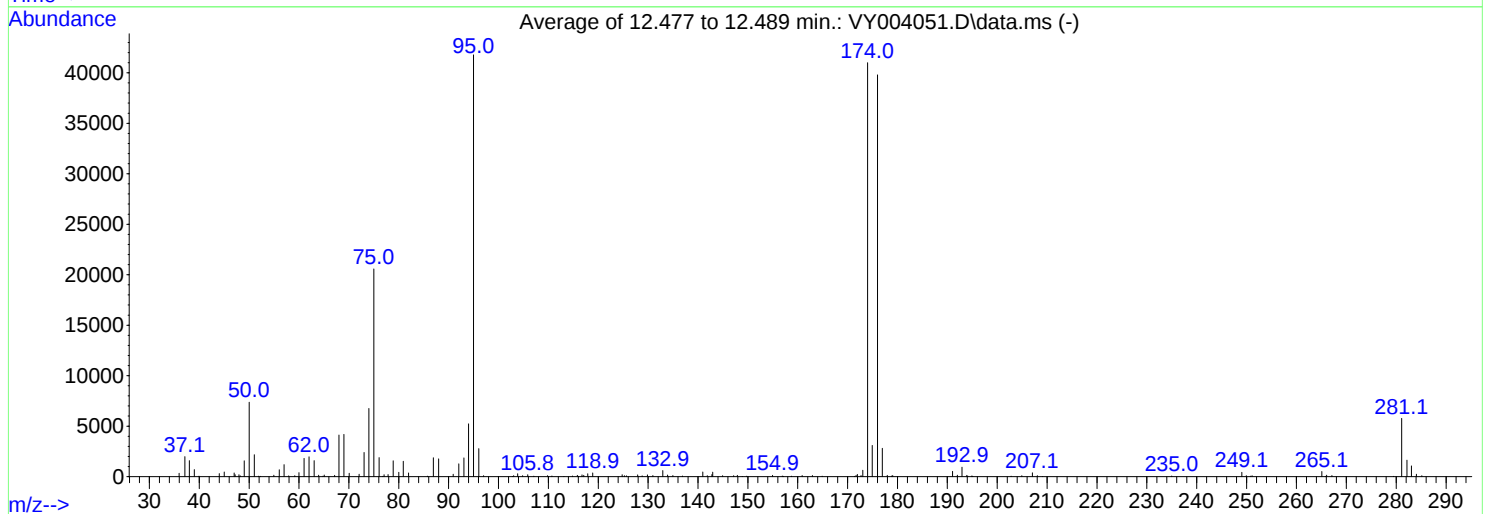


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030321\
Data File : VY004051.D
Acq On : 03 Mar 2021 10:24
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030321S.M
Title : SW846 8260
Last Update : Wed Mar 03 13:49:02 2021

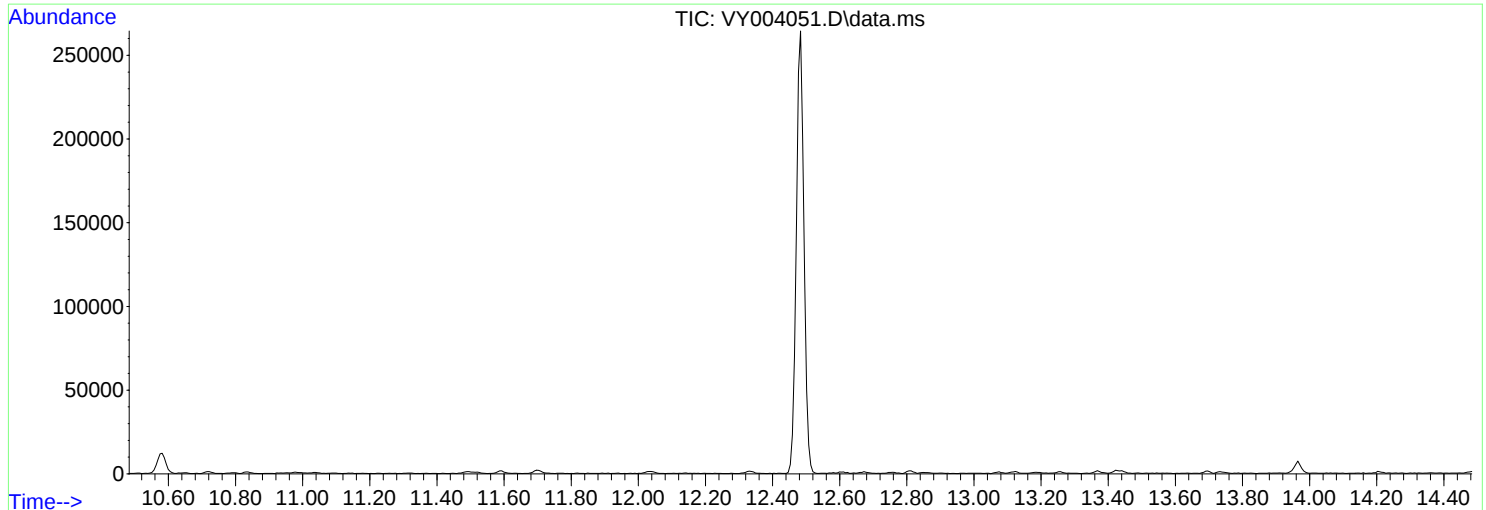

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	7377	PASS
75	95	30	60	49.2	20571	PASS
95	95	100	100	100.0	41781	PASS
96	95	5	9	6.7	2780	PASS
173	174	0.00	2	1.6	642	PASS
174	95	50	100	98.1	40997	PASS
175	174	5	9	7.5	3092	PASS
176	174	95	101	97.1	39795	PASS
177	176	5	9	7.1	2806	PASS