

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030323\
 Data File : VY012797.D
 Acq On : 03 Mar 2023 15:41
 Operator : KP/MD
 Sample : 01749-03
 Misc : 6.70g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CF-5

Quant Time: Mar 04 01:24:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 03 01:13:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	40547	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	59645	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	47361	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	15406	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	24997	62.092	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 124.180%	
35) Dibromofluoromethane	7.716	113	24173	67.155	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 134.320%	
50) Toluene-d8	10.179	98	75047	57.030	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 114.060%	
62) 4-Bromofluorobenzene	12.483	95	18153	40.871	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 81.740%	
Target Compounds						
					Qvalue	
16) Acetone	3.942	43	184	1.164	ug/l #	44
20) Methylene Chloride	4.710	84	2340	Below Cal		84
31) Cyclohexane	7.789	56	985	1.278	ug/l #	1
36) 1,1-Dichloropropene	7.789	75	3155	5.230	ug/l #	49
38) Carbon Tetrachloride	7.789	117	3876	6.222	ug/l #	16
76) 1,2,3-Trichloropropane	12.483	75	9524	51.769	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.483	75	9524	107.266	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030323\
Data File : VY012797.D
Acq On : 03 Mar 2023 15:41
Operator : KP/MD
Sample : 01749-03
Misc : 6.70g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CF-5

Quant Time: Mar 04 01:24:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 03 01:13:13 2023
Response via : Initial Calibration




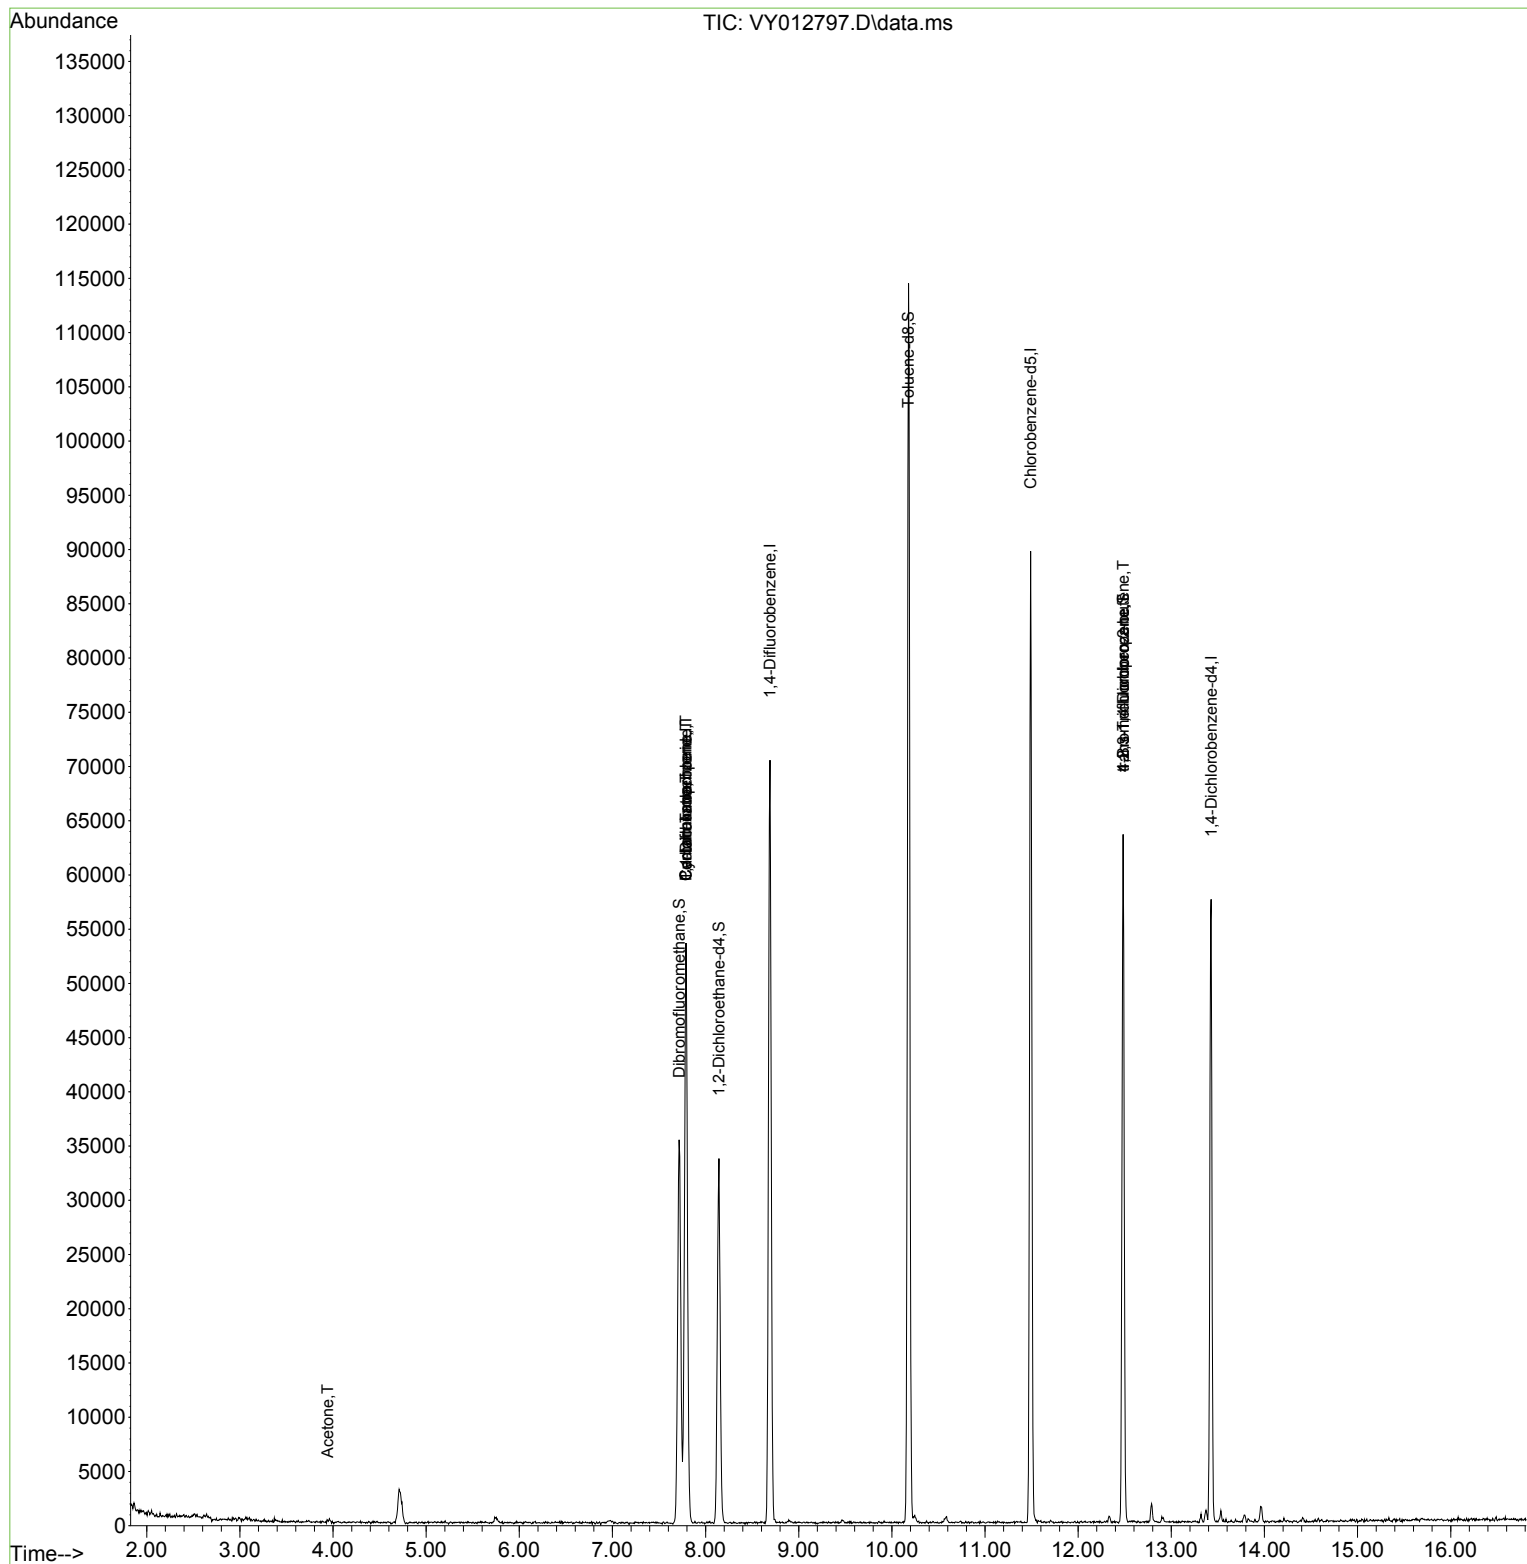


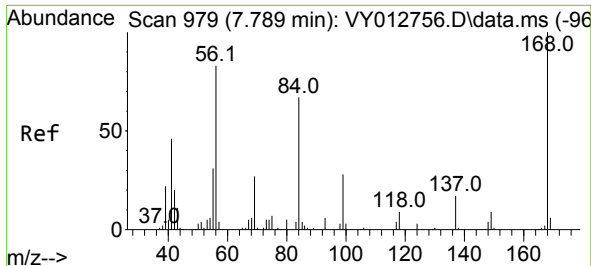

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41




Instrument :
MSVOA_Y
ClientSampleId :
CF-5


Tgt Ion:168 Resp: 40547
Ion Ratio Lower Upper
168 100
99 51.9 41.7 62.5

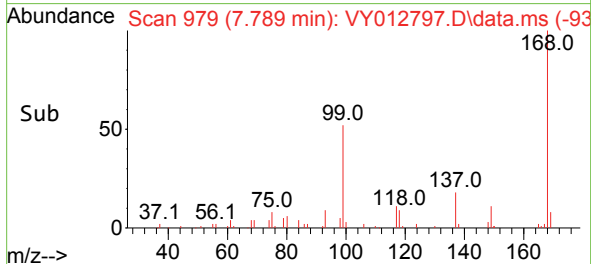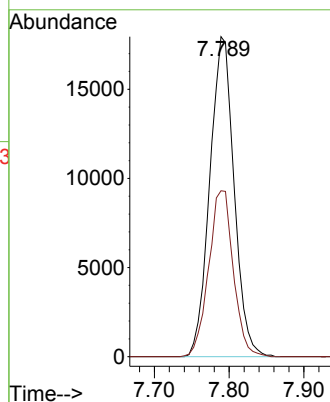

#16
Acetone
Concen: 1.164 ug/l
RT: 3.942 min Scan# 348
Delta R.T. 0.000 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41


Tgt Ion: 43 Resp: 184
Ion Ratio Lower Upper
43 100
58 0.0 24.2 36.2#

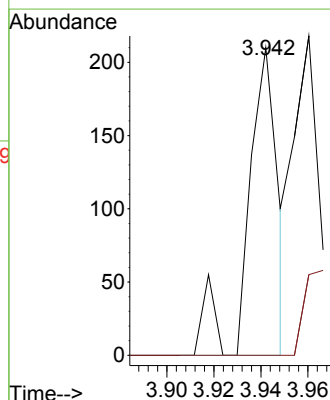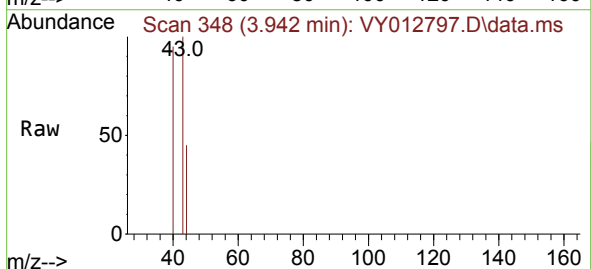



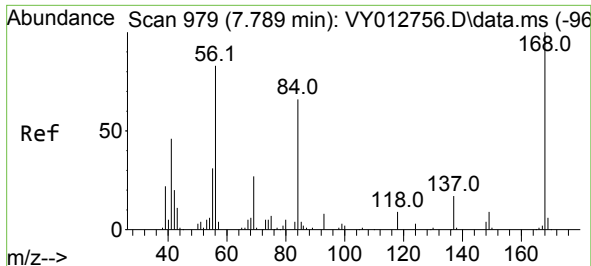


#31
Cyclohexane
Concen: 1.278 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41

Instrument :
MSVOA_Y
ClientSampleId :
CF-5



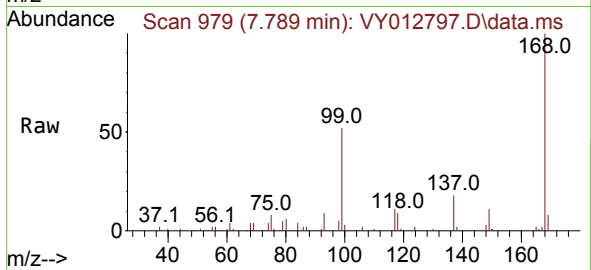



Tgt Ion: 56 Resp: 985
Ion Ratio Lower Upper
56 100
69 140.4 25.7 38.5#
84 148.9 64.3 96.5#

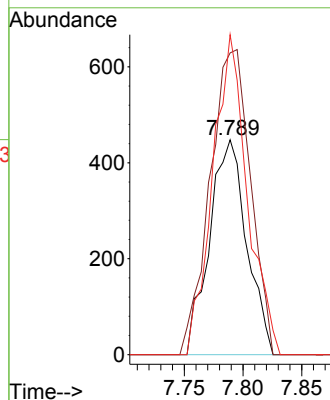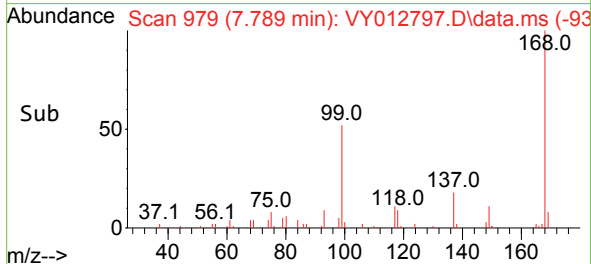

#33
1,2-Dichloroethane-d4
Concen: 62.092 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41

Tgt Ion: 65 Resp: 24997
Ion Ratio Lower Upper
65 100
67 52.3 0.0 104.0

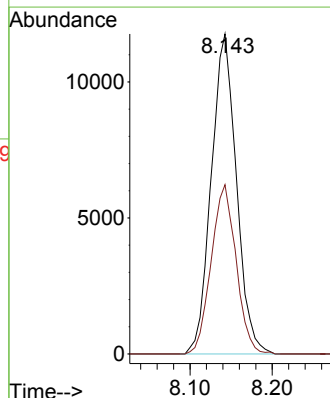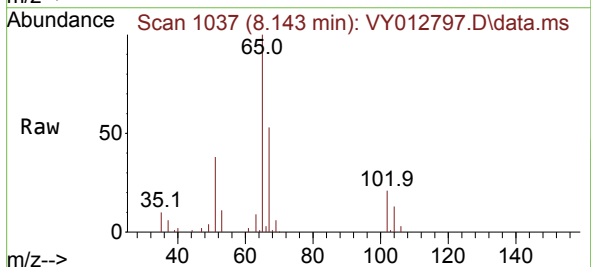

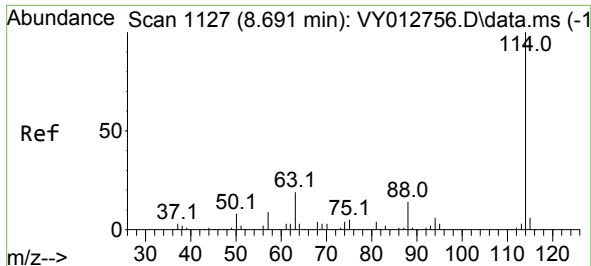

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY012797.D

Acq: 03 Mar 2023 15:41

Instrument :

MSVOA_Y

ClientSampleId :

CF-5





Tgt Ion:114 Resp: 59645

Ion Ratio Lower Upper

114 100

63 19.9 0.0 37.4

88 14.0 0.0 28.6

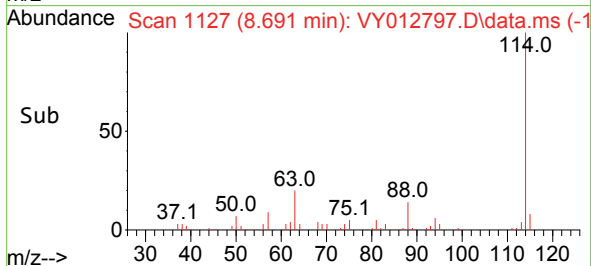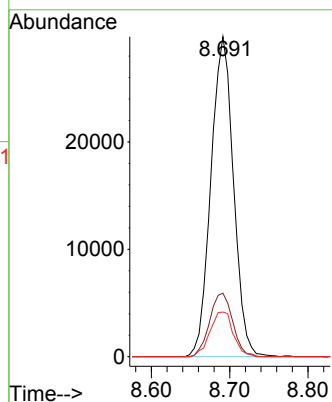

#35

Dibromofluoromethane

Concen: 67.155 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012797.D

Acq: 03 Mar 2023 15:41




Tgt Ion:113 Resp: 24173


Ion Ratio Lower Upper

113 100

111 105.5 82.2 123.2

192 21.8 16.8 25.2


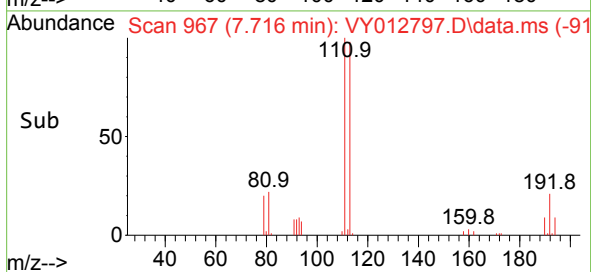
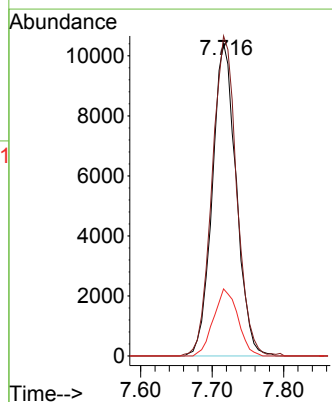
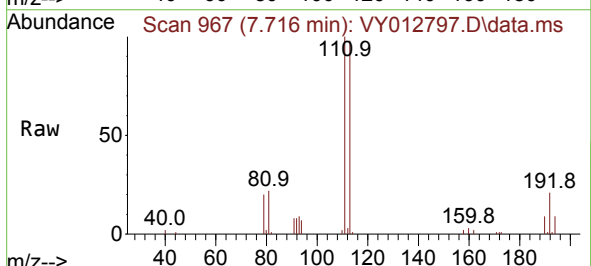


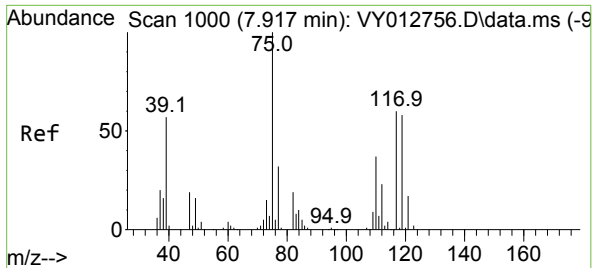

#36
1,1-Dichloropropene
Concen: 5.230 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.128 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41




Instrument :
MSVOA_Y
ClientSampleId :
CF-5


Tgt Ion: 75 Resp: 3155
Ion Ratio Lower Upper
75 100
110 8.4 17.8 53.3#
77 0.0 25.0 37.4#

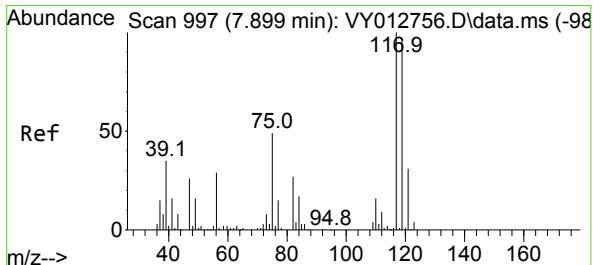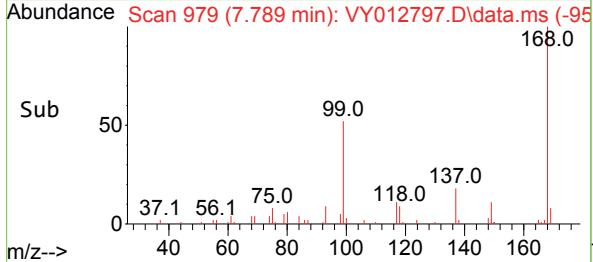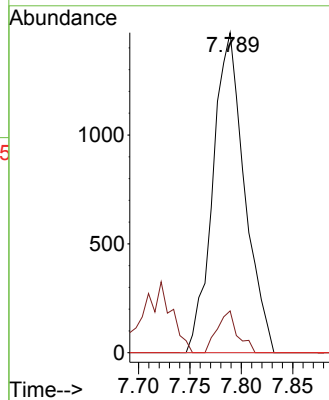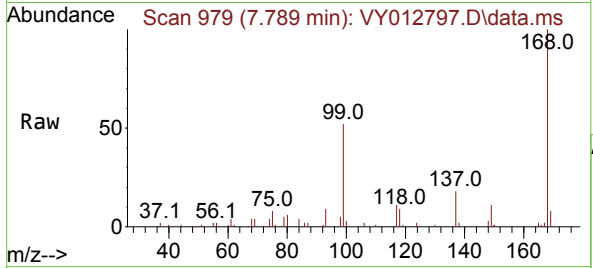

#38
Carbon Tetrachloride
Concen: 6.222 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.110 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41

Tgt Ion: 117 Resp: 3876
Ion Ratio Lower Upper
117 100
119 5.9 77.2 115.8#
121 0.0 24.7 37.1#


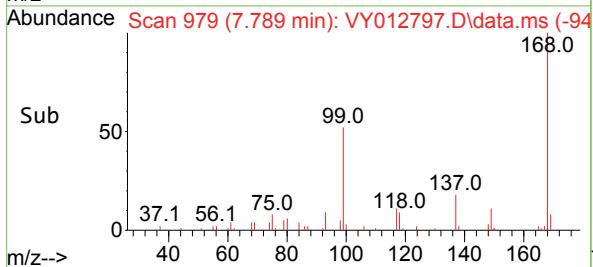
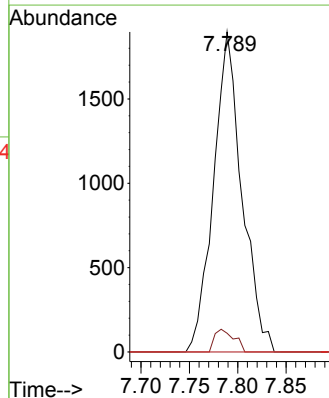
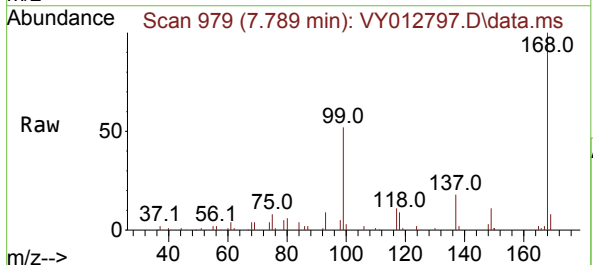




#50
Toluene-d8
Concen: 57.030 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41




Instrument :
MSVOA_Y
ClientSampleId :
CF-5


Tgt Ion: 98 Resp: 75047
Ion Ratio Lower Upper
98 100
100 64.9 50.9 76.3

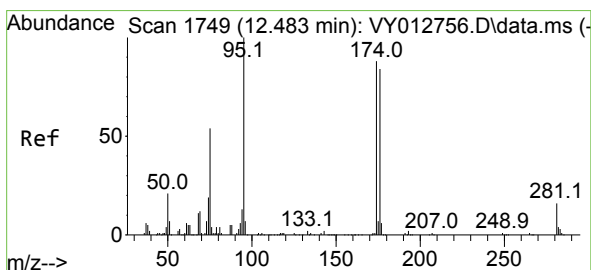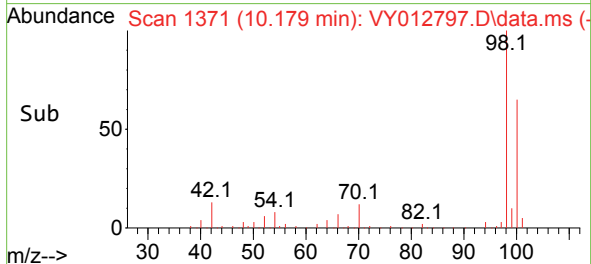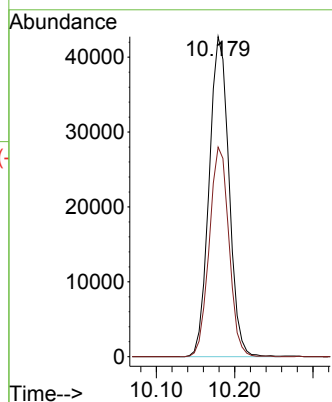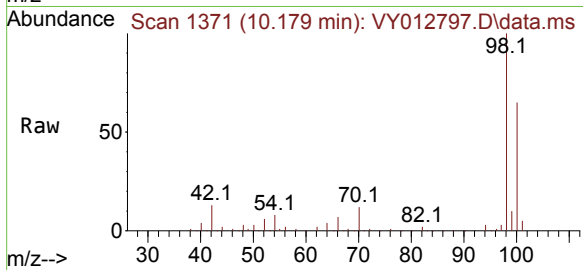

#62
4-Bromofluorobenzene
Concen: 40.871 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41

Tgt Ion: 95 Resp: 18153
Ion Ratio Lower Upper
95 100
174 90.5 0.0 176.6
176 88.1 0.0 170.2


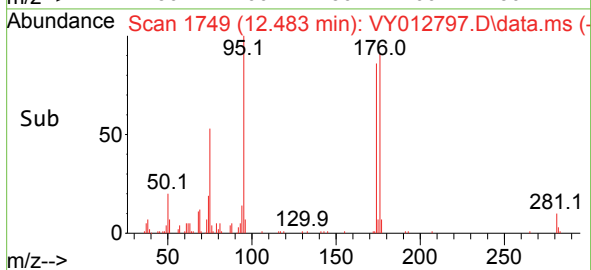
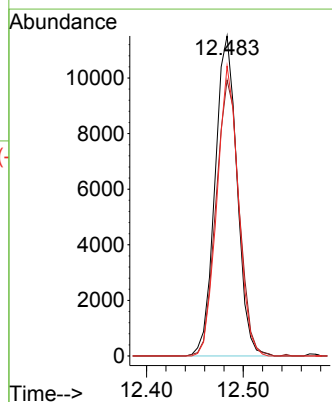
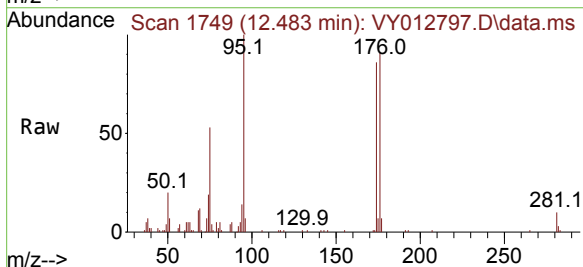


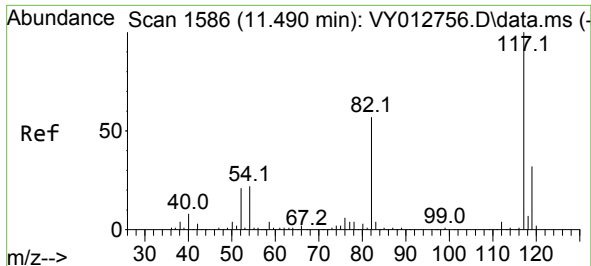

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41




Instrument :
MSVOA_Y
ClientSampleId :
CF-5


Tgt Ion:117 Resp: 47361
Ion Ratio Lower Upper
117 100
82 57.6 45.4 68.0
119 32.4 25.6 38.4

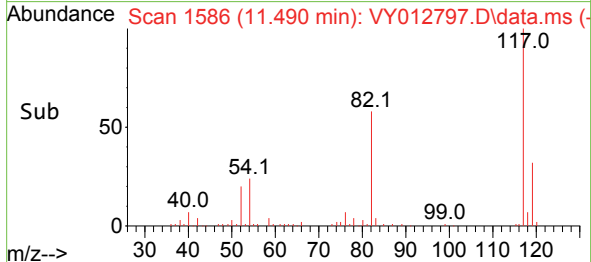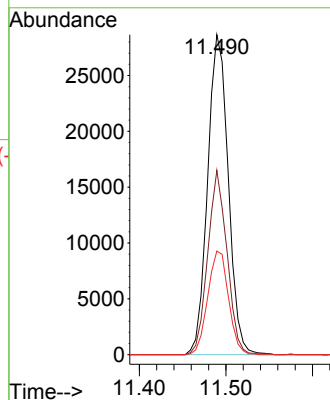

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41

Tgt Ion:152 Resp: 15406
Ion Ratio Lower Upper
152 100
115 55.4 27.1 81.3
150 156.7 0.0 347.8


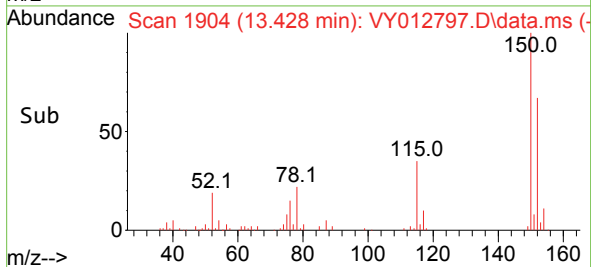
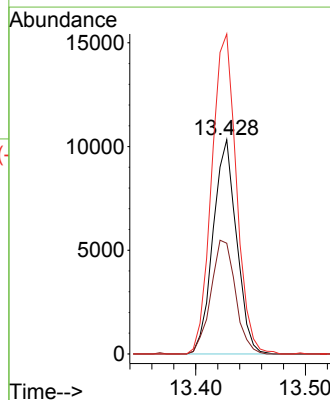
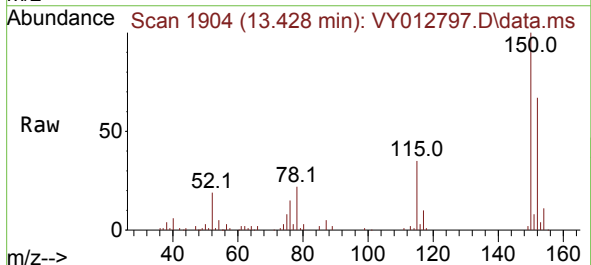


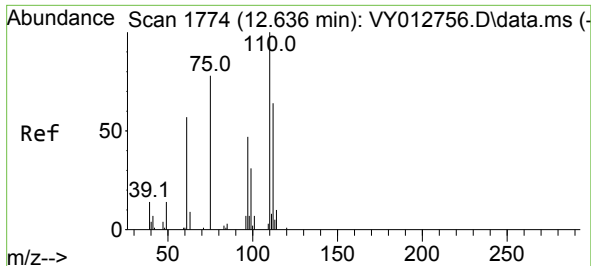

#76
1,2,3-Trichloropropane
Concen: 51.769 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.152 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41

Instrument :
MSVOA_Y
ClientSampleId :
CF-5

Tgt Ion: 75 Resp: 9524
Ion Ratio Lower Upper
75 100
77 0.3 0.0 0.0#

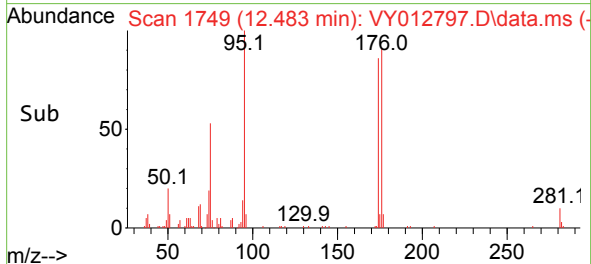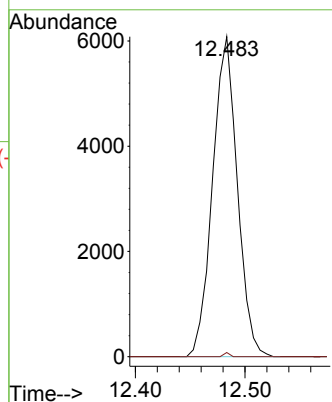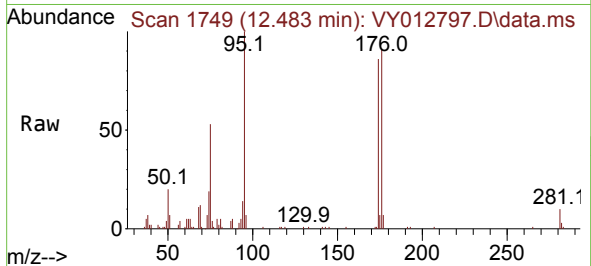

#81
trans-1,4-Dichloro-2-butene
Concen: 107.266 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.104 min
Lab File: VY012797.D
Acq: 03 Mar 2023 15:41

Tgt Ion: 75 Resp: 9524
Ion Ratio Lower Upper
75 100
53 0.0 73.4 110.0#
89 0.0 36.6 55.0#

