

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030323\
 Data File : VY012796.D
 Acq On : 03 Mar 2023 15:18
 Operator : KP/MD
 Sample : 01749-02
 Misc : 6.85g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CF-4

Quant Time: Mar 04 01:24:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 03 01:13:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	102458	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	166029	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	138654	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	51144	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	60514	59.486	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.980%
35) Dibromofluoromethane	7.716	113	61723	61.601	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	123.200%
50) Toluene-d8	10.179	98	204128	55.726	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	111.460%
62) 4-Bromofluorobenzene	12.483	95	55363	44.779	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	89.560%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030323\
Data File : VY012796.D
Acq On : 03 Mar 2023 15:18
Operator : KP/MD
Sample : 01749-02
Misc : 6.85g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CF-4

Quant Time: Mar 04 01:24:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 03 01:13:13 2023
Response via : Initial Calibration




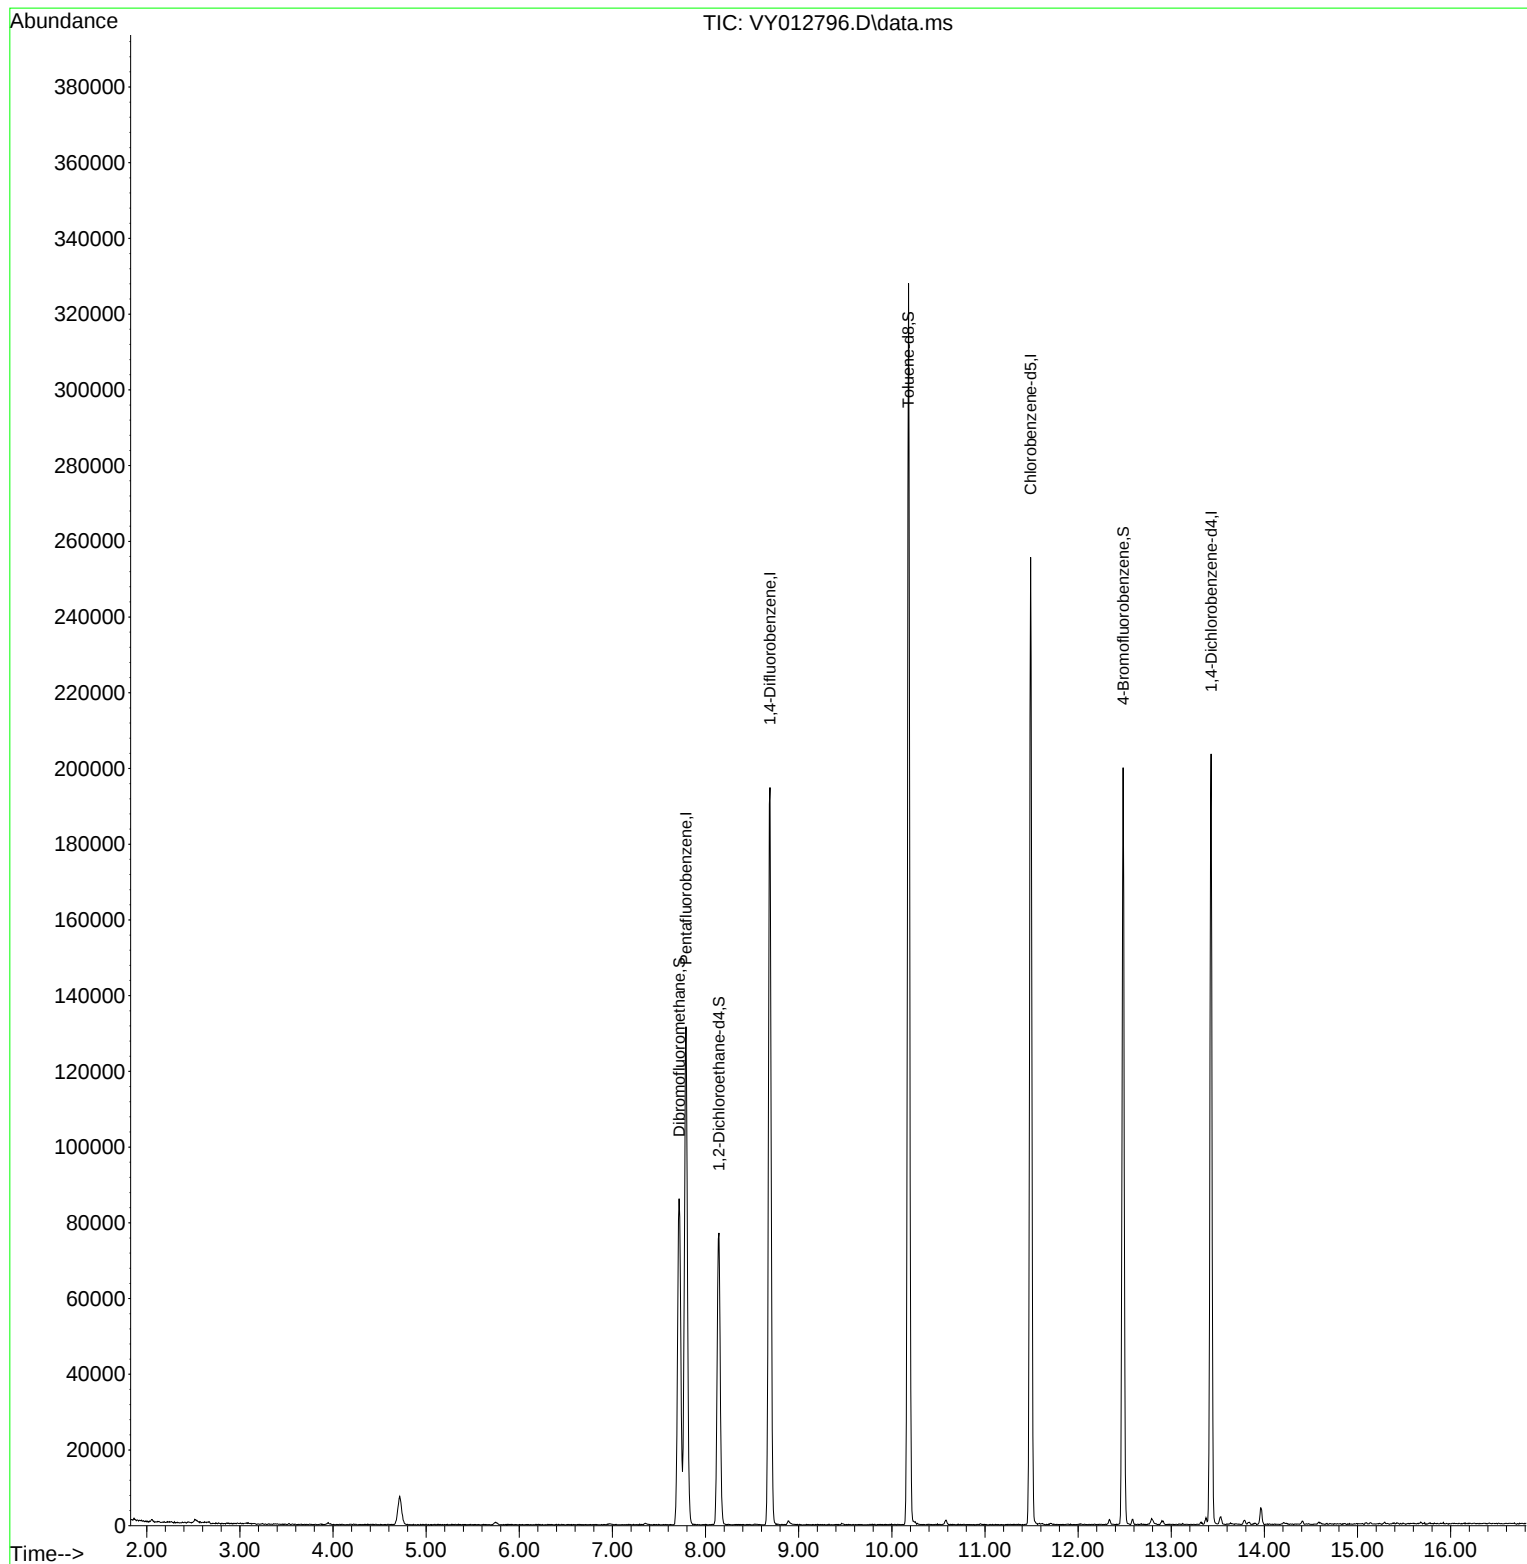


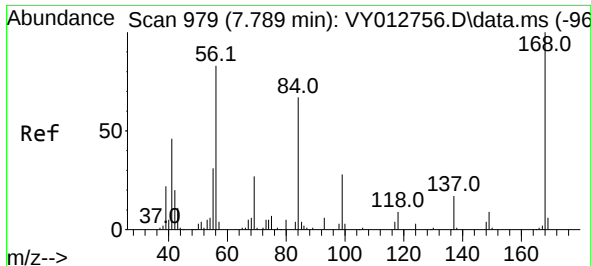

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY012796.D
Acq: 03 Mar 2023 15:18




Instrument :
MSVOA_Y
ClientSampleId :
CF-4


Tgt Ion:168 Resp: 102458
Ion Ratio Lower Upper
168 100
99 51.4 41.7 62.5

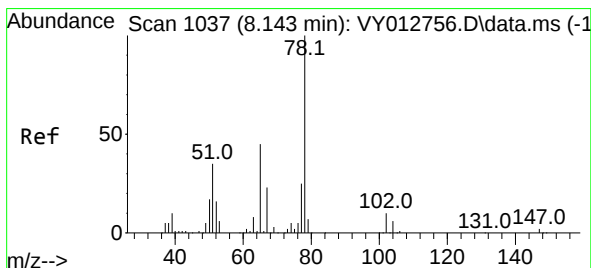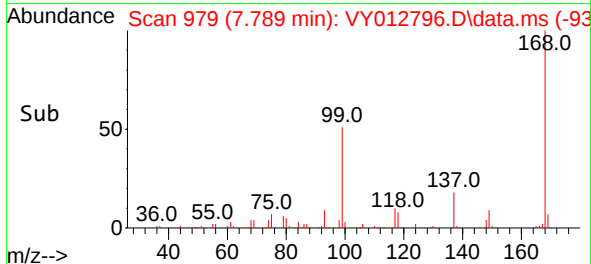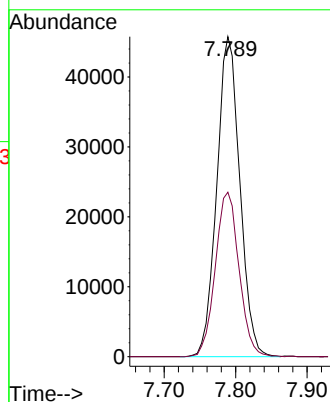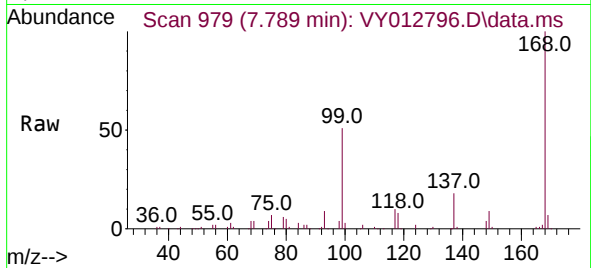

#33
1,2-Dichloroethane-d4
Concen: 59.486 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY012796.D
Acq: 03 Mar 2023 15:18

Tgt Ion: 65 Resp: 60514
Ion Ratio Lower Upper
65 100
67 53.5 0.0 104.0

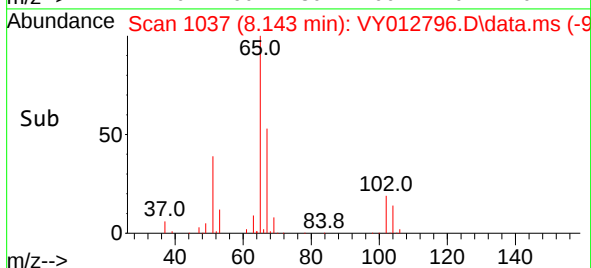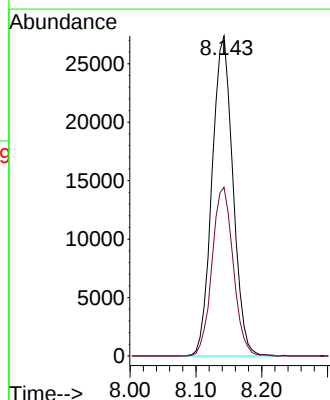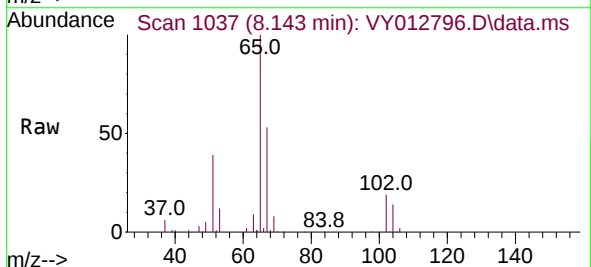

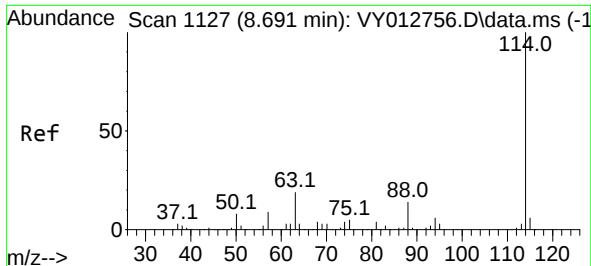

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012796.D

Acq: 03 Mar 2023 15:18

Instrument :

MSVOA_Y

ClientSampleId :

CF-4





Tgt Ion:114 Resp: 166029

Ion Ratio Lower Upper

114 100

63 20.2 0.0 37.4

88 14.5 0.0 28.6

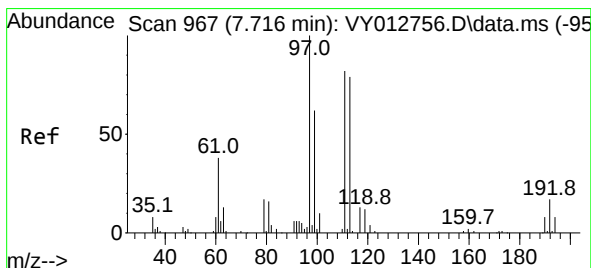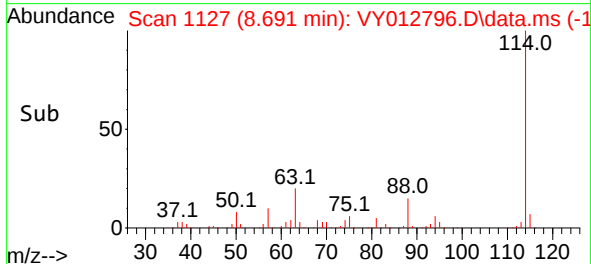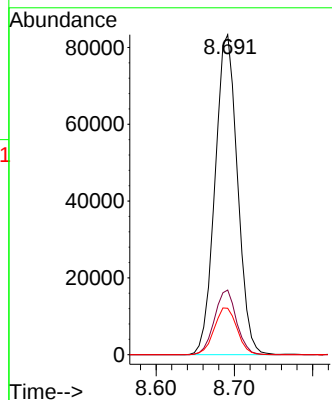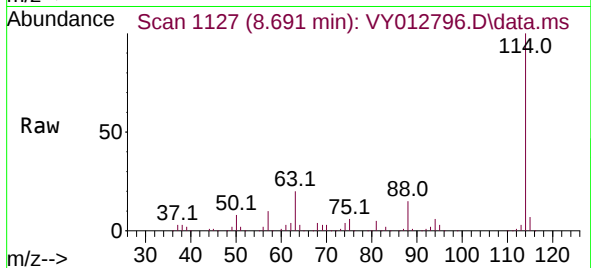

#35

Dibromofluoromethane

Concen: 61.601 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY012796.D

Acq: 03 Mar 2023 15:18




Tgt Ion:113 Resp: 61723


Ion Ratio Lower Upper

113 100

111 102.2 82.2 123.2

192 20.2 16.8 25.2


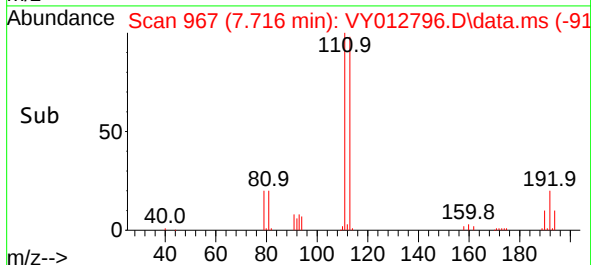
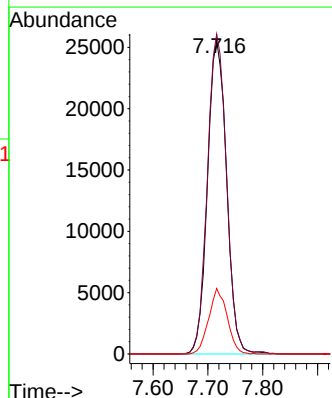
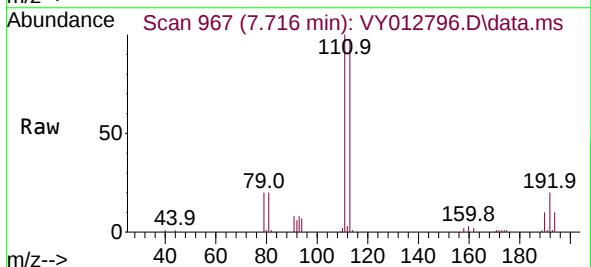


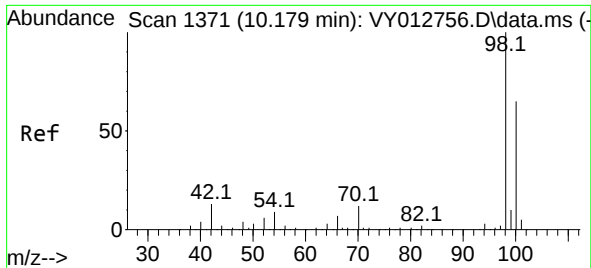

#50
Toluene-d8
Concen: 55.726 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.000 min
Lab File: VY012796.D
Acq: 03 Mar 2023 15:18




Instrument :
MSVOA_Y
ClientSampleId :
CF-4


Tgt Ion: 98 Resp: 204128
Ion Ratio Lower Upper
98 100
100 64.0 50.9 76.3

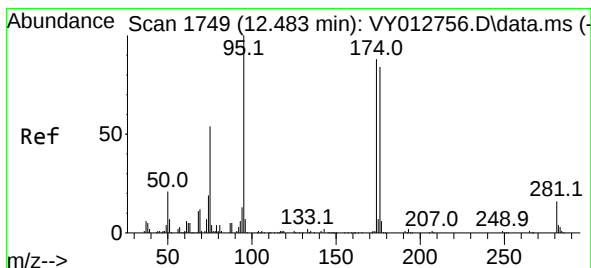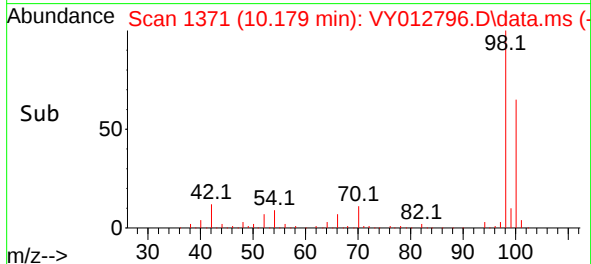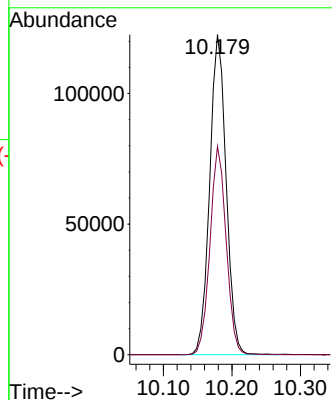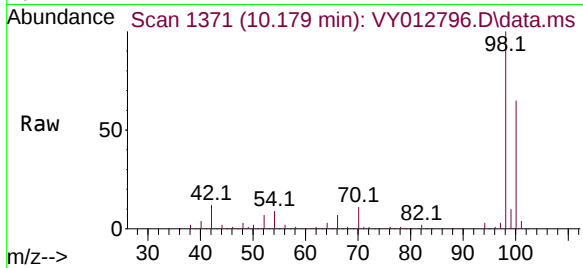

#62
4-Bromofluorobenzene
Concen: 44.779 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012796.D
Acq: 03 Mar 2023 15:18

Tgt Ion: 95 Resp: 55363
Ion Ratio Lower Upper
95 100
174 91.1 0.0 176.6
176 88.1 0.0 170.2


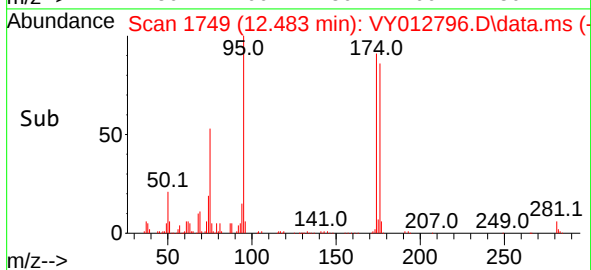
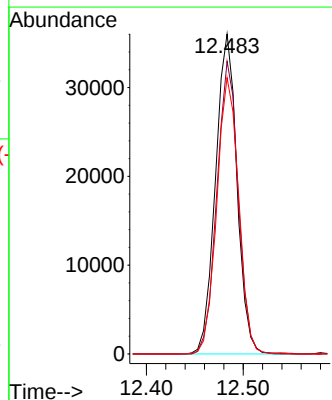
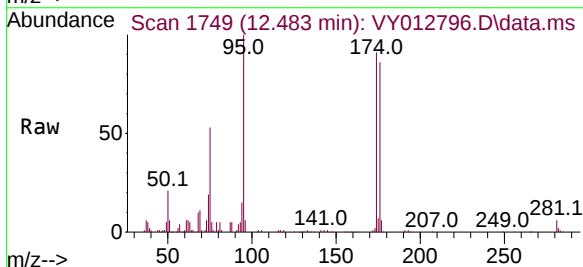


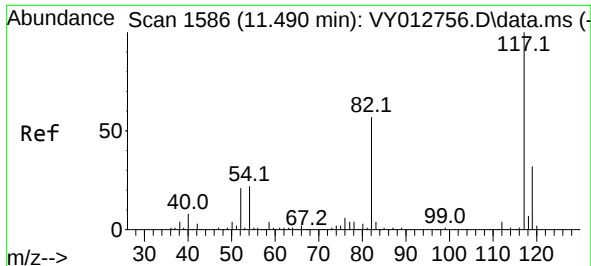

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY012796.D
Acq: 03 Mar 2023 15:18

Instrument :
MSVOA_Y
ClientSampleId :
CF-4

Tgt Ion:117 Resp: 138654
Ion Ratio Lower Upper
117 100
82 54.4 45.4 68.0
119 32.0 25.6 38.4

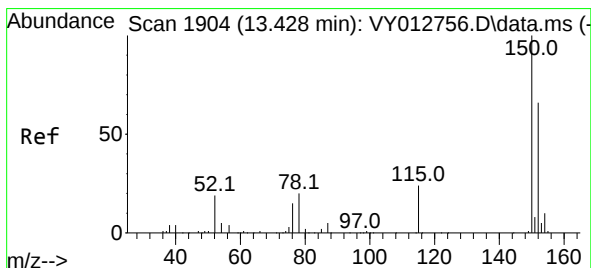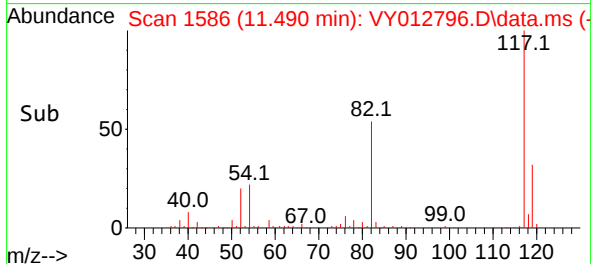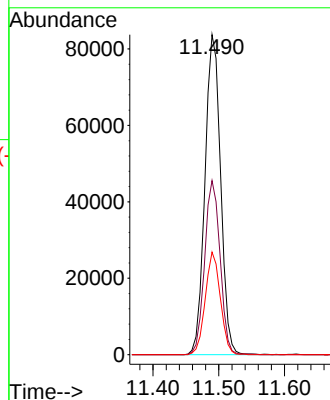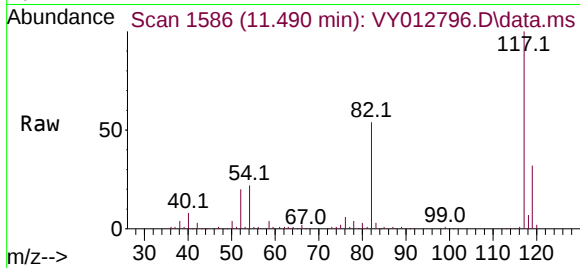

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY012796.D
Acq: 03 Mar 2023 15:18

Tgt Ion:152 Resp: 51144
Ion Ratio Lower Upper
152 100
115 57.2 27.1 81.3
150 159.2 0.0 347.8

